

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037356.D
 Acq On : 03 Nov 2022 20:51
 Operator : CG/JU
 Sample : N5276-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037356.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rBV	83282	100246	0.84%	0.095%
2	3.699	102	104	118	rBV	280889	437662	3.66%	0.415%
3	3.916	137	141	147	rVB	30386	47779	0.40%	0.045%
4	4.016	154	158	165	rVB	31132	45337	0.38%	0.043%
5	4.963	315	319	327	rVB	26623	40928	0.34%	0.039%
6	7.022	663	669	685	rVB	397354	674506	5.65%	0.639%
7	7.187	689	697	709	rBV	1528951	2394978	20.05%	2.271%
8	7.381	723	730	741	rBV	1422326	2256422	18.89%	2.139%
9	7.851	800	810	819	rBV	1479371	2347954	19.66%	2.226%
10	8.569	923	932	949	rBV	1168496	1935874	16.21%	1.835%
11	9.022	1000	1009	1019	rBV	1769018	2922180	24.46%	2.770%
12	9.404	1069	1074	1079	rVB2	14053	23258	0.19%	0.022%
13	9.739	1124	1131	1144	rBV	1391725	2220427	18.59%	2.105%
14	10.275	1213	1222	1243	rBV	1975114	3347656	28.03%	3.174%
15	10.439	1243	1250	1264	rVV	128514	295788	2.48%	0.280%
16	10.651	1278	1286	1297	rBV	2223141	3603268	30.16%	3.416%
17	10.798	1304	1311	1329	rBV	1559690	2683865	22.47%	2.544%
18	11.457	1417	1423	1430	rBV2	48518	102720	0.86%	0.097%
19	12.239	1549	1556	1566	rVB	34926	66421	0.56%	0.063%
20	13.386	1746	1751	1756	rBV3	22078	37216	0.31%	0.035%
21	13.457	1758	1763	1769	rBV4	8585	14662	0.12%	0.014%
22	13.904	1831	1839	1853	rBV	4196903	5604818	46.92%	5.314%
23	14.180	1879	1886	1899	rBV	5281090	7185179	60.15%	6.812%
24	14.486	1931	1938	1948	rBV	3585443	4986171	41.74%	4.727%
25	14.710	1970	1976	1987	rBV	257773	538017	4.50%	0.510%
26	14.910	2004	2010	2017	rVB	21214	50643	0.42%	0.048%
27	15.274	2064	2072	2075	rBV2	10613	19835	0.17%	0.019%
28	15.321	2075	2080	2085	rVB9	7551	13538	0.11%	0.013%
29	15.474	2100	2106	2120	rVV	6873677	9323268	78.05%	8.839%
30	15.604	2121	2128	2141	rVV	2040221	2722594	22.79%	2.581%
31	15.715	2143	2147	2154	rVB2	31889	58659	0.49%	0.056%
32	16.257	2237	2239	2243	rVB5	12570	13572	0.11%	0.013%
33	16.633	2299	2303	2308	rBV7	13589	22121	0.19%	0.021%
34	16.904	2345	2349	2352	rBV5	11489	16838	0.14%	0.016%
35	17.015	2366	2368	2373	rVB4	10879	16322	0.14%	0.015%
36	17.227	2397	2404	2412	rBV	4002659	5625284	47.09%	5.333%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037356.D
 Acq On : 03 Nov 2022 20:51
 Operator : CG/JU
 Sample : N5276-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X6

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	17.327	2414	2421	2432	rBV	7481786	10433455	87.34%	9.891%
38	17.892	2513	2517	2522	rVB	105160	123049	1.03%	0.117%
39	18.115	2551	2555	2565	rBV	176536	301178	2.52%	0.286%
40	18.968	2697	2700	2705	rBV2	38410	51430	0.43%	0.049%
41	19.062	2713	2716	2720	rVB	123529	133232	1.12%	0.126%
42	19.180	2732	2736	2742	rBV3	83323	139345	1.17%	0.132%
43	19.251	2744	2748	2752	rBV	86972	135167	1.13%	0.128%
44	19.392	2769	2772	2780	rBV	141723	217219	1.82%	0.206%
45	19.615	2804	2810	2822	rBV	9944714	11945224	100.00%	11.324%
46	21.397	3108	3113	3122	rBV	4576168	5732536	47.99%	5.435%
47	23.591	3479	3486	3500	rBV2	5134857	9695107	81.16%	9.191%
48	23.744	3505	3512	3523	rVB2	2379723	4778708	40.01%	4.530%




Sum of corrected areas: 105481656

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037356.D
Acq On : 03 Nov 2022 20:51
Operator : CG/JU
Sample : N5276-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

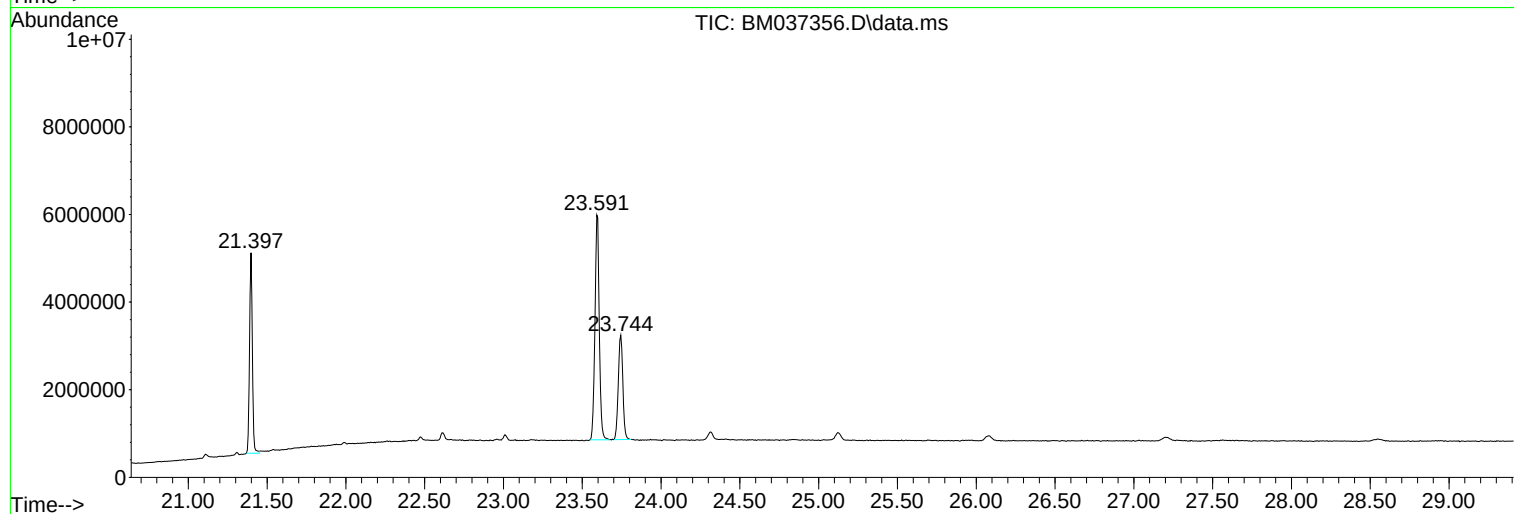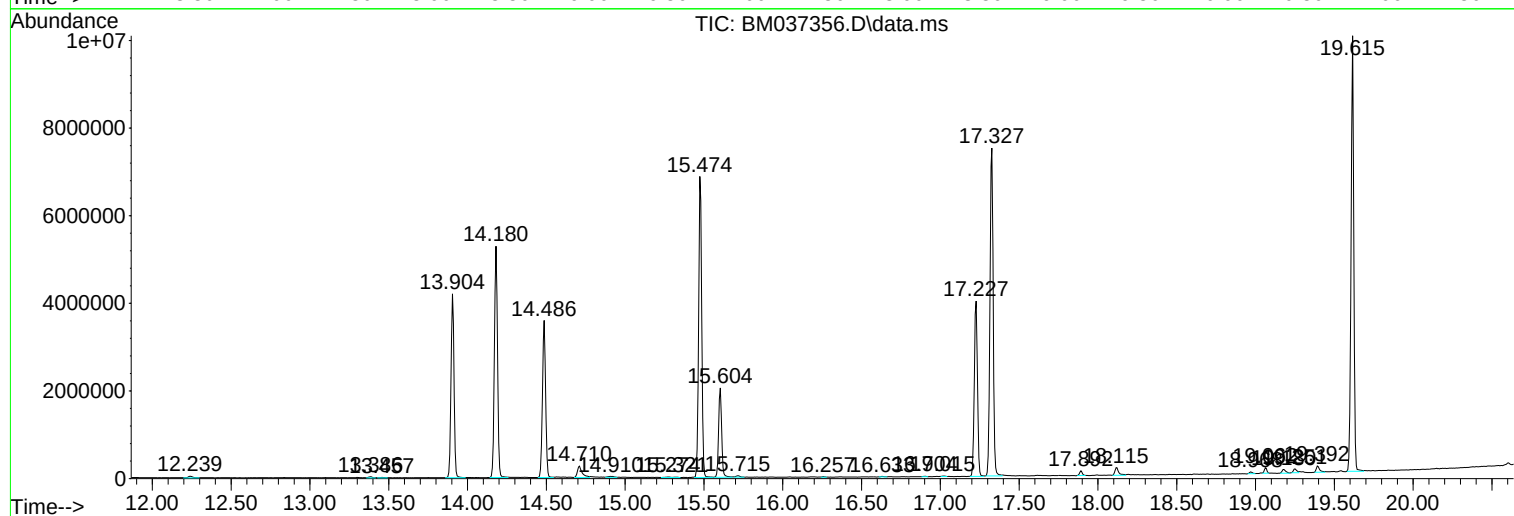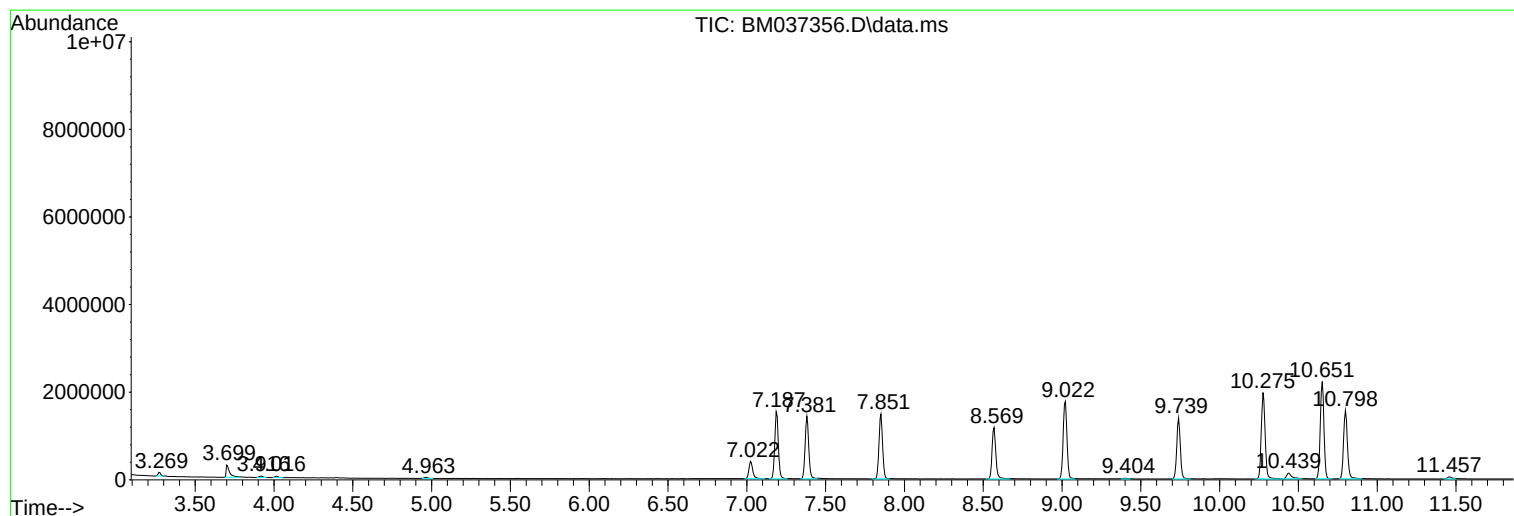

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037356.D
Acq On : 03 Nov 2022 20:51
Operator : CG/JU
Sample : N5276-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037356.D
Acq On : 03 Nov 2022 20:51
Operator : CG/JU
Sample : N5276-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc