

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037357.D
 Acq On : 03 Nov 2022 21:27
 Operator : CG/JU
 Sample : N5276-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	44	rVB	70506	103327	0.98%	0.119%
2	3.916	137	141	147	rVB	25555	38555	0.36%	0.044%
3	4.016	154	158	164	rVB	46730	62510	0.59%	0.072%
4	4.963	314	319	324	rBV	20492	29982	0.28%	0.035%
5	7.022	663	669	683	rVB	308473	523387	4.94%	0.602%
6	7.187	691	697	711	rBV	1245666	1897775	17.91%	2.184%
7	7.381	723	730	739	rBV	1161901	1820589	17.18%	2.096%
8	7.851	802	810	819	rBV	1164330	1867853	17.63%	2.150%
9	8.569	925	932	944	rBV	905651	1533420	14.47%	1.765%
10	9.016	1001	1008	1023	rBV	1435757	2335603	22.04%	2.688%
11	9.739	1123	1131	1145	rBV	1128225	1832547	17.30%	2.109%
12	10.275	1215	1222	1247	rBV	1571027	2750767	25.96%	3.166%
13	10.651	1276	1286	1297	rBV	1803089	2921514	27.57%	3.363%
14	10.810	1302	1313	1323	rBV	68593	159338	1.50%	0.183%
15	11.480	1421	1427	1432	rBV9	9797	23840	0.23%	0.027%
16	11.892	1492	1497	1506	rVB8	5852	11964	0.11%	0.014%
17	12.239	1551	1556	1563	rBV2	26936	46977	0.44%	0.054%
18	13.457	1756	1763	1769	rBV7	7211	11316	0.11%	0.013%
19	13.904	1831	1839	1854	rBV	3446673	4687784	44.24%	5.396%
20	14.180	1879	1886	1901	rBV	4104131	5863717	55.34%	6.749%
21	14.374	1913	1919	1925	rVB9	7781	12662	0.12%	0.015%
22	14.486	1931	1938	1948	rBV	2946503	4146293	39.13%	4.773%
23	14.574	1948	1953	1956	rBV7	7386	15217	0.14%	0.018%
24	14.710	1970	1976	1996	rBV	189539	453083	4.28%	0.522%
25	15.274	2067	2072	2075	rVV3	10824	13309	0.13%	0.015%
26	15.321	2078	2080	2086	rVB6	9623	12010	0.11%	0.014%
27	15.474	2100	2106	2114	rBV	5743162	7828533	73.89%	9.011%
28	15.604	2122	2128	2142	rBV	1815885	2378375	22.45%	2.738%
29	15.715	2143	2147	2155	rVB2	29001	48926	0.46%	0.056%
30	16.186	2223	2227	2234	rVB8	8491	14919	0.14%	0.017%
31	16.898	2345	2348	2355	rBV9	7391	14503	0.14%	0.017%
32	17.227	2397	2404	2414	rBV	3445709	4766741	44.99%	5.487%
33	17.321	2414	2420	2433	rBV	6302572	9064550	85.55%	10.434%
34	17.739	2489	2491	2499	rBV8	5785	13447	0.13%	0.015%
35	17.886	2512	2516	2521	rBV6	29992	46163	0.44%	0.053%
36	18.115	2551	2555	2561	rBV2	53908	78974	0.75%	0.091%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037357.D
 Acq On : 03 Nov 2022 21:27
 Operator : CG/JU
 Sample : N5276-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	18.968	2697	2700	2705	rBV2	33654	38286	0.36%	0.044%
38	19.180	2731	2736	2742	rBV2	70076	105504	1.00%	0.121%
39	19.250	2743	2748	2751	rBV	73853	107744	1.02%	0.124%
40	19.392	2769	2772	2777	rBV5	38405	54666	0.52%	0.063%
41	19.615	2803	2810	2823	rBV	8173521	10595189	100.00%	12.195%
42	21.397	3108	3113	3119	rBV	4142356	5049523	47.66%	5.812%
43	23.591	3479	3486	3497	rVB	5015573	9037177	85.30%	10.402%
44	23.744	3505	3512	3523	rVB2	2273840	4460149	42.10%	5.134%




Sum of corrected areas: 86878708

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037357.D
Acq On : 03 Nov 2022 21:27
Operator : CG/JU
Sample : N5276-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

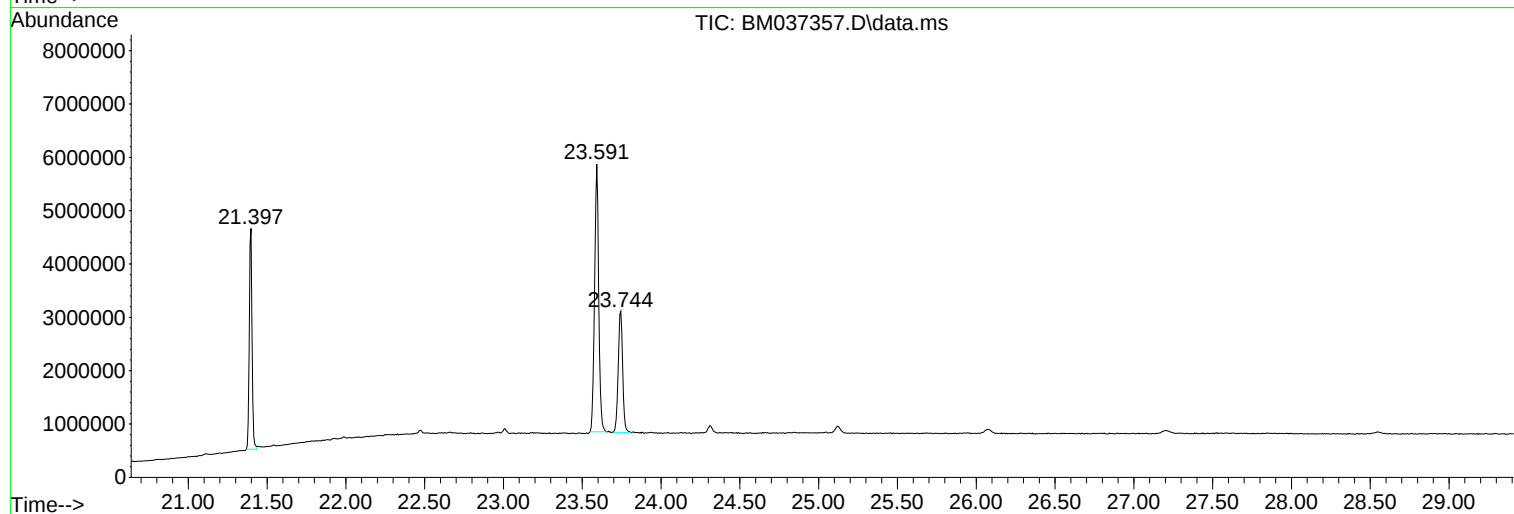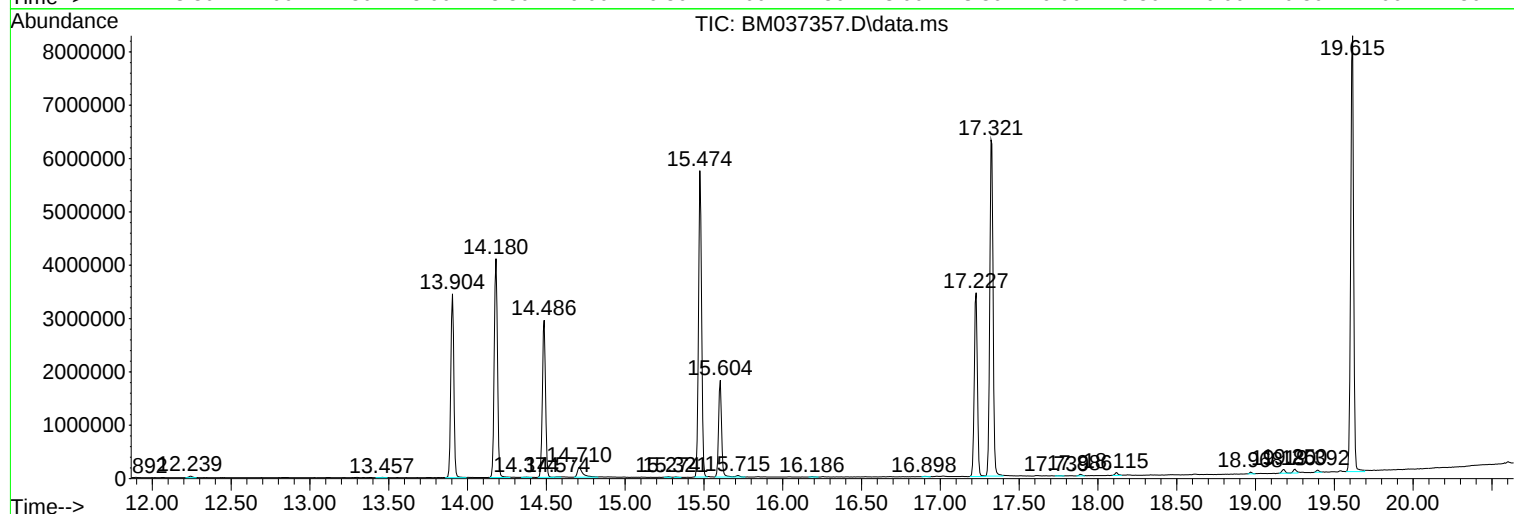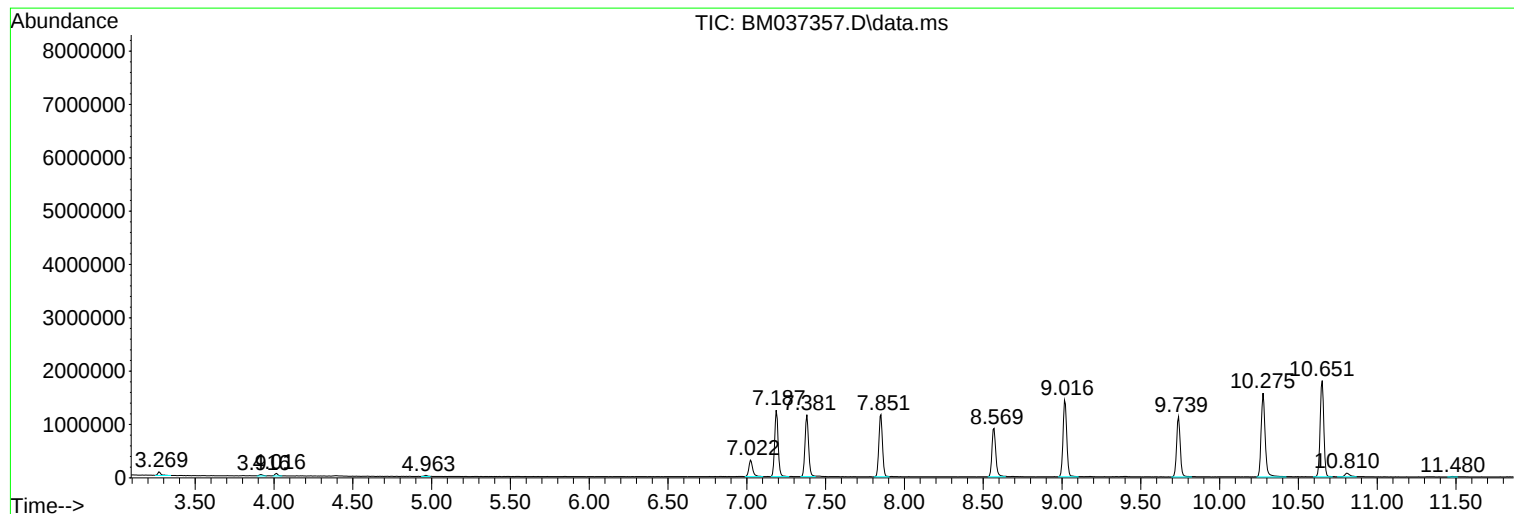

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037357.D
Acq On : 03 Nov 2022 21:27
Operator : CG/JU
Sample : N5276-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037357.D
Acq On : 03 Nov 2022 21:27
Operator : CG/JU
Sample : N5276-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
