

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037358.D
 Acq On : 03 Nov 2022 22:02
 Operator : CG/JU
 Sample : N5276-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	36	rBV	64339	77189	0.88%	0.101%
2	3.728	106	109	117	rBV	24197	49871	0.57%	0.065%
3	3.916	136	141	145	rBV	27112	39762	0.45%	0.052%
4	4.016	154	158	162	rVB	25693	32326	0.37%	0.042%
5	4.963	312	319	328	rBV	20462	38483	0.44%	0.050%
6	7.022	663	669	683	rBV	262549	452047	5.14%	0.593%
7	7.187	691	697	711	rBV	1093455	1677563	19.08%	2.201%
8	7.381	723	730	740	rBV	990067	1563948	17.79%	2.052%
9	7.457	741	743	750	rVB8	10609	14356	0.16%	0.019%
10	7.846	802	809	821	rBV	1143300	1819099	20.69%	2.387%
11	8.563	921	931	947	rBV	747248	1309934	14.90%	1.719%
12	9.016	999	1008	1021	rBV	1294356	2058674	23.42%	2.702%
13	9.404	1069	1074	1079	rVB	9432	16980	0.19%	0.022%
14	9.739	1122	1131	1142	rBV	946764	1553757	17.67%	2.039%
15	10.275	1214	1222	1245	rBV	1365217	2354139	26.78%	3.089%
16	10.445	1245	1251	1266	rVV2	39988	118268	1.35%	0.155%
17	10.651	1278	1286	1295	rBV	1690280	2834731	32.24%	3.720%
18	10.798	1304	1311	1323	rBV	239531	453844	5.16%	0.596%
19	11.892	1492	1497	1502	rVB5	6415	12575	0.14%	0.017%
20	12.239	1551	1556	1564	rBV	23038	39452	0.45%	0.052%
21	13.386	1747	1751	1756	rVB7	7402	12381	0.14%	0.016%
22	13.457	1760	1763	1767	rVB6	6592	8833	0.10%	0.012%
23	13.904	1832	1839	1851	rBV	2966418	3989371	45.38%	5.235%
24	14.180	1878	1886	1901	rBV	3578597	5077074	57.75%	6.662%
25	14.486	1931	1938	1950	rBV	2659170	3987340	45.36%	5.232%
26	14.710	1970	1976	1993	rBV	133245	344586	3.92%	0.452%
27	15.321	2075	2080	2083	rVB7	4885	8950	0.10%	0.012%
28	15.474	2096	2106	2118	rBV	4933727	6701974	76.23%	8.795%
29	15.598	2121	2127	2141	rVV	1311785	1851797	21.06%	2.430%
30	15.710	2143	2146	2152	rVB2	23212	36182	0.41%	0.047%
31	16.251	2235	2238	2244	rVB7	7915	12311	0.14%	0.016%
32	17.221	2397	2403	2412	rBV	3322302	4621873	52.57%	6.065%
33	17.321	2414	2420	2437	rVV	5453805	7656627	87.09%	10.047%
34	17.892	2513	2517	2522	rBV	45939	60209	0.68%	0.079%
35	18.115	2551	2555	2565	rBV3	93065	161240	1.83%	0.212%
36	19.062	2713	2716	2720	rVB5	23273	28450	0.32%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037358.D
Acq On : 03 Nov 2022 22:02
Operator : CG/JU
Sample : N5276-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Title : SVOA CALIBRATION

37	19.180	2732	2736	2742	rBV3	57991	86556	0.98%	0.114%
38	19.251	2744	2748	2754	rBV2	62380	109507	1.25%	0.144%
39	19.392	2769	2772	2780	rBV3	73659	112042	1.27%	0.147%
40	19.609	2803	2809	2821	rBV	6811226	8791286	100.00%	11.536%
41	21.398	3108	3113	3121	rBV	3688640	4711359	53.59%	6.183%
42	23.592	3479	3486	3499	rVB	3773380	7246520	82.43%	9.509%
43	23.739	3505	3511	3522	rVB2	2131017	4070891	46.31%	5.342%




Sum of corrected areas: 76204357

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037358.D
Acq On : 03 Nov 2022 22:02
Operator : CG/JU
Sample : N5276-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

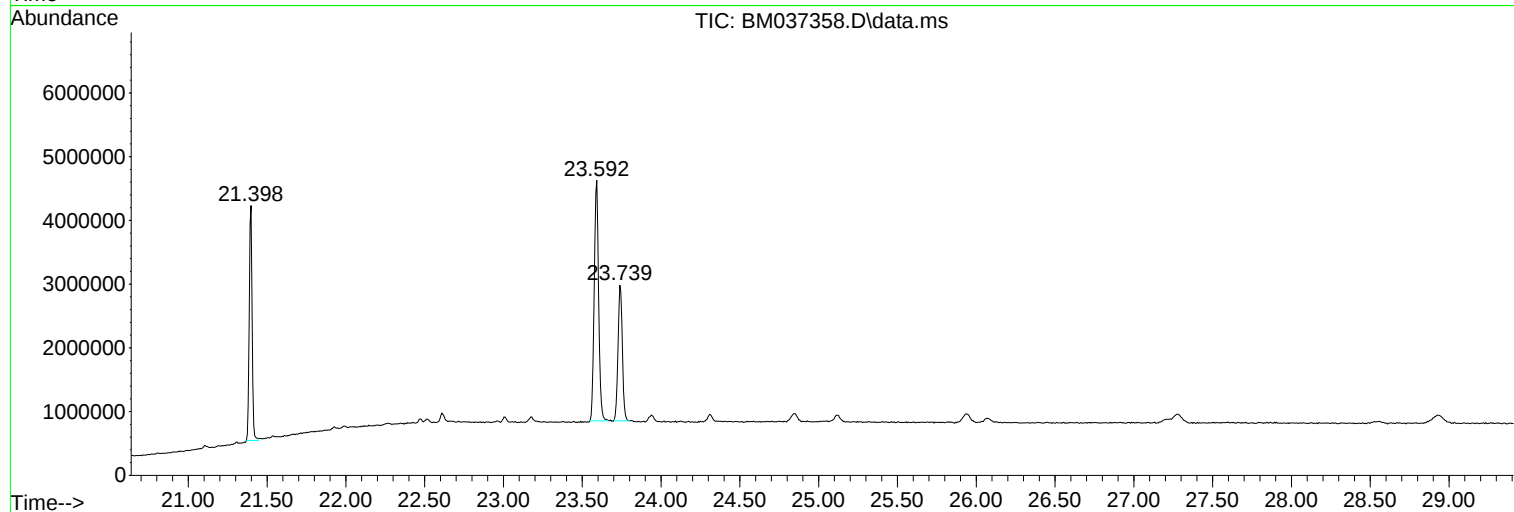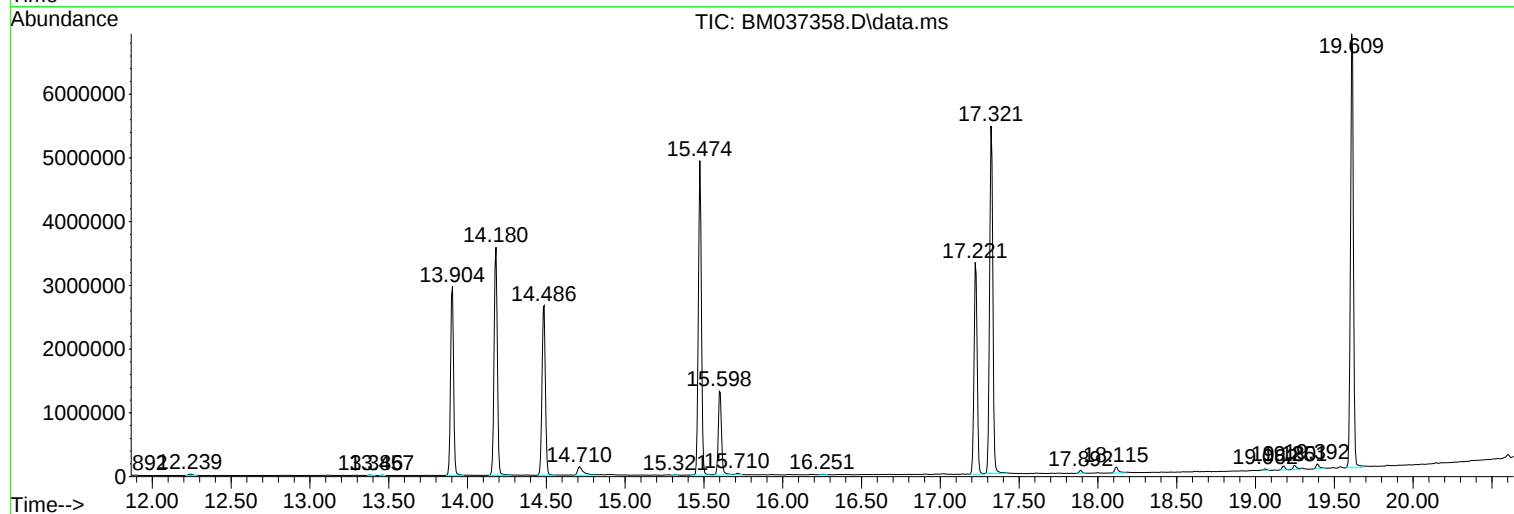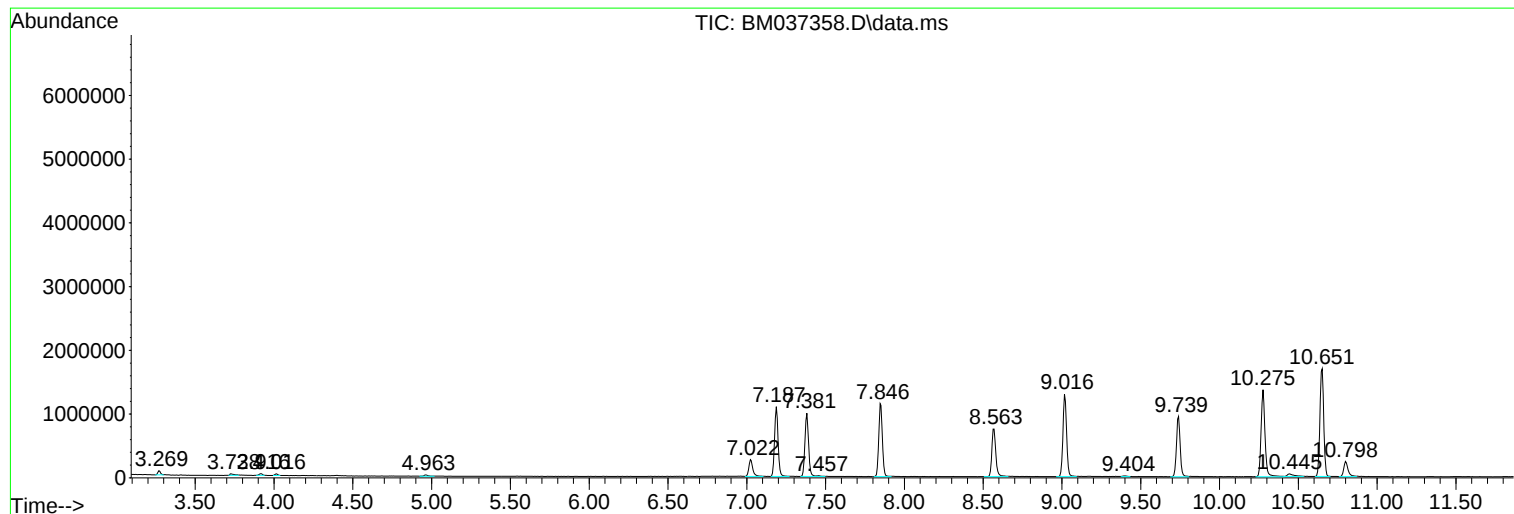

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037358.D
Acq On : 03 Nov 2022 22:02
Operator : CG/JU
Sample : N5276-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037358.D
Acq On : 03 Nov 2022 22:02
Operator : CG/JU
Sample : N5276-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
