

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037363.D
 Acq On : 04 Nov 2022 01:34
 Operator : CG/JU
 Sample : PB148648BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK648

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	42	rVB	106117	145645	1.57%	0.156%
2	3.693	99	103	131	rBV	1202027	1944306	21.02%	2.084%
3	4.011	154	157	162	rVB	20622	28853	0.31%	0.031%
4	7.022	662	669	682	rBV	1499417	2401678	25.97%	2.575%
5	7.187	689	697	710	rBV	1315944	1997848	21.60%	2.142%
6	7.381	722	730	745	rBV	1512439	2452017	26.51%	2.629%
7	7.846	802	809	824	rBV	1193027	1884872	20.38%	2.021%
8	8.563	924	931	946	rBV	1907183	3049694	32.97%	3.269%
9	9.016	1001	1008	1022	rBV	1543534	2440019	26.38%	2.616%
10	9.734	1120	1130	1146	rBV	1221969	2015099	21.79%	2.160%
11	10.275	1214	1222	1240	rBV	1830625	3132325	33.87%	3.358%
12	10.645	1278	1285	1300	rVB	1783206	2943387	31.82%	3.155%
13	10.798	1303	1311	1332	rBV	1793255	3262487	35.27%	3.497%
14	12.245	1547	1557	1567	rBV3	22749	54771	0.59%	0.059%
15	13.381	1745	1750	1757	rBV8	7340	14169	0.15%	0.015%
16	13.463	1759	1764	1769	rVB7	6799	12933	0.14%	0.014%
17	13.898	1828	1838	1851	rBV	3291100	4589060	49.62%	4.919%
18	14.181	1878	1886	1903	rBV	4090713	6043368	65.34%	6.478%
19	14.480	1930	1937	1947	rBV	2939669	4182909	45.23%	4.484%
20	14.698	1966	1974	1997	rBV	1253375	2180495	23.58%	2.337%
21	14.892	2003	2007	2017	rVB	9398	24435	0.26%	0.026%
22	15.475	2099	2106	2121	rBV	5478346	7641280	82.62%	8.191%
23	15.598	2121	2127	2142	rVV	1448380	2048145	22.15%	2.196%
24	15.710	2142	2146	2155	rVB2	26312	44034	0.48%	0.047%
25	17.016	2363	2368	2371	rBV3	6185	10693	0.12%	0.011%
26	17.221	2397	2403	2412	rBV	3415883	4772335	51.60%	5.116%
27	17.321	2414	2420	2440	rVB	6099446	8225768	88.94%	8.818%
28	19.174	2731	2735	2741	rBV2	64455	85671	0.93%	0.092%
29	19.245	2744	2747	2752	rVV	44966	63259	0.68%	0.068%
30	19.610	2803	2809	2818	rBV	7269267	9248788	100.00%	9.915%
31	21.392	3107	3112	3122	rBV	3717400	4855233	52.50%	5.205%
32	23.586	3478	3485	3497	rBV2	3951235	7443566	80.48%	7.979%
33	23.739	3504	3511	3520	rBV2	2108949	4044964	43.74%	4.336%




Sum of corrected areas: 93284106

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037363.D
Acq On : 04 Nov 2022 01:34
Operator : CG/JU
Sample : PB148648BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

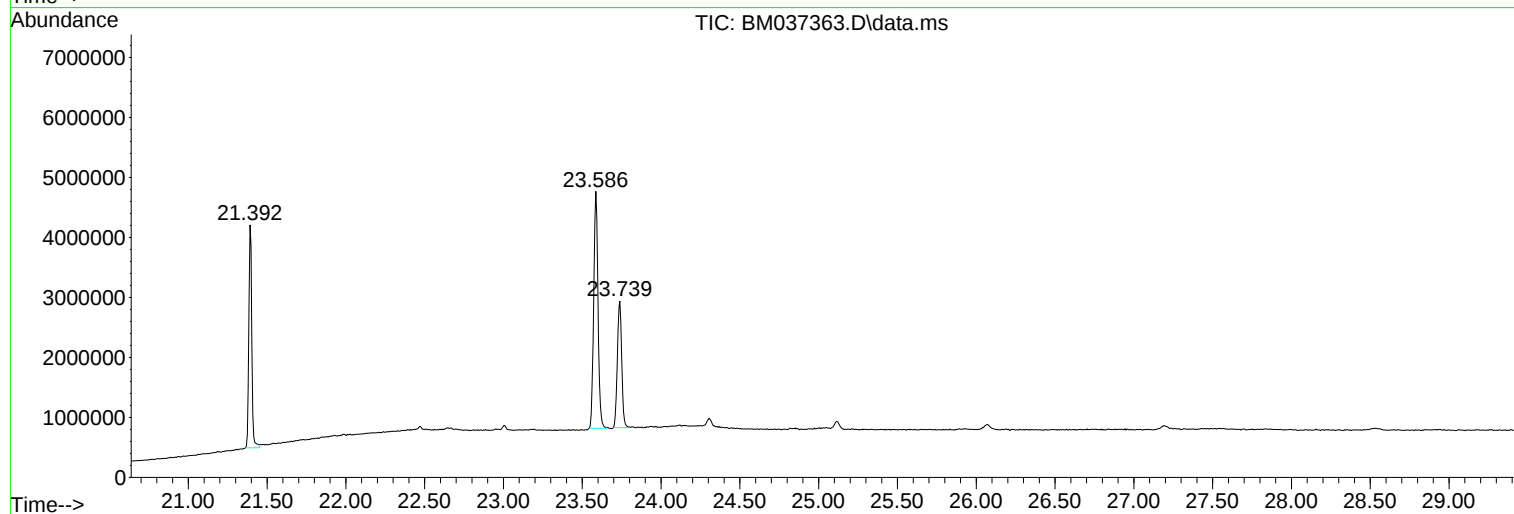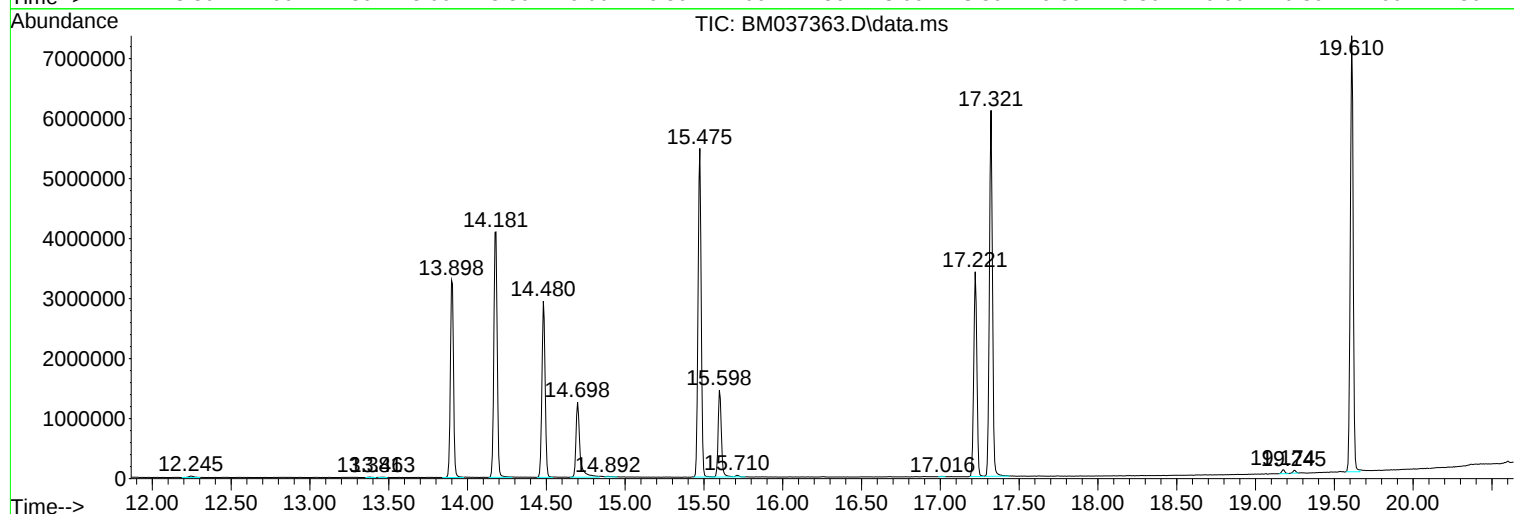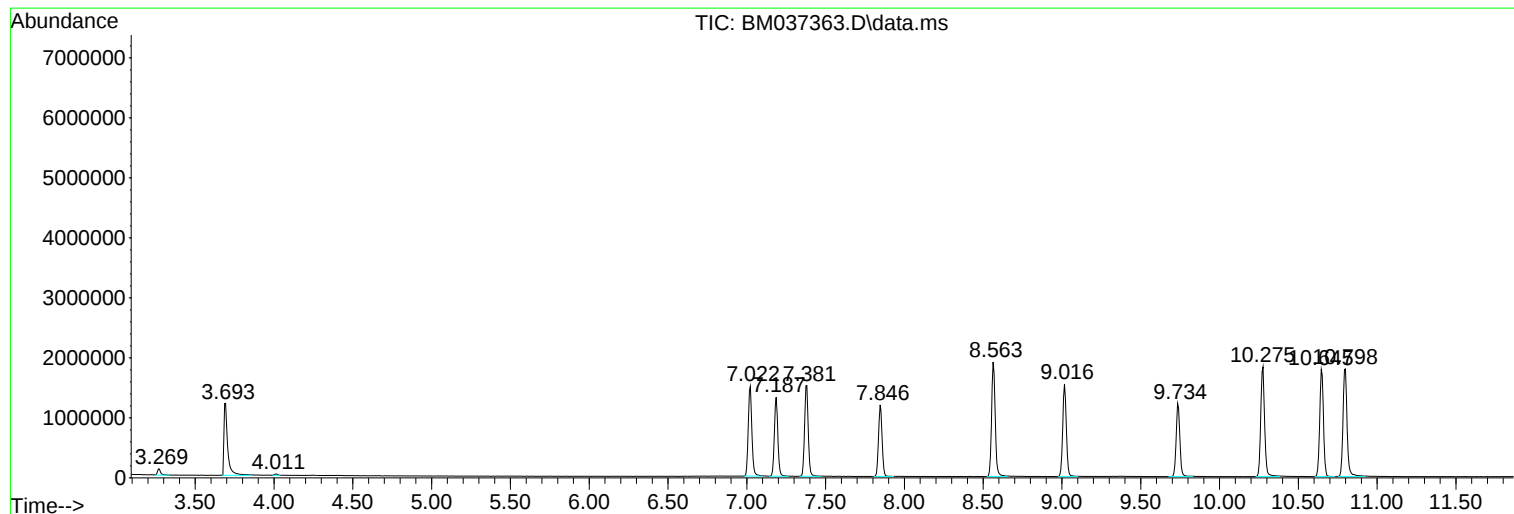

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037363.D
Acq On : 04 Nov 2022 01:34
Operator : CG/JU
Sample : PB148648BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037363.D
Acq On : 04 Nov 2022 01:34
Operator : CG/JU
Sample : PB148648BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc