

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037364.D
 Acq On : 04 Nov 2022 02:09
 Operator : CG/JU
 Sample : PB148654BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	41	rVB	117847	150867	1.50%	0.154%
2	3.693	99	103	126	rBV	1341896	2143298	21.35%	2.186%
3	4.016	154	158	167	rVB	20041	34487	0.34%	0.035%
4	7.022	661	669	684	rBV	1623762	2647613	26.37%	2.701%
5	7.187	689	697	709	rBV	1423905	2163877	21.55%	2.207%
6	7.375	723	729	741	rBV	1685519	2684572	26.74%	2.738%
7	7.845	802	809	820	rBV	1153340	1794686	17.88%	1.831%
8	8.563	924	931	949	rBV	2071668	3332385	33.19%	3.399%
9	9.016	1000	1008	1019	rBV	1663812	2637018	26.27%	2.690%
10	9.734	1122	1130	1141	rBV	1314866	2155121	21.47%	2.198%
11	10.275	1212	1222	1238	rBV	1932180	3373850	33.61%	3.442%
12	10.645	1277	1285	1298	rBV	1729616	2807157	27.96%	2.864%
13	10.792	1303	1310	1326	rBV	1985476	3520088	35.06%	3.591%
14	12.239	1551	1556	1567	rBV2	23202	48821	0.49%	0.050%
15	13.457	1758	1763	1768	rBV6	5489	10665	0.11%	0.011%
16	13.898	1831	1838	1852	rBV	3553930	4886308	48.67%	4.984%
17	14.174	1879	1885	1900	rBV	4406949	6398019	63.73%	6.527%
18	14.480	1930	1937	1947	rBV	2801895	3940223	39.25%	4.019%
19	14.698	1967	1974	1994	rBV	1385599	2359396	23.50%	2.407%
20	15.474	2099	2106	2121	rVB	5833506	8153874	81.22%	8.318%
21	15.598	2121	2127	2141	rBV	1590029	2238431	22.30%	2.283%
22	15.710	2142	2146	2154	rVB3	28767	44327	0.44%	0.045%
23	17.015	2364	2368	2374	rBV6	6683	12171	0.12%	0.012%
24	17.221	2397	2403	2413	rBV	3424215	4520482	45.03%	4.611%
25	17.321	2413	2420	2437	rVV	6742566	8801762	87.67%	8.979%
26	19.174	2731	2735	2741	rBV3	64506	89392	0.89%	0.091%
27	19.245	2743	2747	2752	rBV	54656	83422	0.83%	0.085%
28	19.609	2803	2809	2819	rBV	8123910	10039560	100.00%	10.241%
29	21.392	3107	3112	3121	rBV	3726039	4659806	46.41%	4.753%
30	23.586	3478	3485	3498	rBV2	4567579	8321430	82.89%	8.489%
31	23.739	3504	3511	3525	rVB2	2066028	3977646	39.62%	4.058%




Sum of corrected areas: 98030754

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037364.D
Acq On : 04 Nov 2022 02:09
Operator : CG/JU
Sample : PB148654BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK654

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

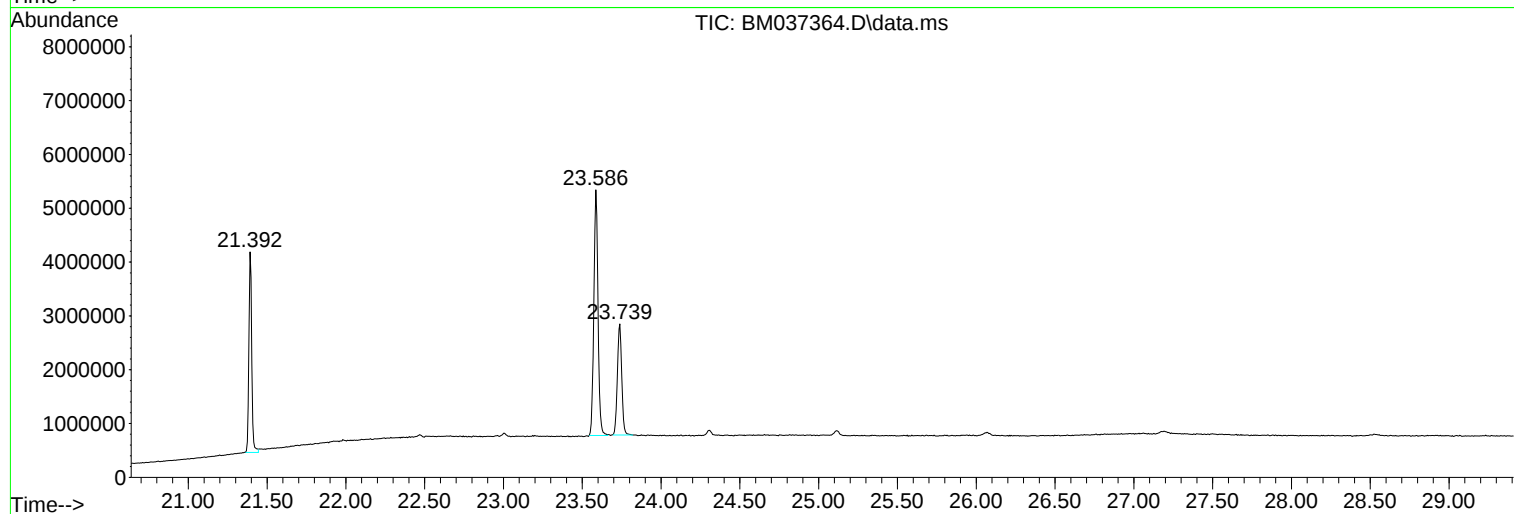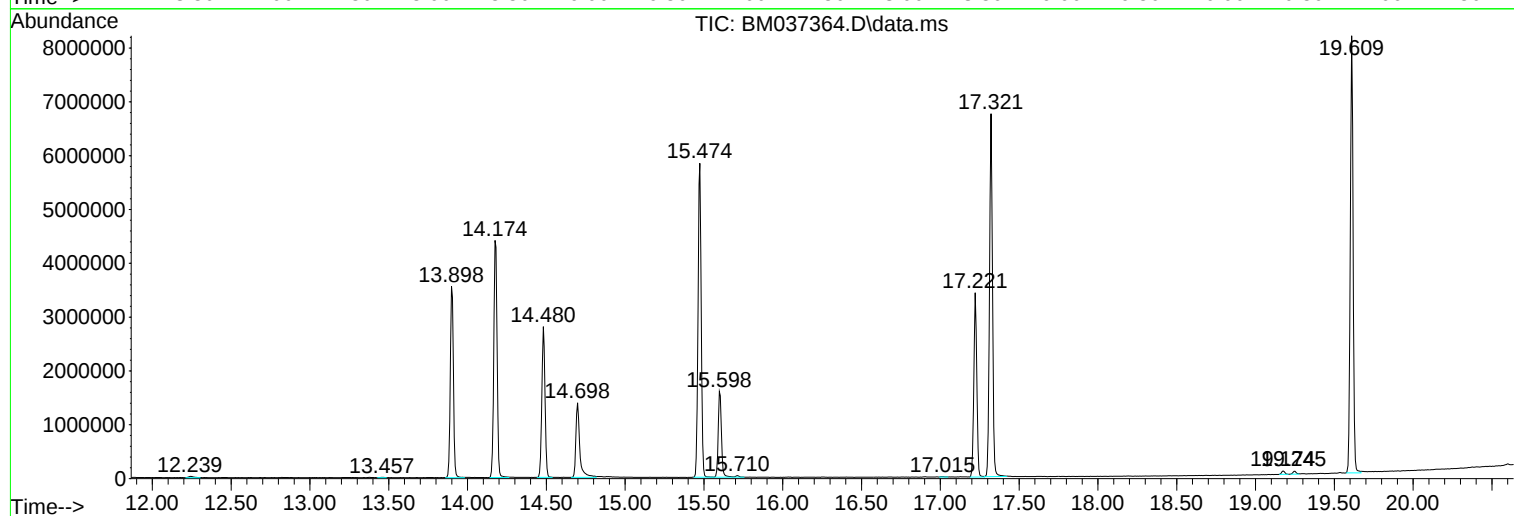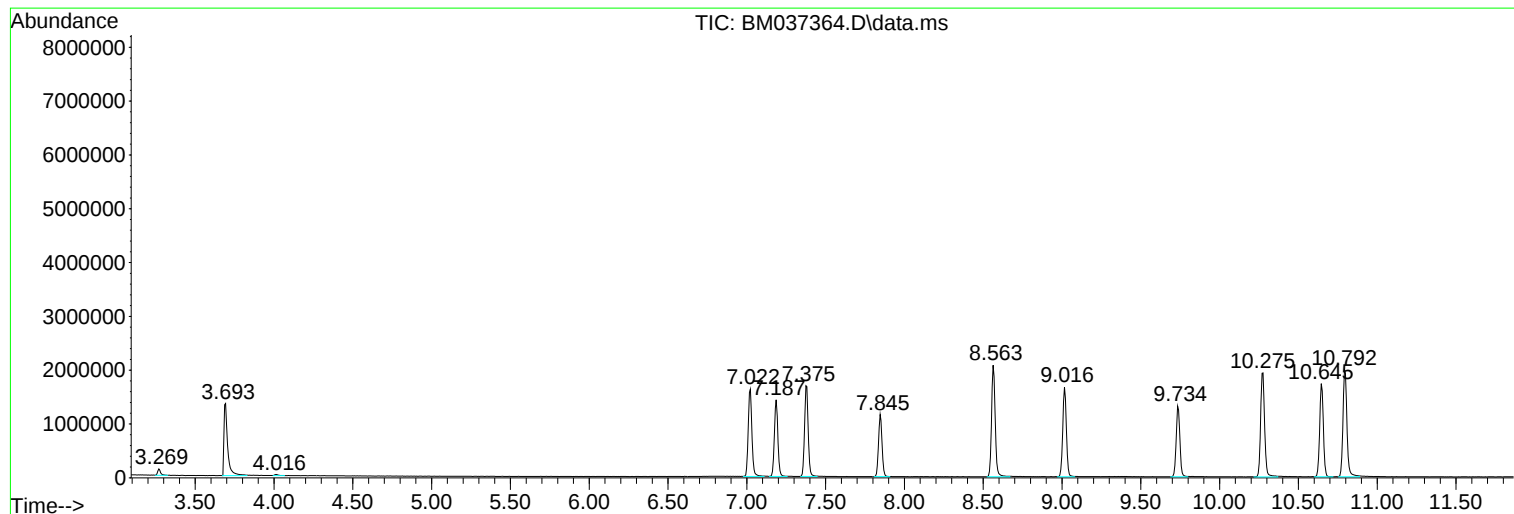

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037364.D
Acq On : 04 Nov 2022 02:09
Operator : CG/JU
Sample : PB148654BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK654

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037364.D
Acq On : 04 Nov 2022 02:09
Operator : CG/JU
Sample : PB148654BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK654

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc