

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037365.D
 Acq On : 04 Nov 2022 02:45
 Operator : CG/JU
 Sample : N5276-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	37	rBV	70661	88351	0.92%	0.104%
2	3.916	137	141	145	rVB	25642	35365	0.37%	0.042%
3	4.010	153	157	162	rBV	39896	56579	0.59%	0.066%
4	4.434	227	229	236	rVB5	8937	15220	0.16%	0.018%
5	4.957	314	318	328	rVB	16603	31895	0.33%	0.037%
6	7.022	663	669	685	rVB	357735	601021	6.27%	0.705%
7	7.187	690	697	710	rBV	1395049	2176136	22.69%	2.554%
8	7.375	723	729	740	rBV	1311108	2081863	21.70%	2.443%
9	7.845	802	809	817	rBV	1263194	1976513	20.60%	2.320%
10	7.916	819	821	826	rVB5	6812	9889	0.10%	0.012%
11	8.563	925	931	948	rBV	1068845	1725369	17.99%	2.025%
12	9.016	1000	1008	1020	rBV	1665892	2661546	27.75%	3.124%
13	9.398	1070	1073	1081	rVB8	8608	14301	0.15%	0.017%
14	9.734	1121	1130	1142	rBV	1294153	2067567	21.55%	2.427%
15	10.269	1214	1221	1239	rBV	1822448	3083872	32.15%	3.619%
16	10.451	1246	1252	1260	rBV10	10094	27018	0.28%	0.032%
17	10.645	1275	1285	1293	rBV	1838224	3025706	31.54%	3.551%
18	10.804	1305	1312	1320	rBV2	60331	131143	1.37%	0.154%
19	11.886	1491	1496	1503	rVB9	6163	13042	0.14%	0.015%
20	11.998	1511	1515	1521	rVB	14965	25581	0.27%	0.030%
21	12.233	1550	1555	1561	rBV2	27635	48972	0.51%	0.057%
22	12.304	1562	1567	1579	rBV	56626	165502	1.73%	0.194%
23	12.851	1653	1660	1664	rBV9	5912	11118	0.12%	0.013%
24	13.092	1696	1701	1705	rBV7	7797	13649	0.14%	0.016%
25	13.298	1730	1736	1741	rBV8	5529	12914	0.13%	0.015%
26	13.451	1757	1762	1767	rBV8	8535	16172	0.17%	0.019%
27	13.898	1831	1838	1849	rBV	3636824	4882133	50.89%	5.730%
28	14.004	1852	1856	1862	rVB9	12867	22570	0.24%	0.026%
29	14.174	1878	1885	1898	rBV	4378111	6379507	66.50%	7.487%
30	14.480	1930	1937	1948	rBV	2825398	4053020	42.25%	4.757%
31	14.704	1970	1975	1989	rBV	184548	414024	4.32%	0.486%
32	14.892	2003	2007	2010	rBV5	7167	12796	0.13%	0.015%
33	15.274	2067	2072	2073	rBV	11412	14947	0.16%	0.018%
34	15.304	2073	2077	2087	rVB	101289	138730	1.45%	0.163%
35	15.474	2099	2106	2120	rVB	5886860	8080420	84.24%	9.483%
36	15.598	2120	2127	2141	rBV	1708989	2266099	23.62%	2.660%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037365.D
 Acq On : 04 Nov 2022 02:45
 Operator : CG/JU
 Sample : N5276-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	15.710	2141	2146	2152	rVB2	28737	48189	0.50%	0.057%
38	15.886	2172	2176	2180	rBV6	7414	13246	0.14%	0.016%
39	16.045	2198	2203	2207	rBV7	5972	10904	0.11%	0.013%
40	16.727	2314	2319	2328	rBV	125763	252328	2.63%	0.296%
41	17.221	2397	2403	2413	rBV	3283741	4474984	46.65%	5.252%
42	17.321	2413	2420	2435	rVV	6418697	8665557	90.34%	10.170%
43	17.509	2448	2452	2458	rVB4	7218	11216	0.12%	0.013%
44	17.609	2465	2469	2479	rBV9	12268	24611	0.26%	0.029%
45	17.892	2513	2517	2521	rBV6	11405	15817	0.16%	0.019%
46	18.115	2550	2555	2564	rBV3	98641	172907	1.80%	0.203%
47	19.174	2731	2735	2742	rVB2	68186	92278	0.96%	0.108%
48	19.245	2743	2747	2753	rBV	68604	107318	1.12%	0.126%
49	19.392	2768	2772	2778	rBV	91279	133320	1.39%	0.156%
50	19.609	2803	2809	2825	rBV	7801479	9592641	100.00%	11.258%
51	21.392	3107	3112	3120	rBV	3485085	4160069	43.37%	4.882%
52	23.586	3478	3485	3496	rVB2	3912866	7405354	77.20%	8.691%
53	23.733	3504	3510	3523	rVB2	1881087	3644751	38.00%	4.278%




Sum of corrected areas: 85206040

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037365.D
Acq On : 04 Nov 2022 02:45
Operator : CG/JU
Sample : N5276-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

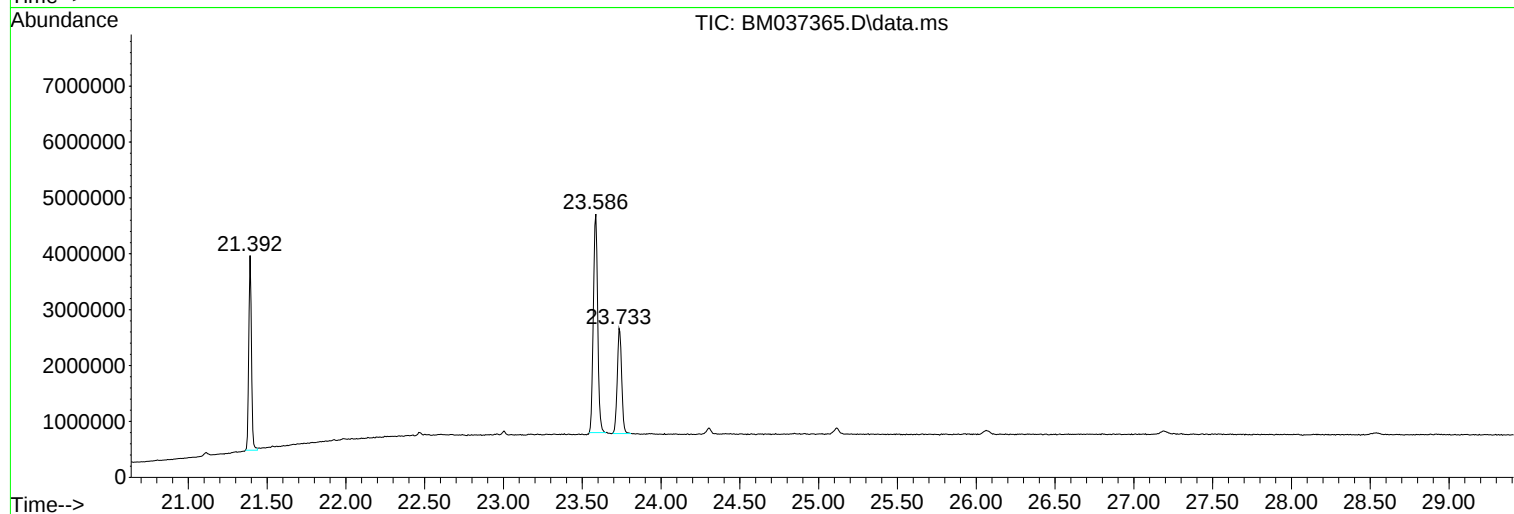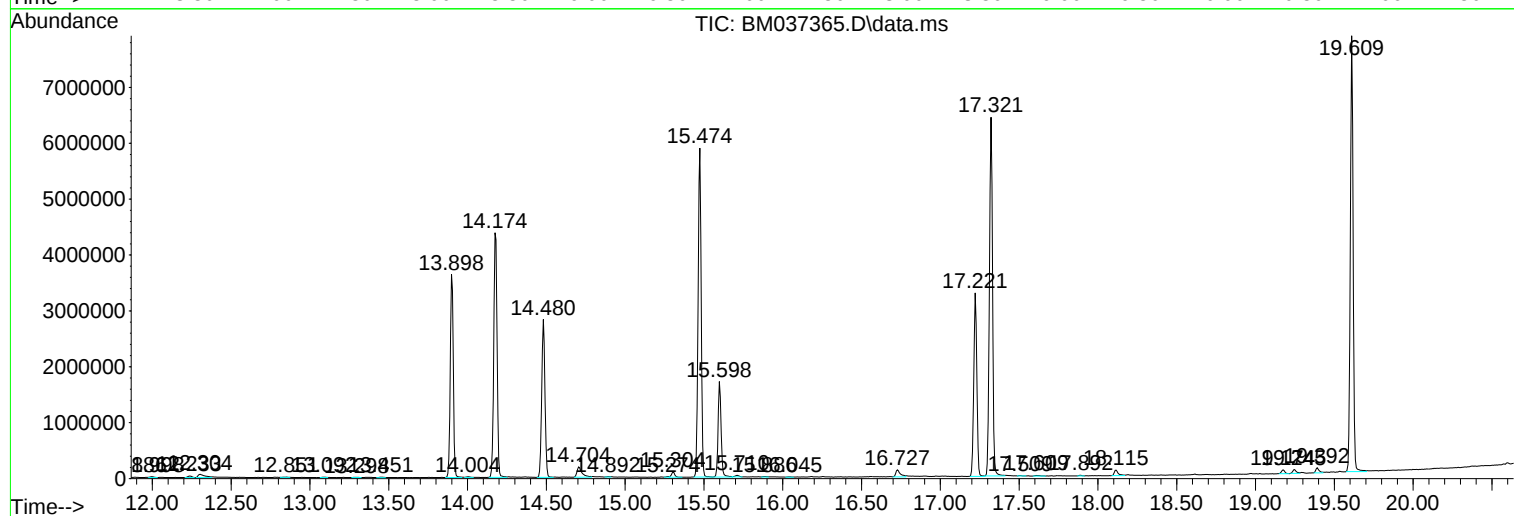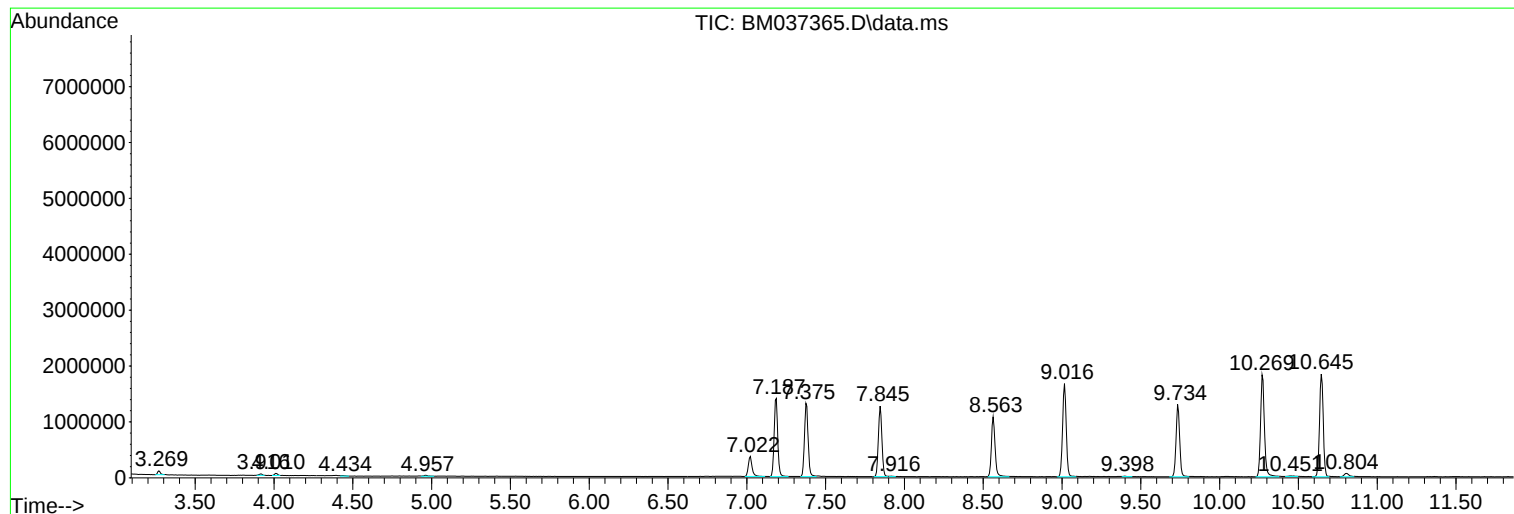

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037365.D
Acq On : 04 Nov 2022 02:45
Operator : CG/JU
Sample : N5276-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037365.D
Acq On : 04 Nov 2022 02:45
Operator : CG/JU
Sample : N5276-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
