

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037366.D
 Acq On : 04 Nov 2022 03:20
 Operator : CG/JU
 Sample : N5276-17
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037366.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rVB	75322	90484	1.00%	0.103%
2	3.699	102	104	126	rBV	320395	524371	5.79%	0.599%
3	3.916	137	141	148	rVB	32991	50855	0.56%	0.058%
4	4.010	154	157	162	rVB	25450	35370	0.39%	0.040%
5	4.963	313	319	327	rVB	30298	48670	0.54%	0.056%
6	6.510	576	582	588	rBV9	5832	10666	0.12%	0.012%
7	7.022	663	669	687	rVB	408383	726370	8.01%	0.830%
8	7.187	690	697	709	rBV	1536123	2413620	26.63%	2.758%
9	7.375	722	729	740	rBV	1430327	2329525	25.70%	2.662%
10	7.451	740	742	747	rVB4	10430	14506	0.16%	0.017%
11	7.845	802	809	818	rBV	1044329	1615257	17.82%	1.846%
12	7.916	818	821	826	rVB5	9442	16605	0.18%	0.019%
13	8.563	919	931	949	rBV	1211540	1974721	21.79%	2.257%
14	9.016	1000	1008	1025	rBV	1853916	2934408	32.37%	3.353%
15	9.392	1069	1072	1082	rVB2	18920	33523	0.37%	0.038%
16	9.734	1123	1130	1141	rBV	1411493	2251354	24.84%	2.573%
17	10.269	1214	1221	1241	rBV	2013653	3402477	37.54%	3.888%
18	10.434	1244	1249	1262	rBV2	61500	165267	1.82%	0.189%
19	10.645	1277	1285	1295	rBV	1525002	2441029	26.93%	2.790%
20	10.792	1303	1310	1324	rBV	1621942	2827696	31.20%	3.231%
21	11.457	1418	1423	1434	rBV4	26715	77134	0.85%	0.088%
22	11.886	1493	1496	1502	rVB2	8491	12660	0.14%	0.014%
23	12.233	1548	1555	1563	rBV3	35510	60213	0.66%	0.069%
24	13.298	1733	1736	1742	rVB5	7788	12232	0.13%	0.014%
25	13.375	1744	1749	1755	rBV4	10925	19711	0.22%	0.023%
26	13.451	1758	1762	1767	rBV4	8072	12415	0.14%	0.014%
27	13.898	1829	1838	1851	rBV	3785319	5340026	58.91%	6.102%
28	14.010	1851	1857	1861	rVB7	13347	21978	0.24%	0.025%
29	14.175	1873	1885	1901	rBV	5036616	7041830	77.69%	8.047%
30	14.369	1915	1918	1923	rVB6	6118	9375	0.10%	0.011%
31	14.480	1929	1937	1945	rBV	2268021	3200484	35.31%	3.657%
32	14.563	1947	1951	1955	rBV6	11197	19605	0.22%	0.022%
33	14.704	1970	1975	1991	rBV	199394	445292	4.91%	0.509%
34	14.992	2019	2024	2029	rBV9	4986	9260	0.10%	0.011%
35	15.104	2040	2043	2048	rVB5	7340	9651	0.11%	0.011%
36	15.269	2066	2071	2075	rBV2	19344	28094	0.31%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037366.D
 Acq On : 04 Nov 2022 03:20
 Operator : CG/JU
 Sample : N5276-17
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	15.316	2075	2079	2083	rVB4	10316	16015	0.18%	0.018%
38	15.474	2099	2106	2121	rBV	6211396	8763370	96.68%	10.015%
39	15.598	2121	2127	2141	rVV	1788956	2298301	25.36%	2.626%
40	15.710	2142	2146	2152	rVB2	31047	48040	0.53%	0.055%
41	15.927	2180	2183	2192	rVB2	8579	14707	0.16%	0.017%
42	16.039	2198	2202	2207	rBV7	6109	12482	0.14%	0.014%
43	16.180	2223	2226	2232	rVV5	7880	12516	0.14%	0.014%
44	16.257	2235	2239	2243	rVB7	9303	14819	0.16%	0.017%
45	16.633	2297	2303	2306	rBV7	6284	12722	0.14%	0.015%
46	16.680	2308	2311	2317	rVB8	4634	9100	0.10%	0.010%
47	16.898	2345	2348	2354	rVB7	9832	15483	0.17%	0.018%
48	16.968	2357	2360	2364	rBV6	8154	14512	0.16%	0.017%
49	17.139	2386	2389	2394	rVB6	7977	9358	0.10%	0.011%
50	17.221	2396	2403	2413	rBV	2367244	3298849	36.40%	3.770%
51	17.321	2413	2420	2431	rBV	6545870	8876313	97.93%	10.144%
52	17.610	2467	2469	2474	rBV5	11944	14619	0.16%	0.017%
53	17.886	2513	2516	2520	rVB2	23874	25171	0.28%	0.029%
54	18.110	2550	2554	2565	rBV	127595	220498	2.43%	0.252%
55	18.962	2696	2699	2704	rBV	39715	45694	0.50%	0.052%
56	19.174	2731	2735	2740	rBV2	66302	92649	1.02%	0.106%
57	19.245	2743	2747	2755	rVV2	59686	102728	1.13%	0.117%
58	19.386	2768	2771	2777	rBV	62418	96331	1.06%	0.110%
59	19.609	2803	2809	2820	rBV	7270606	9063952	100.00%	10.358%
60	21.115	3061	3065	3071	rBV4	132542	256525	2.83%	0.293%
61	21.392	3107	3112	3118	rBV	2370130	2914853	32.16%	3.331%
62	23.586	3478	3485	3500	rVB2	4249897	8199116	90.46%	9.370%
63	23.733	3505	3510	3521	rVB2	1465317	2831213	31.24%	3.235%




Sum of corrected areas: 87506670

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037366.D
Acq On : 04 Nov 2022 03:20
Operator : CG/JU
Sample : N5276-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

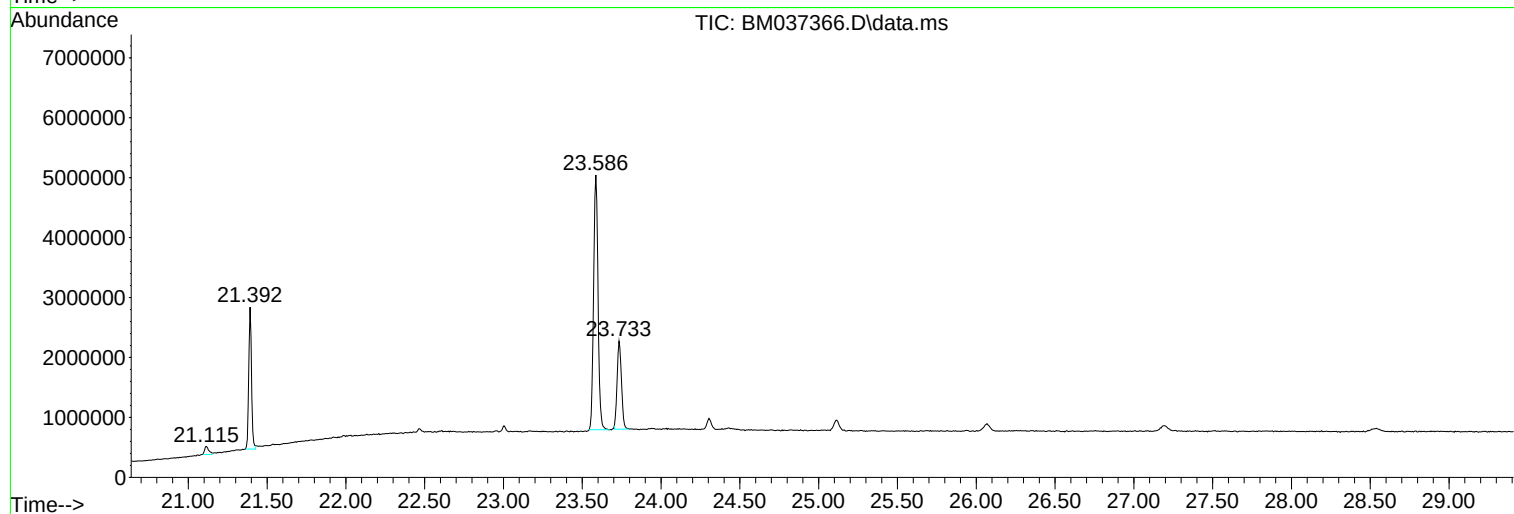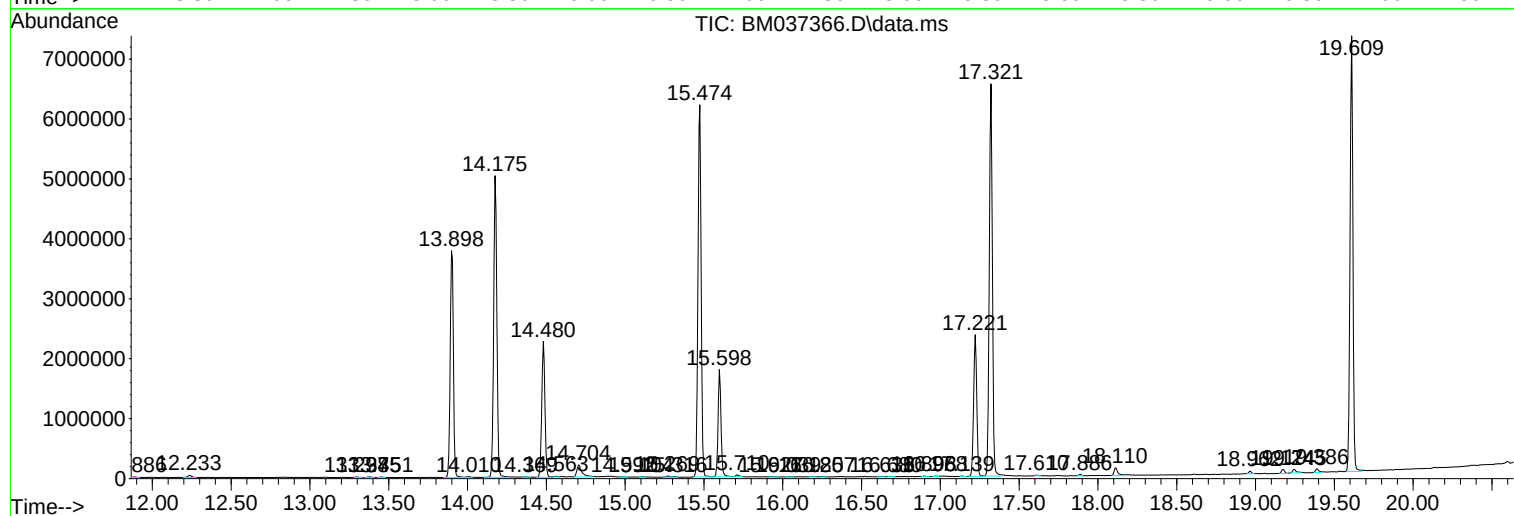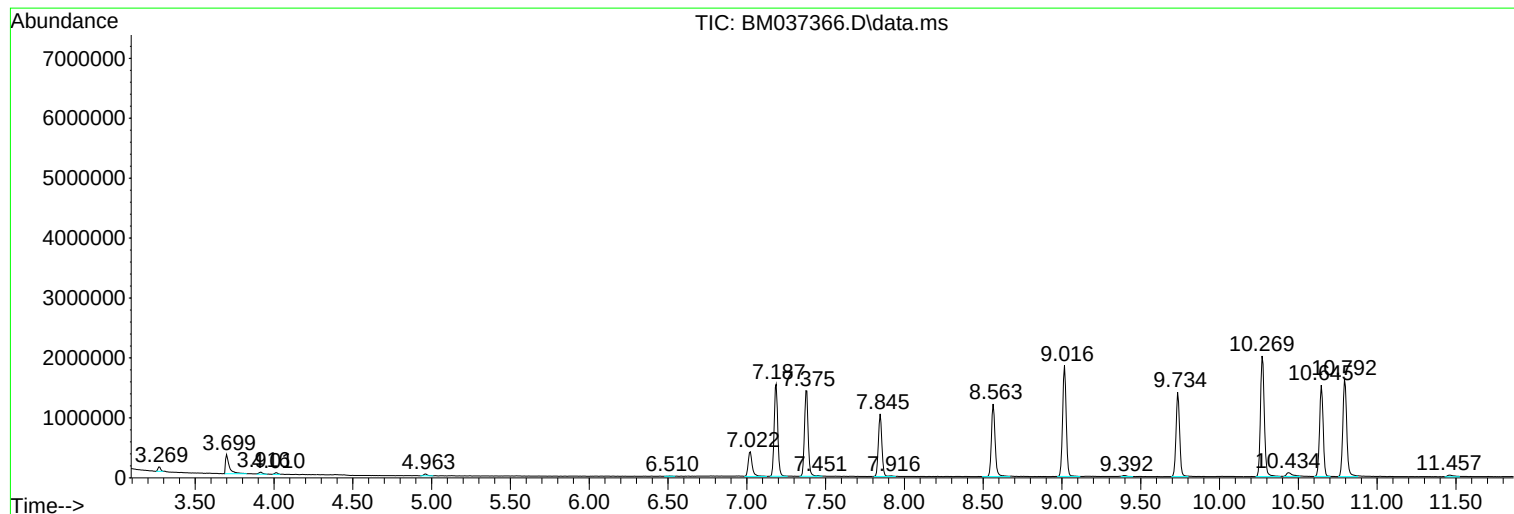

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037366.D
Acq On : 04 Nov 2022 03:20
Operator : CG/JU
Sample : N5276-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037366.D
Acq On : 04 Nov 2022 03:20
Operator : CG/JU
Sample : N5276-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
