

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037371.D
 Acq On : 04 Nov 2022 06:15
 Operator : CG/JU
 Sample : N5276-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rVB	77768	93255	0.88%	0.093%
2	3.699	101	104	119	rBV	300785	458110	4.33%	0.455%
3	3.916	137	141	146	rVB	34065	47253	0.45%	0.047%
4	4.010	153	157	168	rVB	36888	55910	0.53%	0.055%
5	4.957	315	318	323	rVB	12837	18707	0.18%	0.019%
6	7.016	663	668	682	rVB	468378	785586	7.42%	0.780%
7	7.181	690	696	709	rBV	1539293	2376397	22.44%	2.358%
8	7.375	722	729	739	rBV	1521554	2396614	22.63%	2.378%
9	7.845	802	809	817	rBV	1384077	2156117	20.36%	2.140%
10	7.910	817	820	825	rVB4	11431	16436	0.16%	0.016%
11	8.563	923	931	949	rBV	1330460	2154588	20.34%	2.138%
12	9.016	1000	1008	1022	rVV	1818322	2976403	28.11%	2.954%
13	9.133	1024	1028	1035	rVV5	13174	24692	0.23%	0.025%
14	9.392	1067	1072	1078	rVB2	16050	26935	0.25%	0.027%
15	9.733	1122	1130	1141	rBV	1464591	2370740	22.39%	2.353%
16	9.910	1155	1160	1169	rBV	19533	50430	0.48%	0.050%
17	10.269	1214	1221	1238	rBV	2204880	3638680	34.36%	3.611%
18	10.433	1243	1249	1263	rVV	131908	286395	2.70%	0.284%
19	10.645	1277	1285	1293	rBV	2047934	3343731	31.57%	3.318%
20	10.792	1302	1310	1323	rBV	1641539	2829024	26.71%	2.807%
21	11.310	1391	1398	1404	rVV	24101	46259	0.44%	0.046%
22	11.451	1415	1422	1427	rBV9	13415	30325	0.29%	0.030%
23	11.886	1491	1496	1504	rVB4	9811	15963	0.15%	0.016%
24	11.992	1509	1514	1517	rBV7	8023	13379	0.13%	0.013%
25	12.063	1520	1526	1534	rBV7	10099	22633	0.21%	0.022%
26	12.233	1549	1555	1565	rVB	39844	69376	0.66%	0.069%
27	13.086	1694	1700	1708	rVB10	7415	13926	0.13%	0.014%
28	13.298	1729	1736	1740	rVV8	8721	20306	0.19%	0.020%
29	13.374	1744	1749	1755	rVV3	33884	59575	0.56%	0.059%
30	13.451	1758	1762	1768	rVB4	10752	18403	0.17%	0.018%
31	13.898	1830	1838	1851	rBV	4191967	5705284	53.87%	5.662%
32	13.998	1851	1855	1862	rVB10	10046	21262	0.20%	0.021%
33	14.174	1874	1885	1895	rBV	5265069	7412222	69.99%	7.356%
34	14.286	1901	1904	1909	rVB5	11741	18913	0.18%	0.019%
35	14.480	1929	1937	1948	rBV	3258384	4538804	42.86%	4.504%
36	14.704	1969	1975	1994	rBV	318533	654252	6.18%	0.649%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
 Data File : BM037371.D
 Acq On : 04 Nov 2022 06:15
 Operator : CG/JU
 Sample : N5276-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4X9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
 Title : SVOA CALIBRATION

37	14.851	1997	2000	2004	rBV6	12924	17911	0.17%	0.018%
38	14.980	2021	2022	2030	rVB8	8305	12759	0.12%	0.013%
39	15.227	2061	2064	2068	rBV4	8458	11884	0.11%	0.012%
40	15.274	2068	2072	2073	rVV	20398	27892	0.26%	0.028%
41	15.304	2073	2077	2084	rVB	101770	147880	1.40%	0.147%
42	15.474	2095	2106	2119	rBV	6698427	9416715	88.92%	9.345%
43	15.598	2121	2127	2139	rVV	2080648	2699995	25.50%	2.679%
44	15.710	2142	2146	2151	rVB2	33485	53939	0.51%	0.054%
45	15.921	2179	2182	2188	rVB8	10022	16390	0.15%	0.016%
46	16.045	2197	2203	2208	rBV9	8081	16393	0.15%	0.016%
47	16.180	2222	2226	2234	rVB9	11479	22322	0.21%	0.022%
48	16.251	2234	2238	2242	rBV6	10399	14481	0.14%	0.014%
49	16.368	2253	2258	2261	rBV7	8126	12961	0.12%	0.013%
50	16.627	2298	2302	2306	rBV7	10939	16512	0.16%	0.016%
51	16.674	2306	2310	2312	rBV5	8861	11627	0.11%	0.012%
52	16.733	2316	2320	2322	rBV3	10216	12807	0.12%	0.013%
53	17.133	2385	2388	2392	rBV6	12751	16487	0.16%	0.016%
54	17.221	2396	2403	2409	rBV	3620637	4936901	46.62%	4.899%
55	17.321	2413	2420	2440	rVV	7177082	10004479	94.47%	9.928%
56	17.504	2447	2451	2456	rVB	29153	40003	0.38%	0.040%
57	17.615	2465	2470	2476	rBV7	19126	42663	0.40%	0.042%
58	17.886	2512	2516	2521	rVB2	48269	59179	0.56%	0.059%
59	18.109	2550	2554	2563	rBV	206027	317112	2.99%	0.315%
60	18.874	2680	2684	2687	rBV	143410	223988	2.12%	0.222%
61	19.174	2731	2735	2741	rVB	79373	110408	1.04%	0.110%
62	19.245	2743	2747	2753	rBV	84920	131112	1.24%	0.130%
63	19.386	2768	2771	2777	rBV	98450	135049	1.28%	0.134%
64	19.609	2803	2809	2820	rBV	8508656	10590264	100.00%	10.509%
65	21.115	3061	3065	3074	rBV2	202585	351354	3.32%	0.349%
66	21.392	3107	3112	3118	rBV	3634375	4294835	40.55%	4.262%
67	23.585	3478	3485	3495	rVB2	4485238	8301875	78.39%	8.239%
68	23.733	3504	3510	3520	rVB2	2014370	3933661	37.14%	3.904%




Sum of corrected areas: 100768723

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037371.D
Acq On : 04 Nov 2022 06:15
Operator : CG/JU
Sample : N5276-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

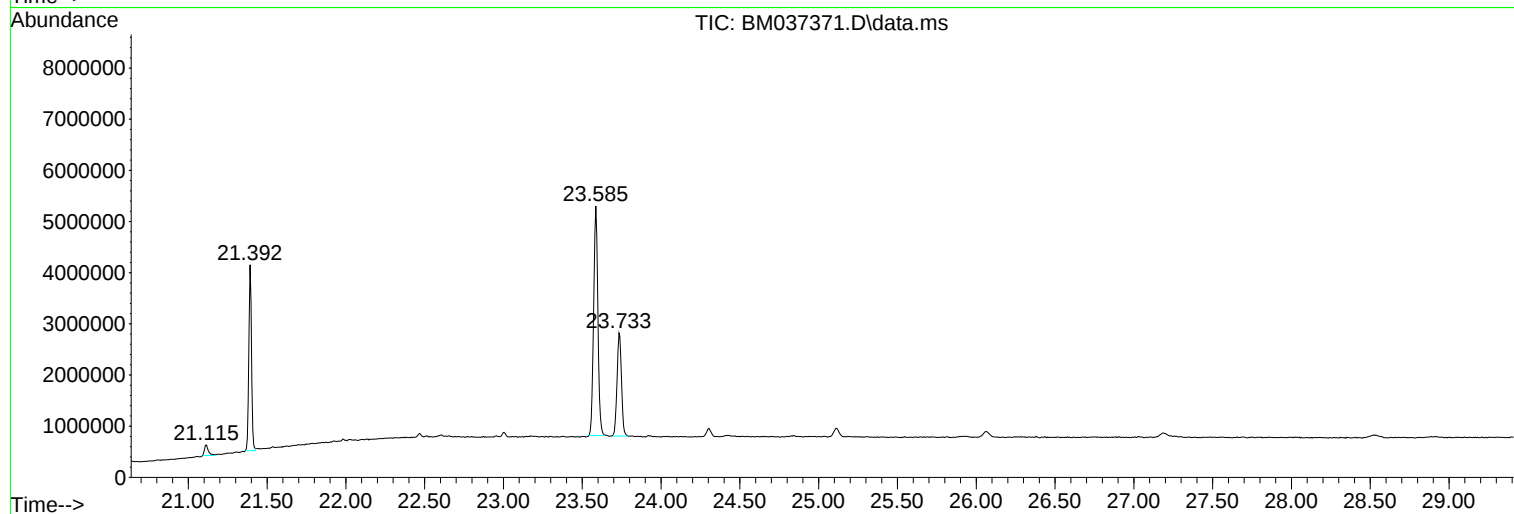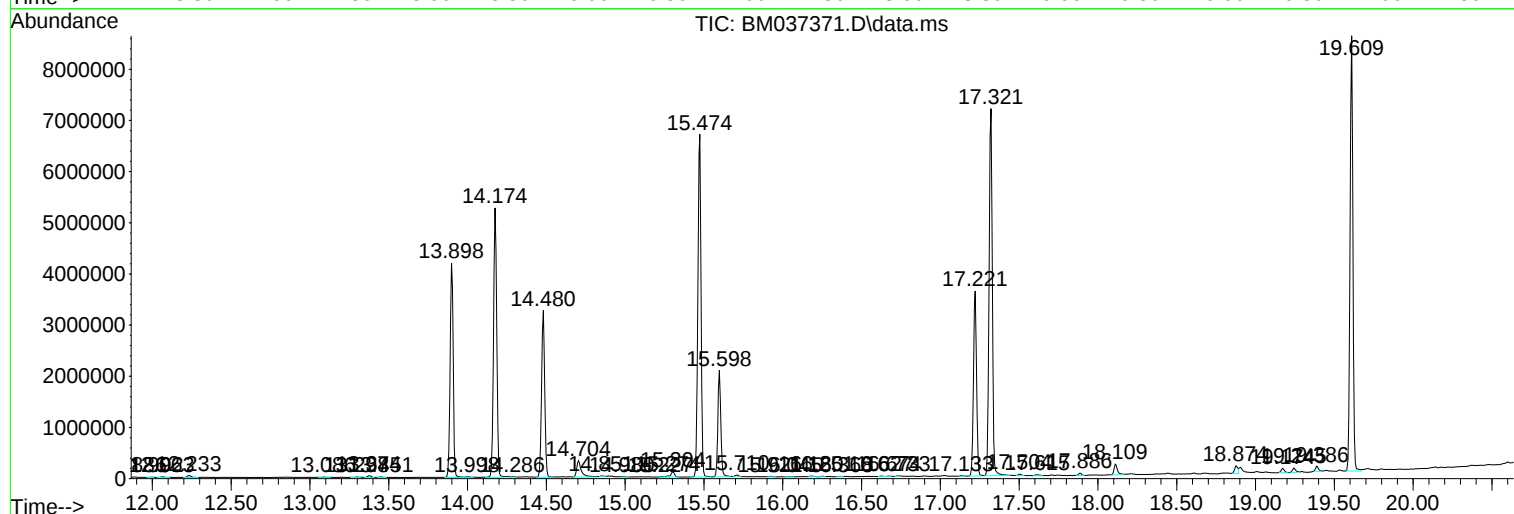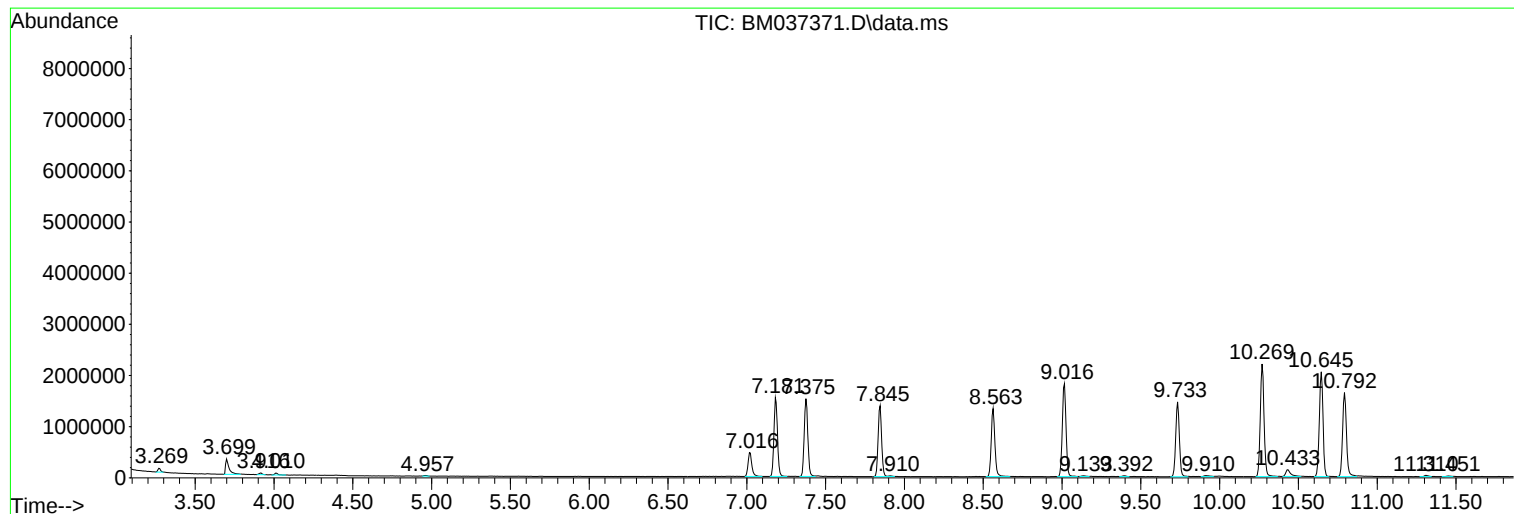

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037371.D
Acq On : 04 Nov 2022 06:15
Operator : CG/JU
Sample : N5276-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110322\
Data File : BM037371.D
Acq On : 04 Nov 2022 06:15
Operator : CG/JU
Sample : N5276-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4X9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
