



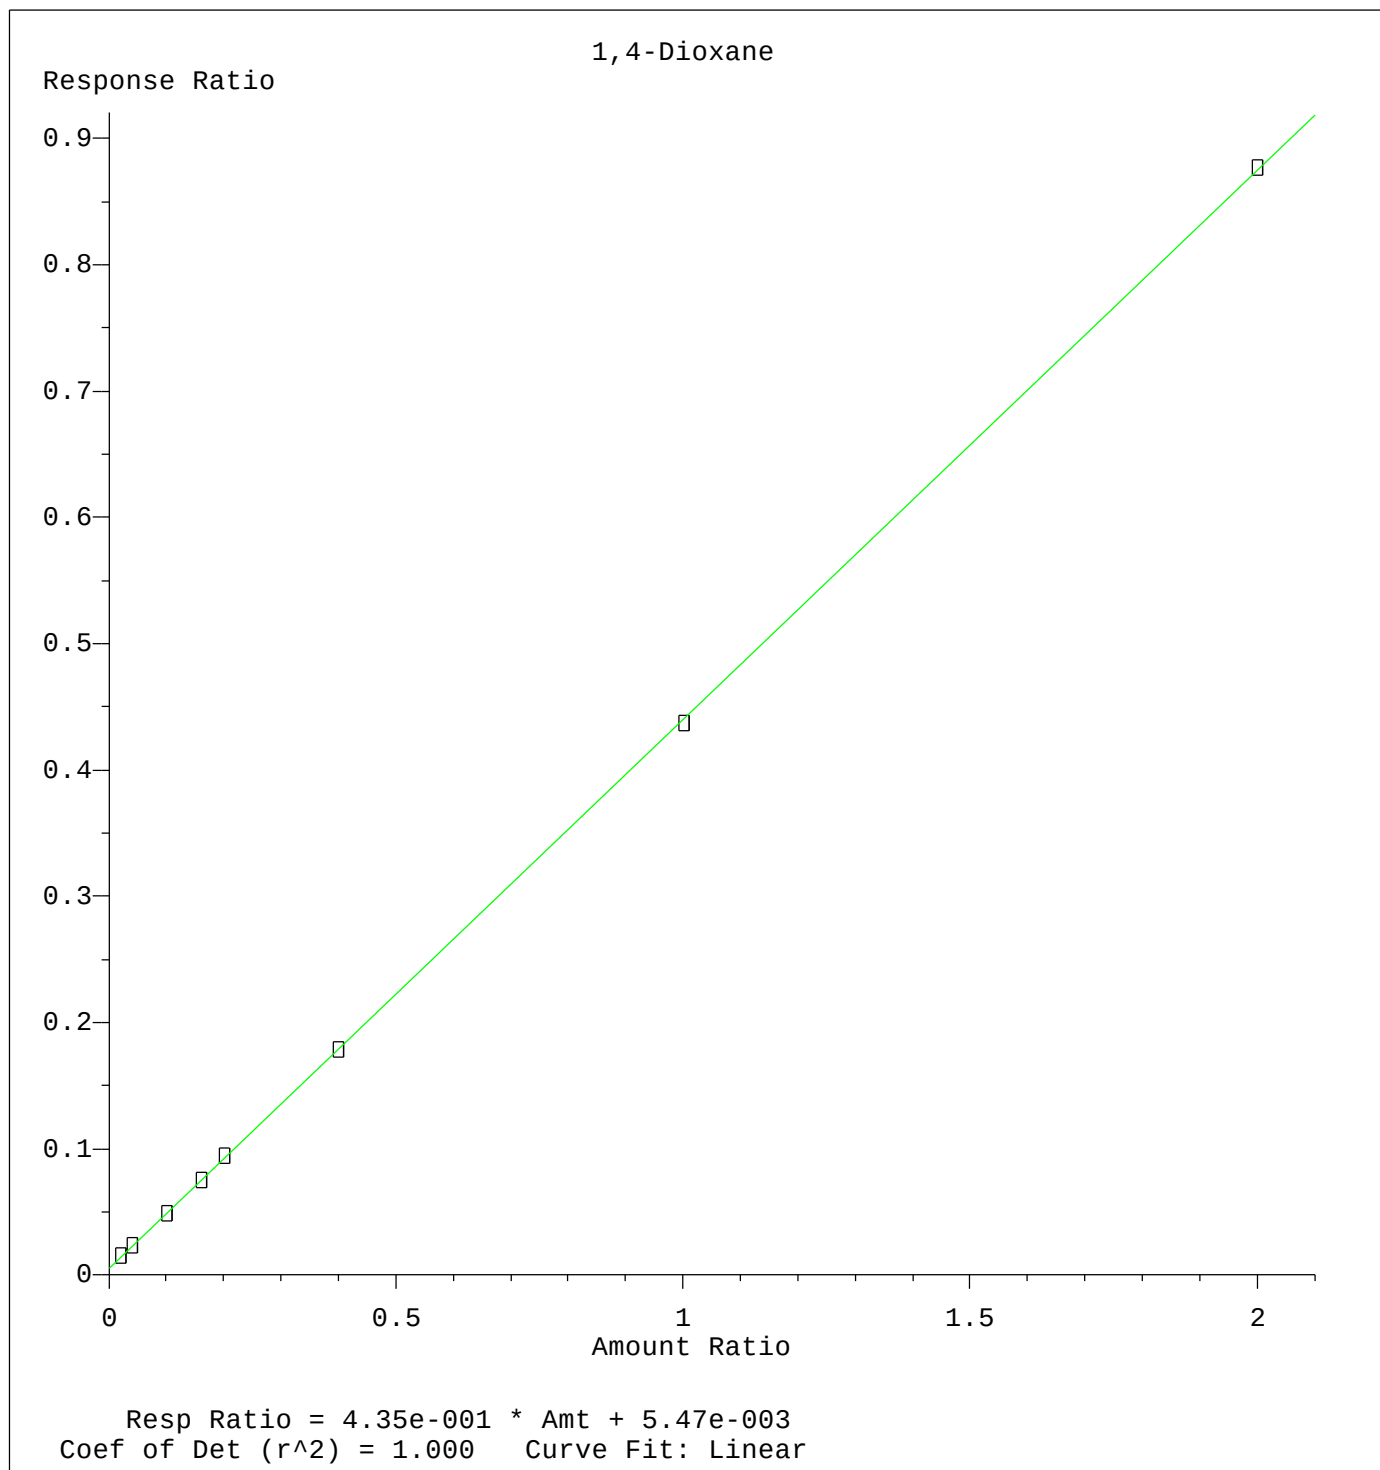

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:21:55 2015


4-Bromophenyl-phenylether

Response Ratio

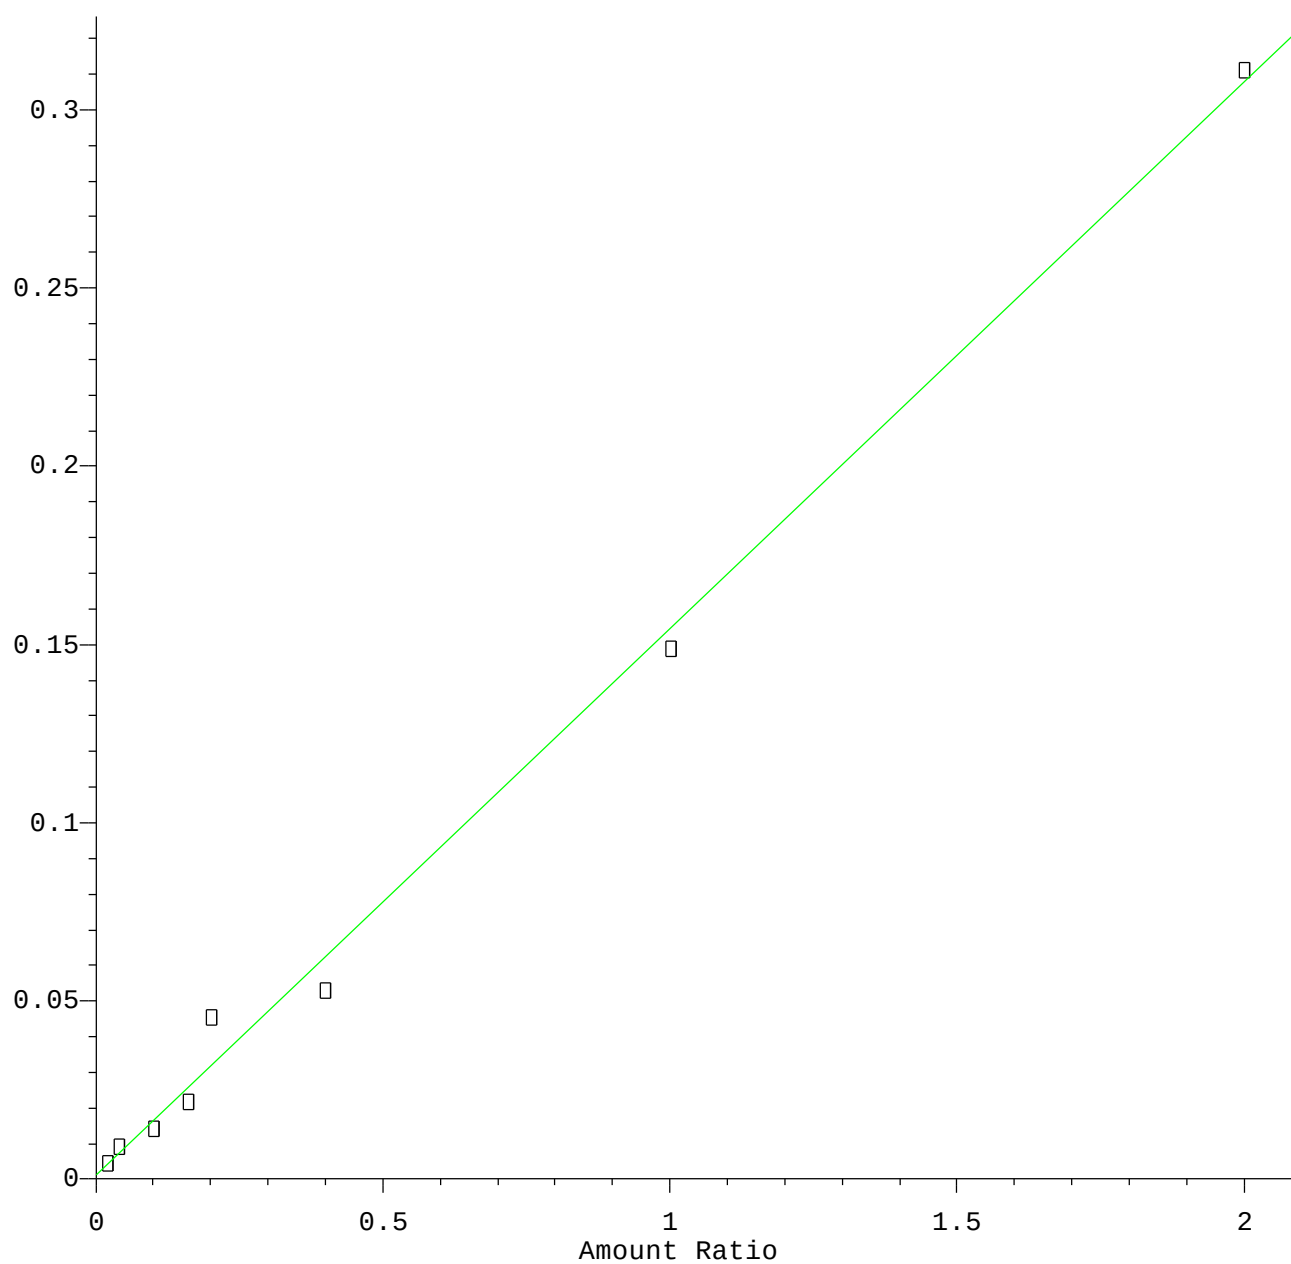


Resp Ratio = $1.53 \times 10^{-1} \times \text{Amt} + 6.78 \times 10^{-4}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:21:55 2015

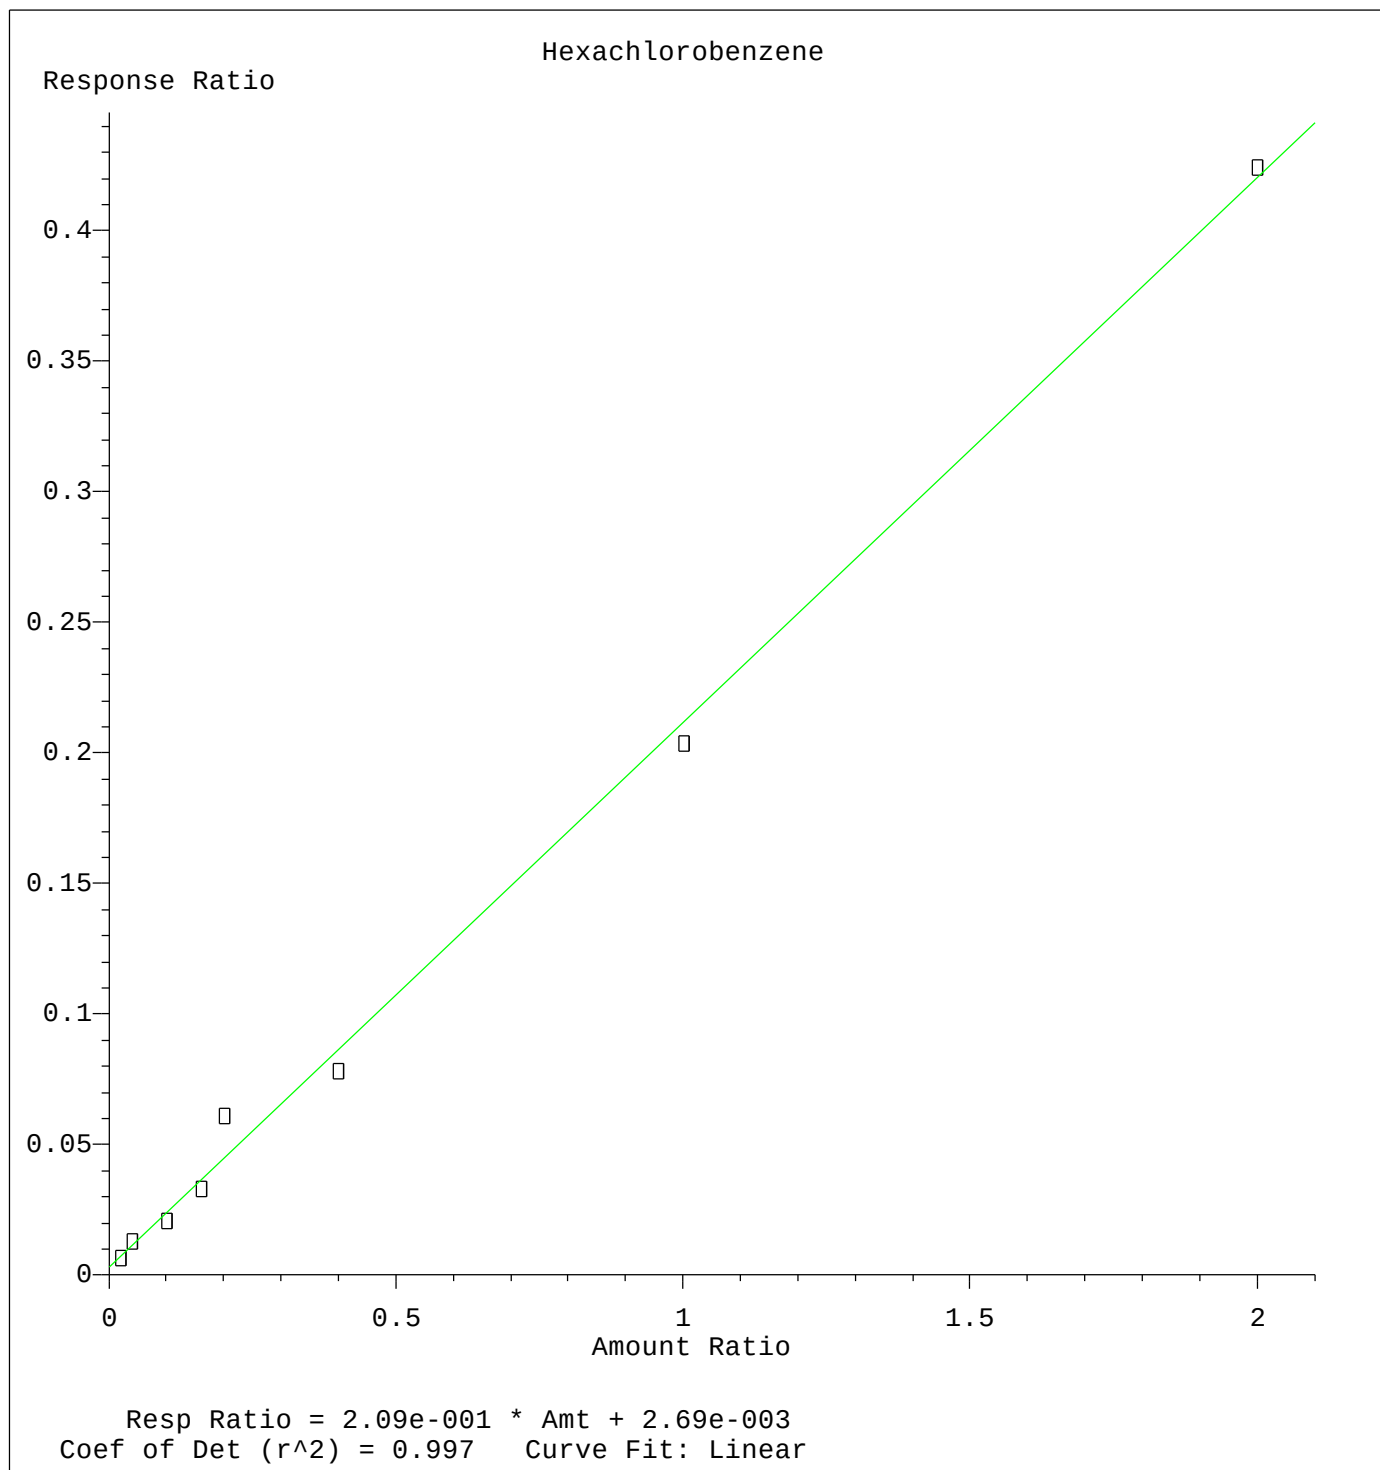


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:24:03 2015

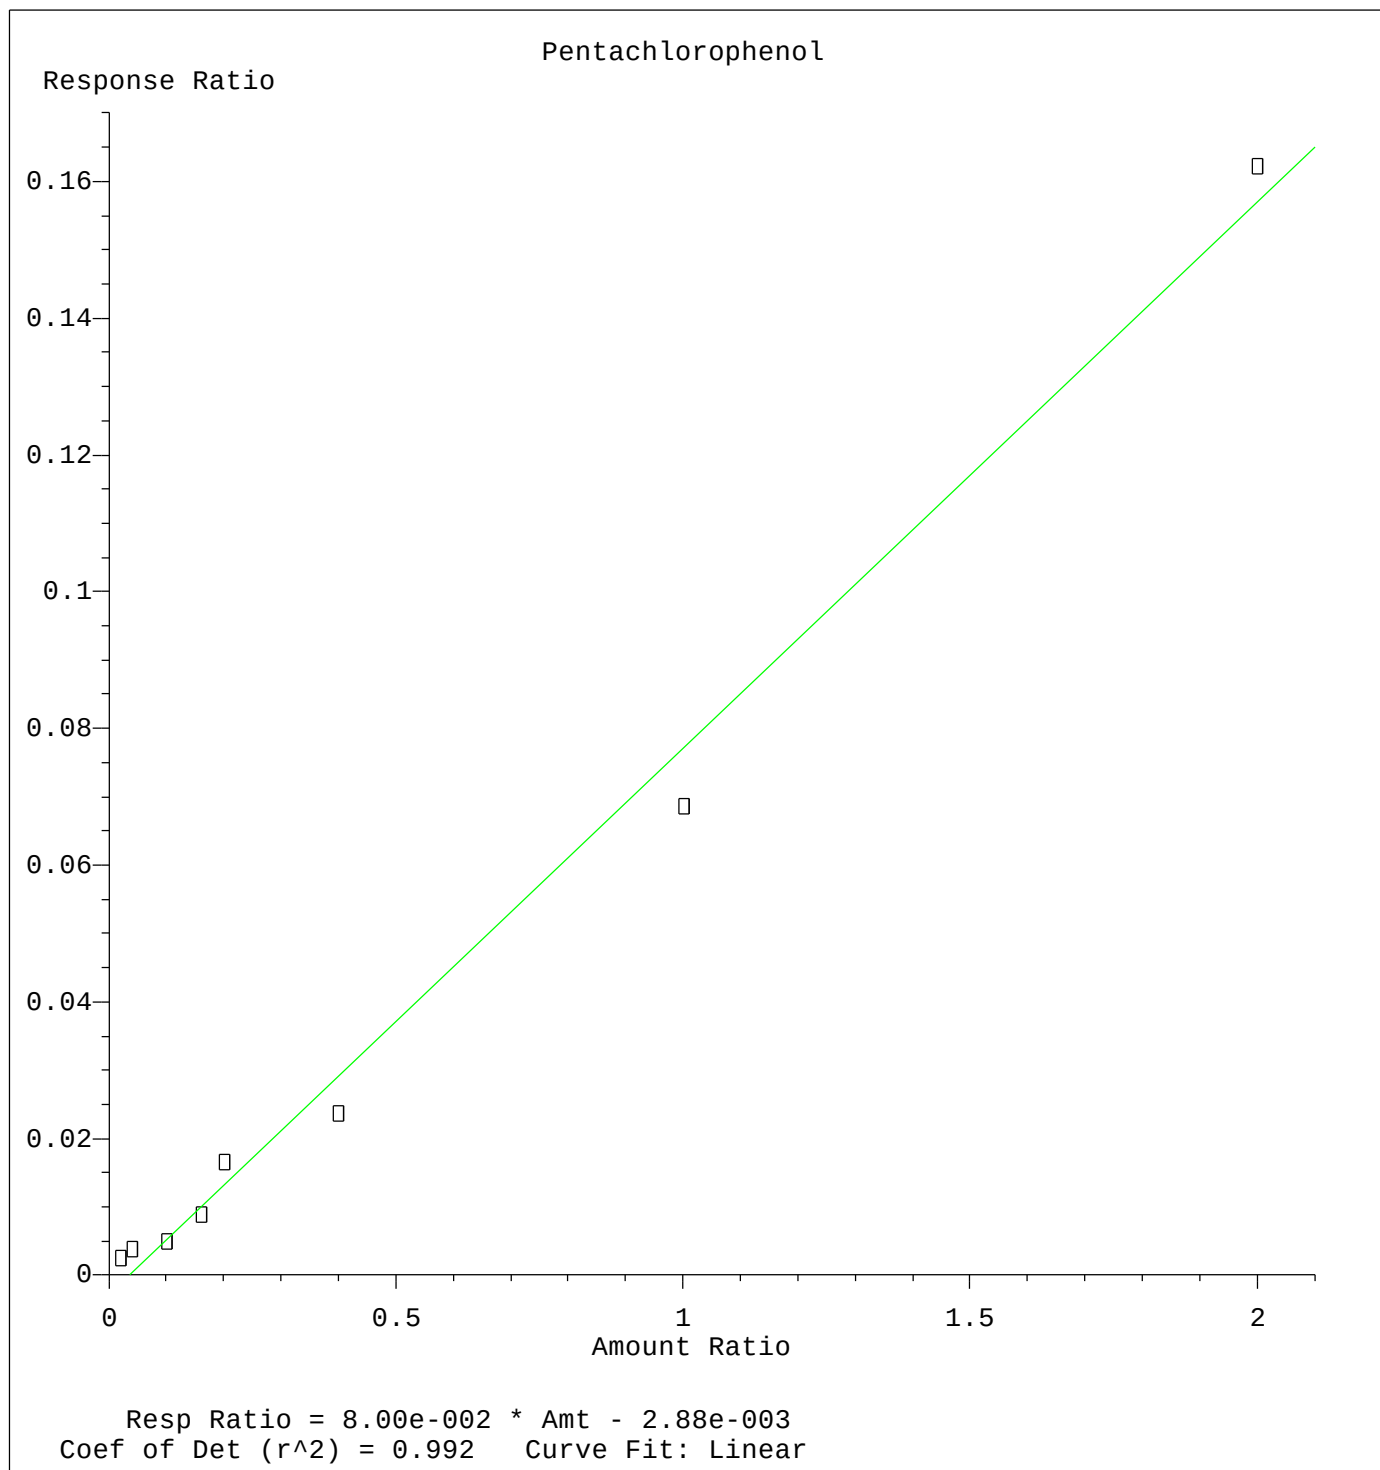


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:24:13 2015

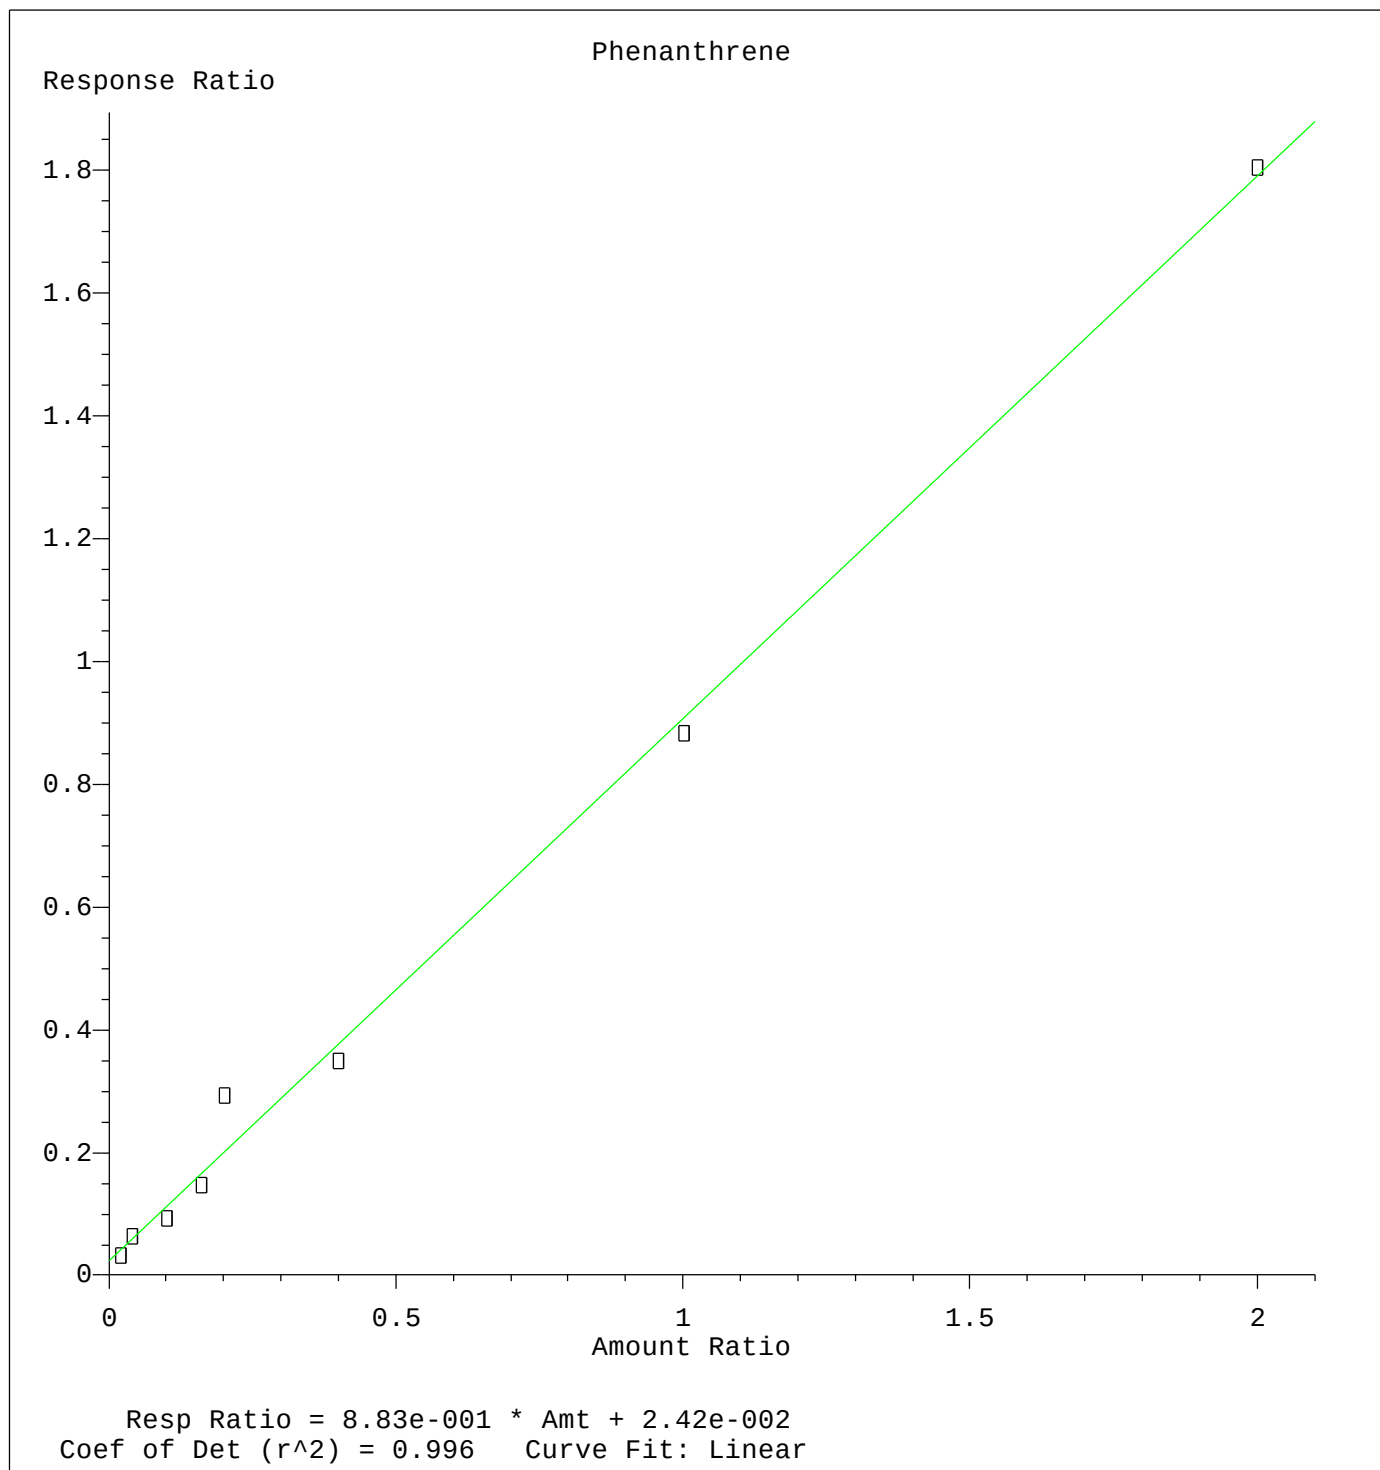


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:24:31 2015

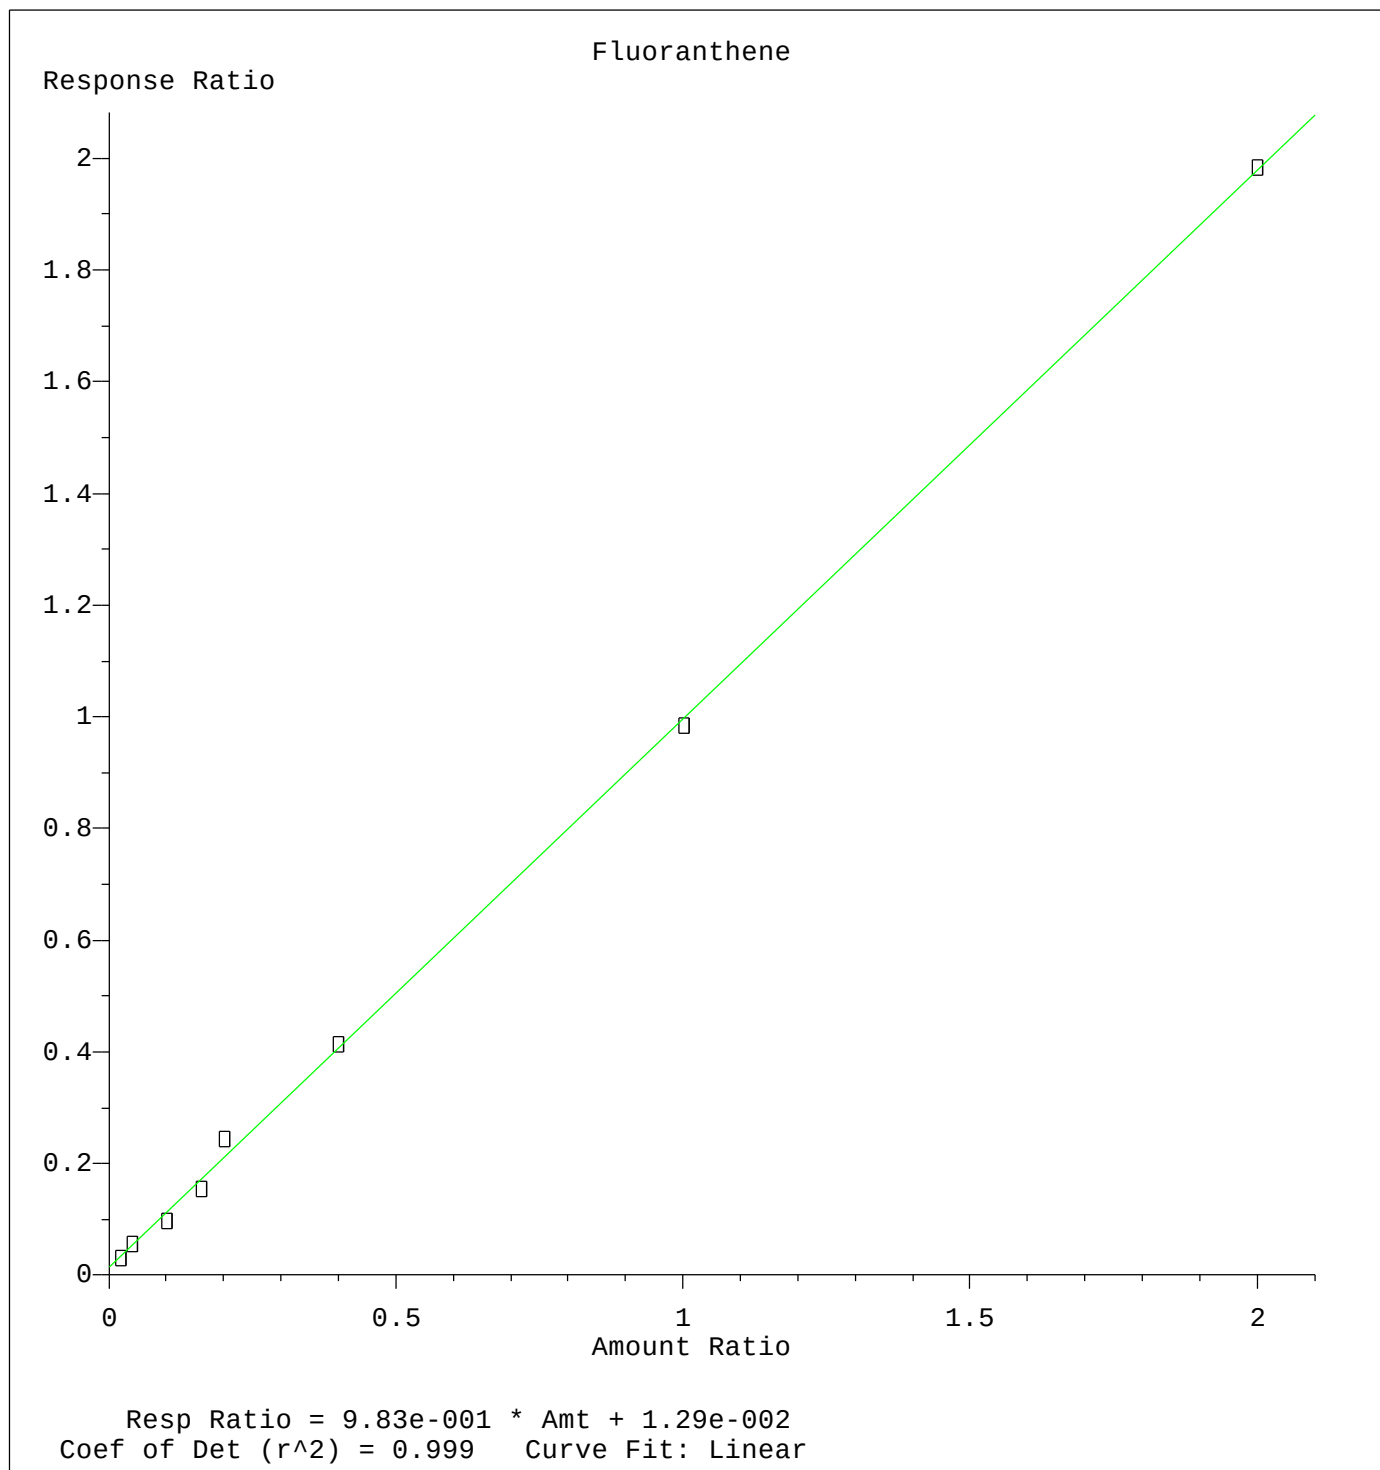

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:24:45 2015

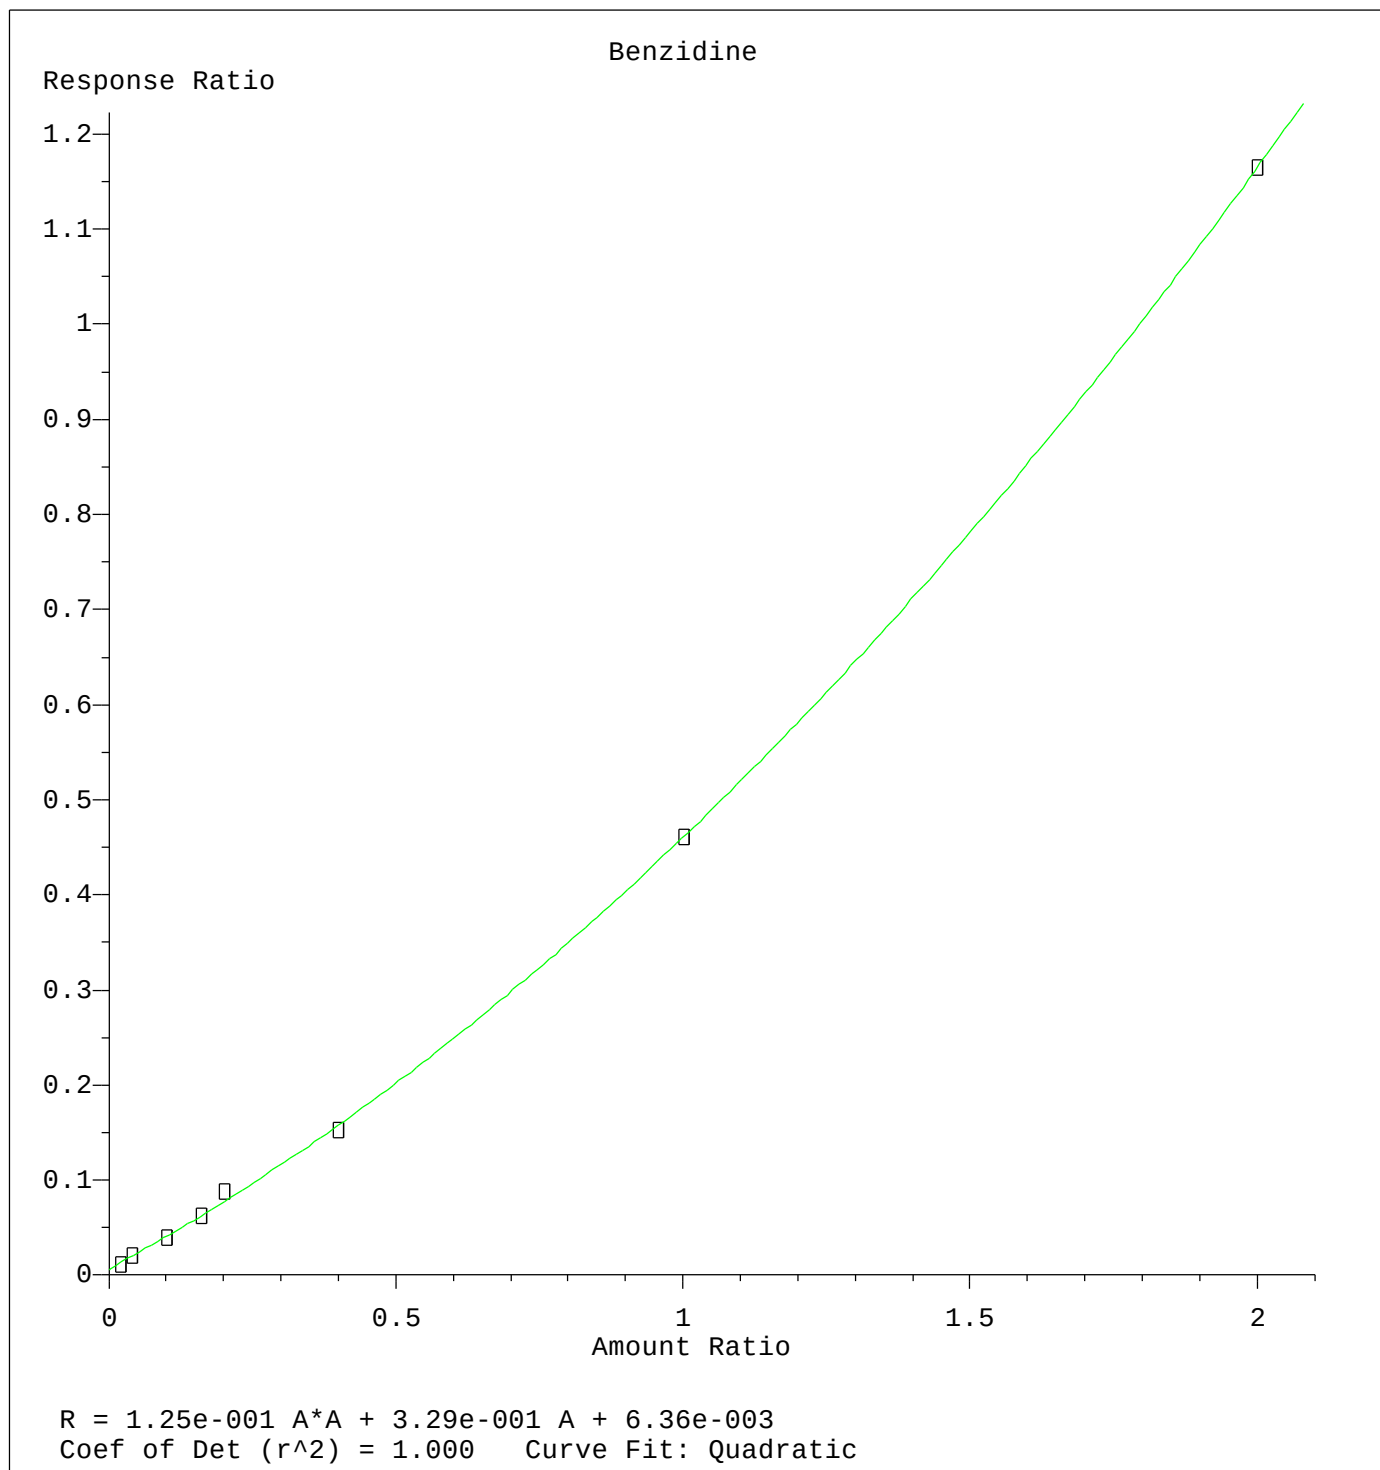


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:25:59 2015

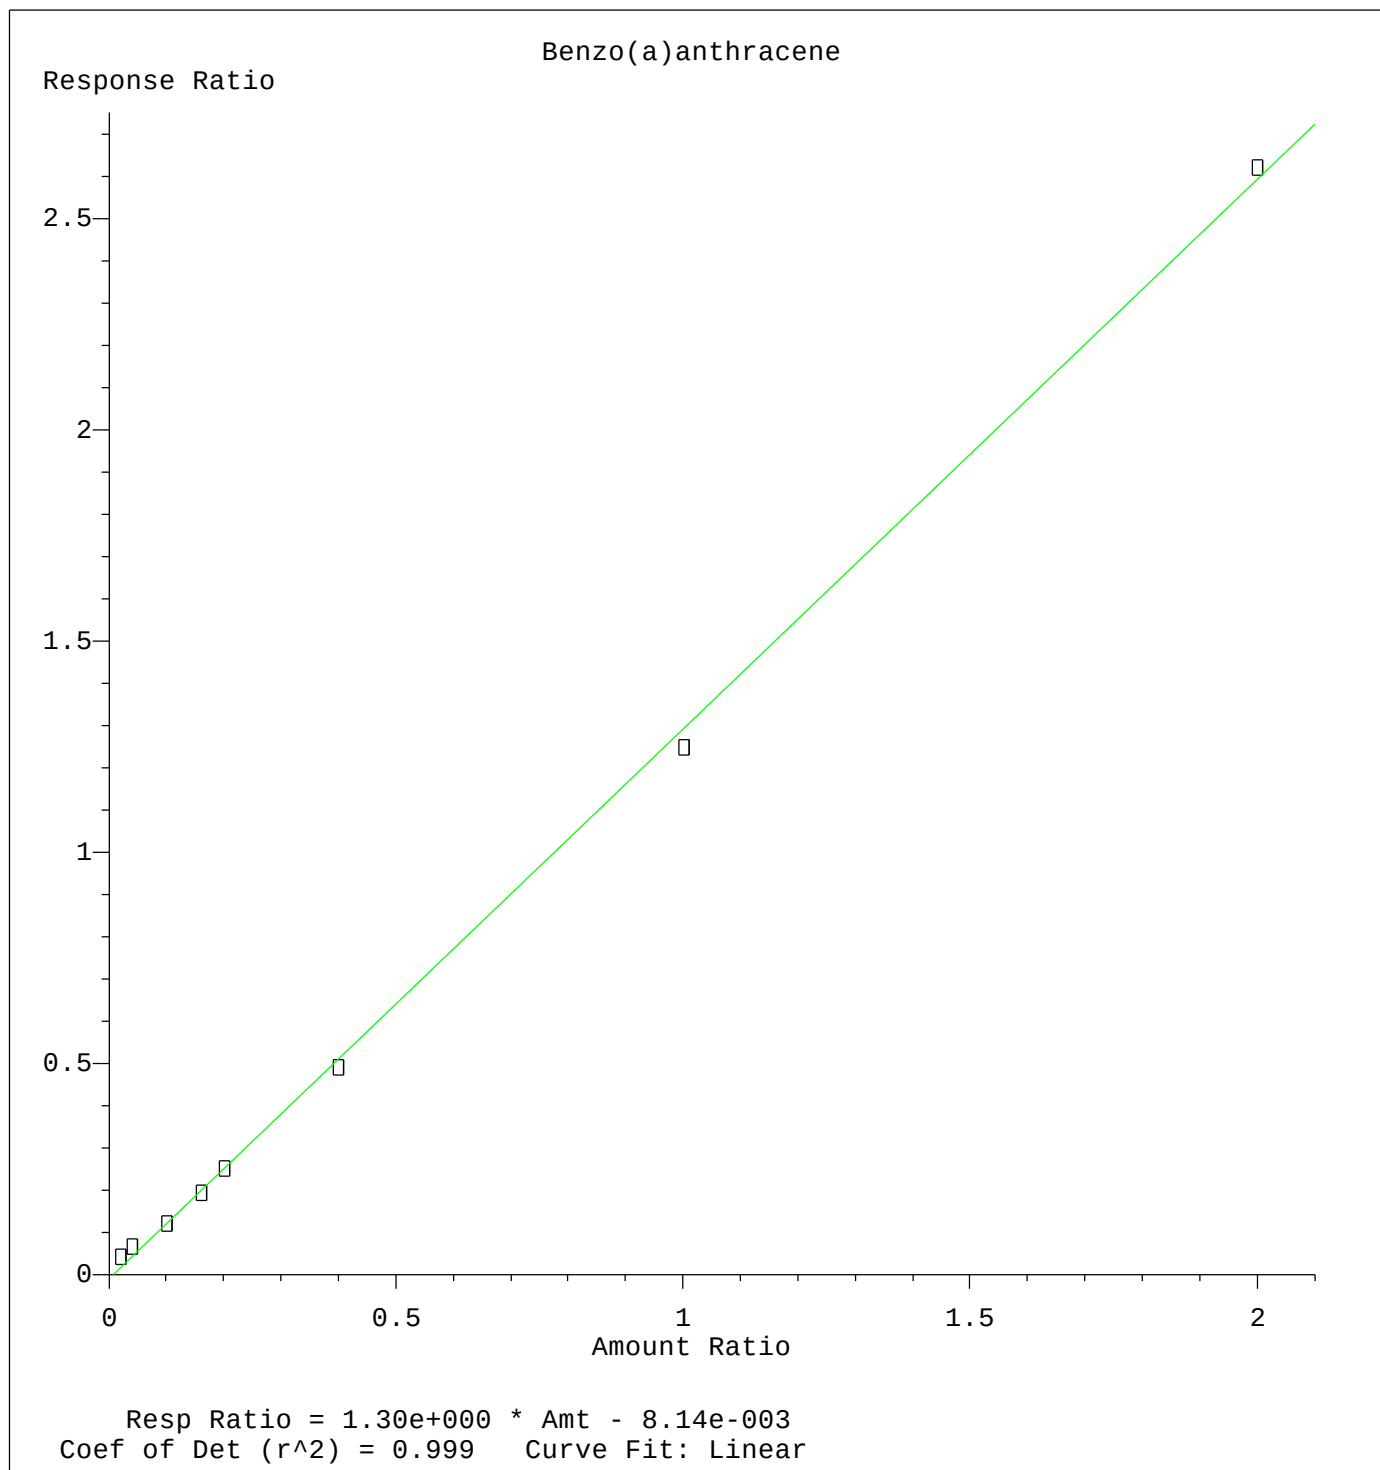

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:26:21 2015


3,3'-Dichlorobenzidine

Response Ratio

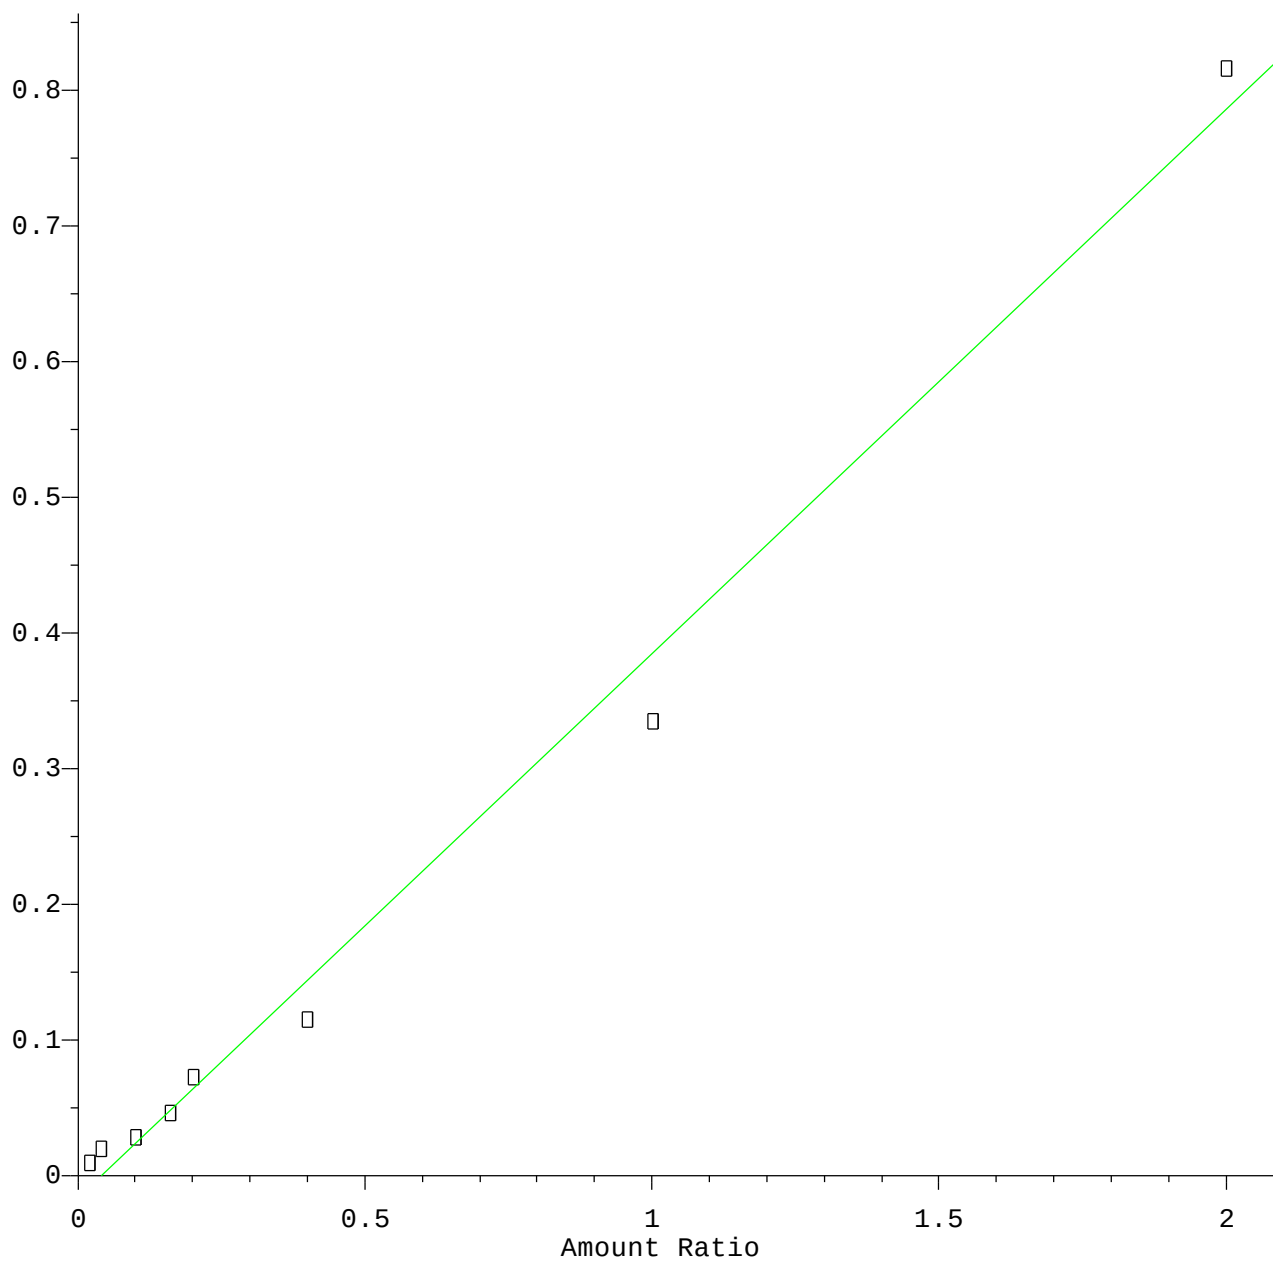

Resp Ratio = $4.01 \times 10^{-1} \times \text{Amt} - 1.64 \times 10^{-2}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:26:32 2015

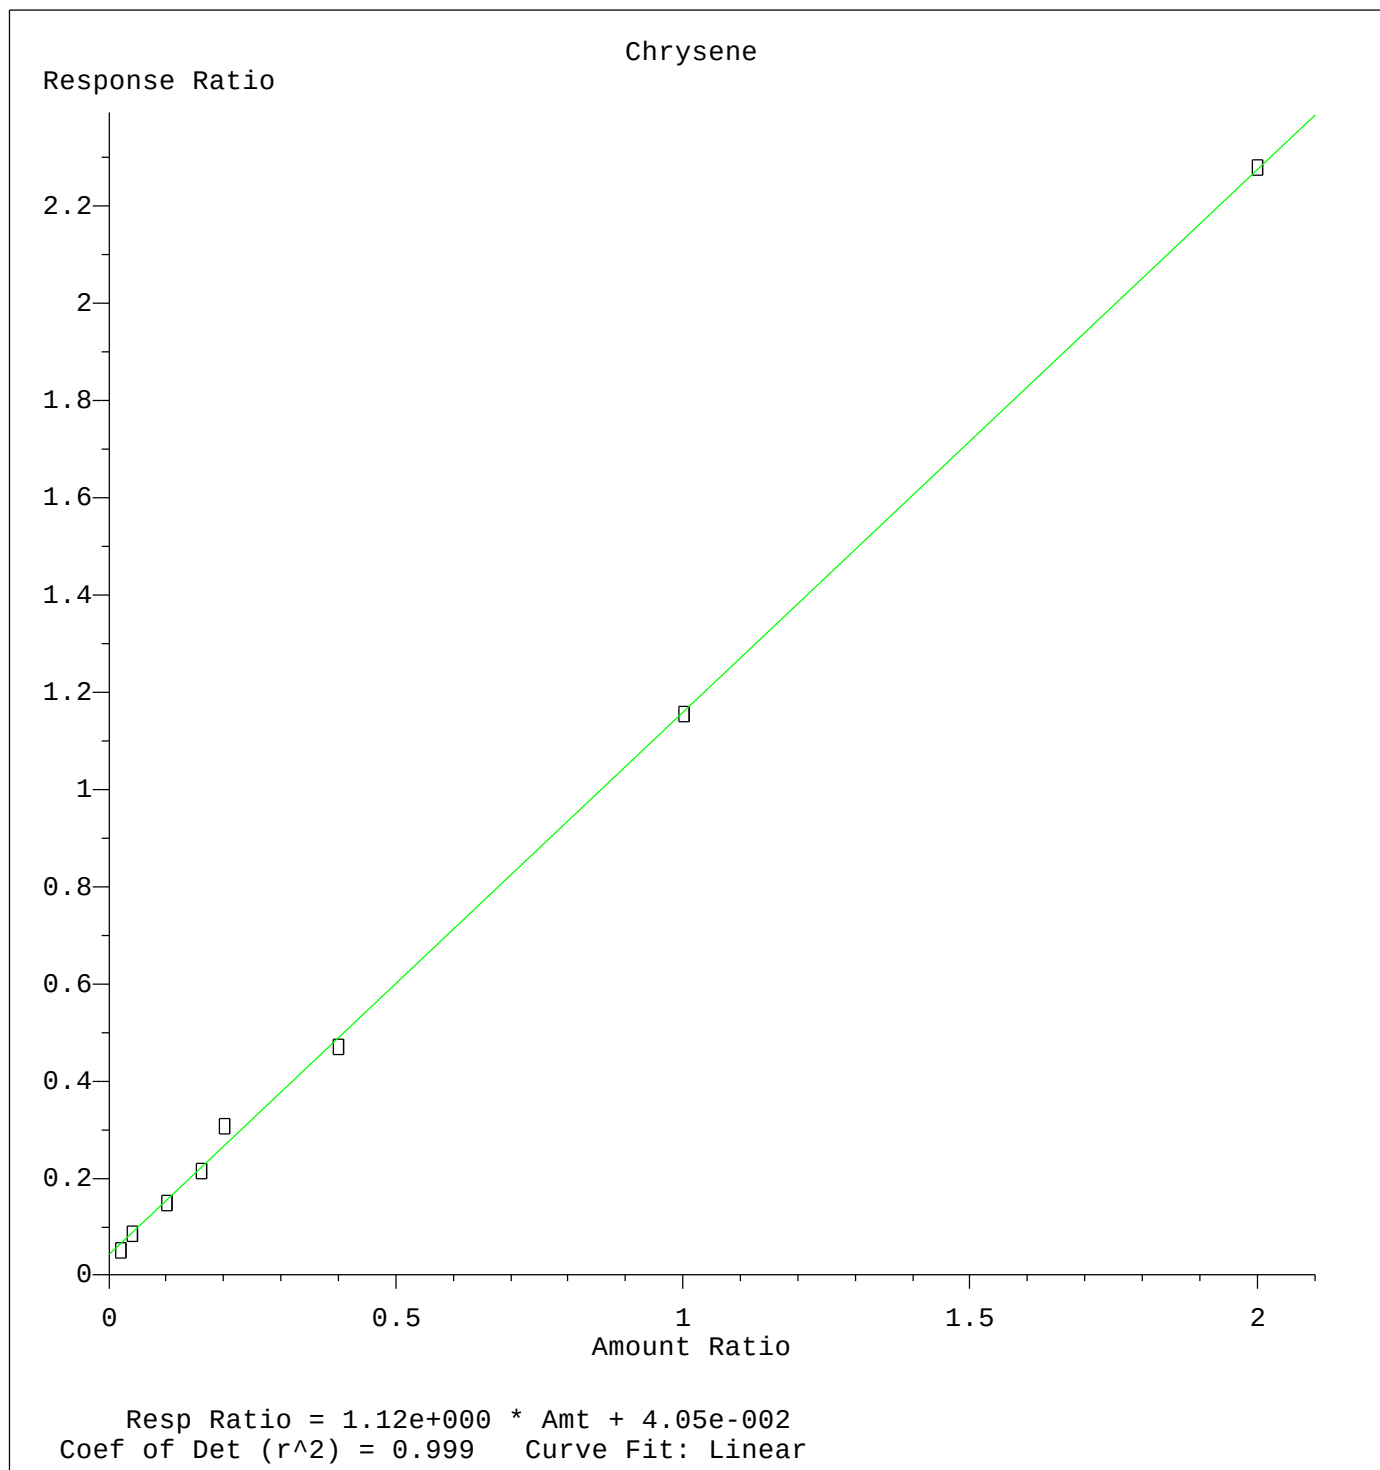

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:26:49 2015


Bis(2-ethylhexyl)phthalate

Response Ratio

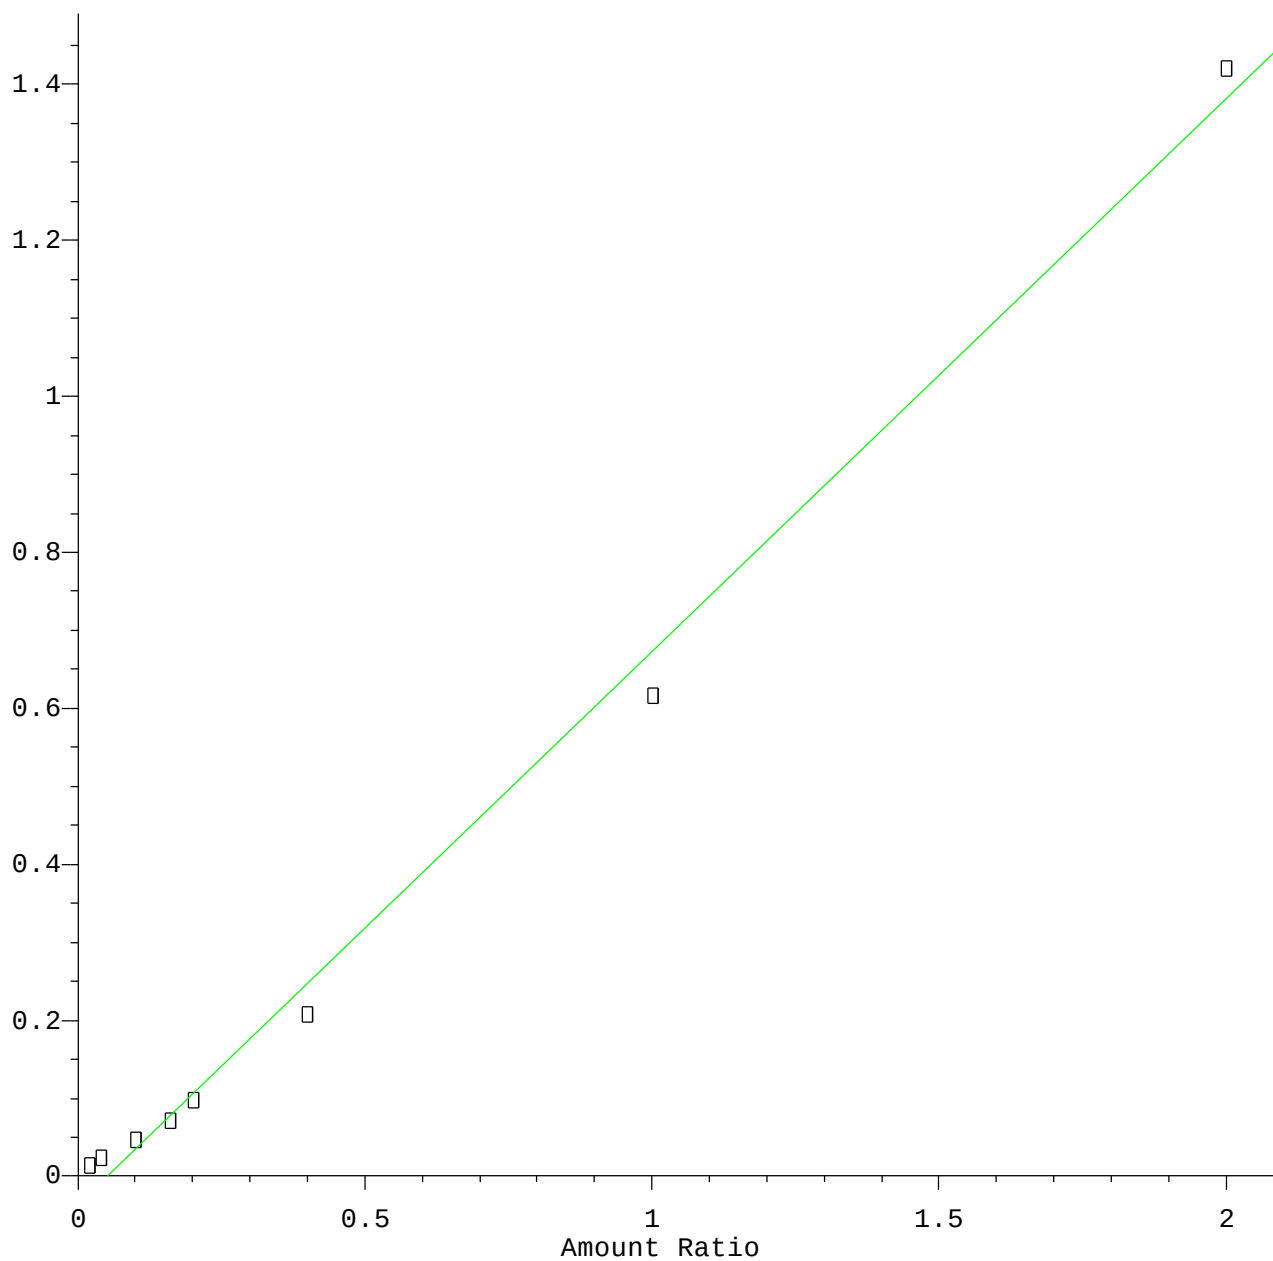


Resp Ratio = $7.09 \times 10^{-1} \times \text{Amt} - 3.62 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:27:05 2015

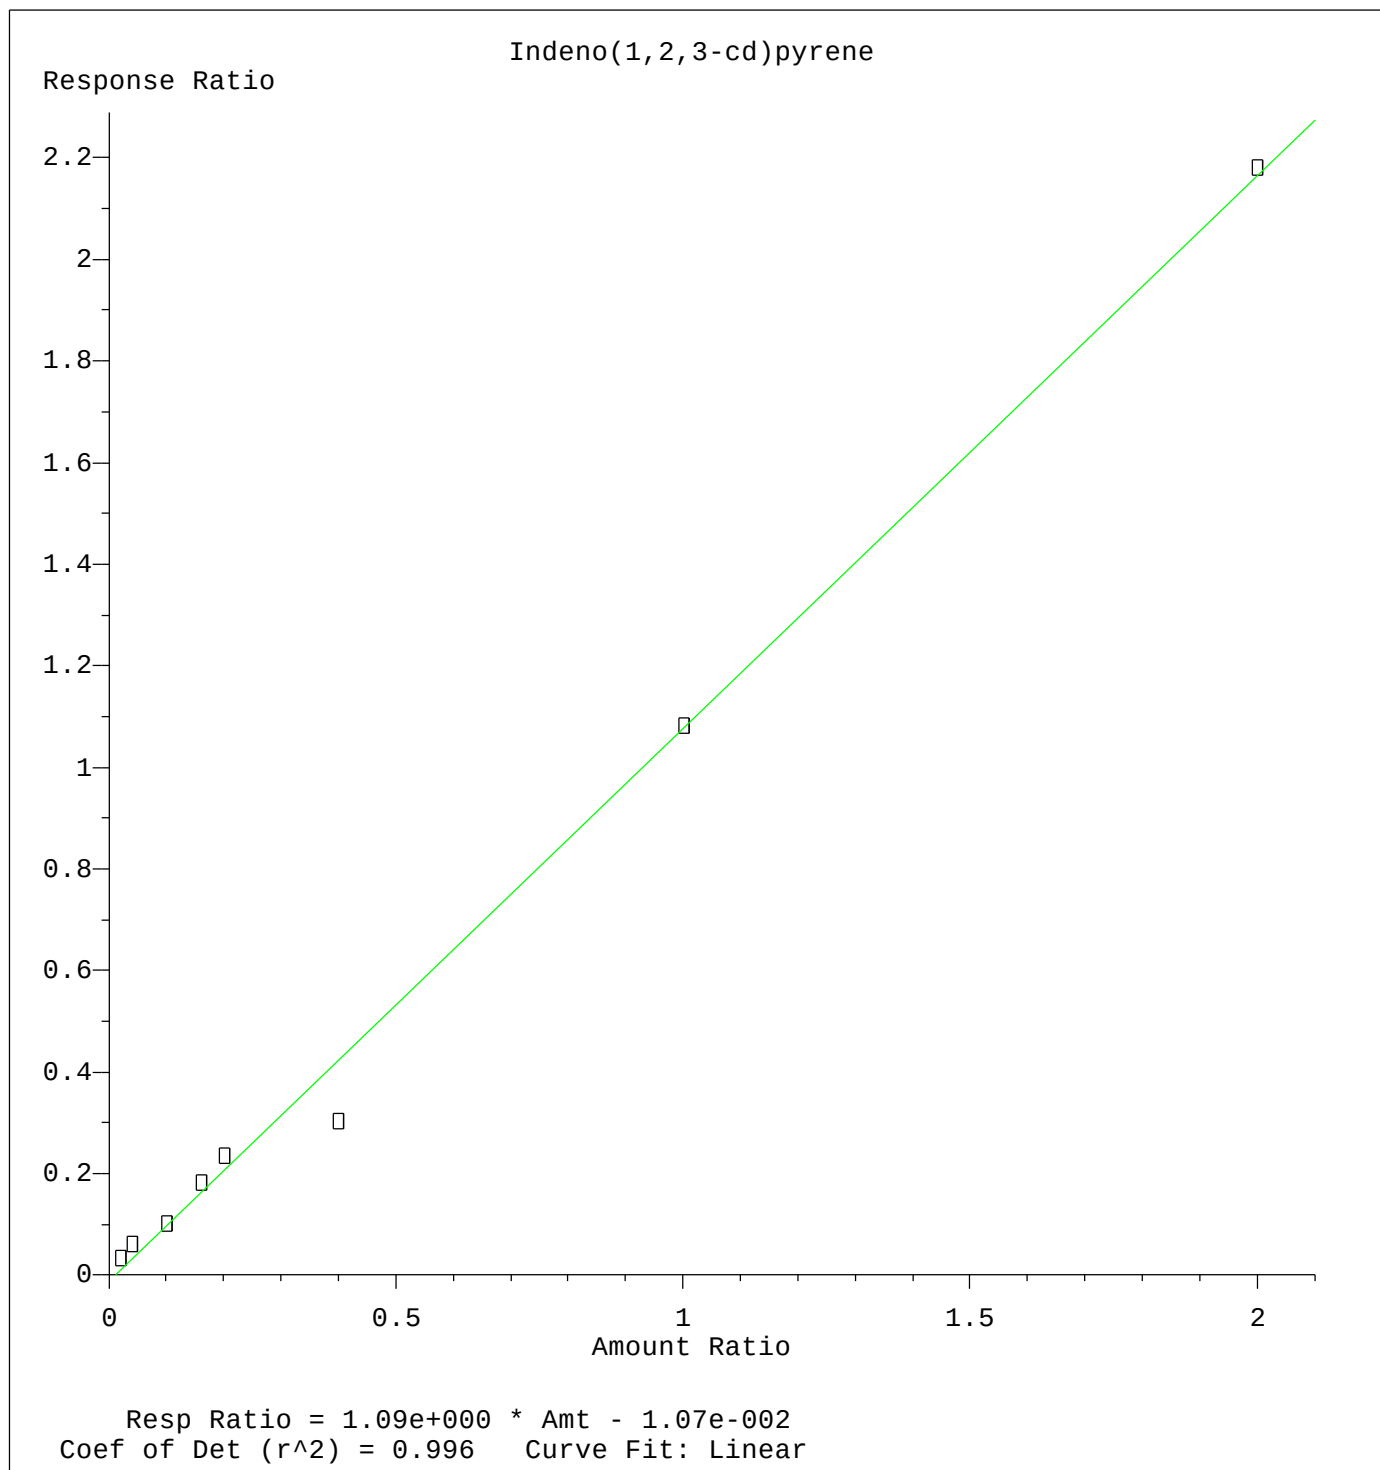

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:27:21 2015

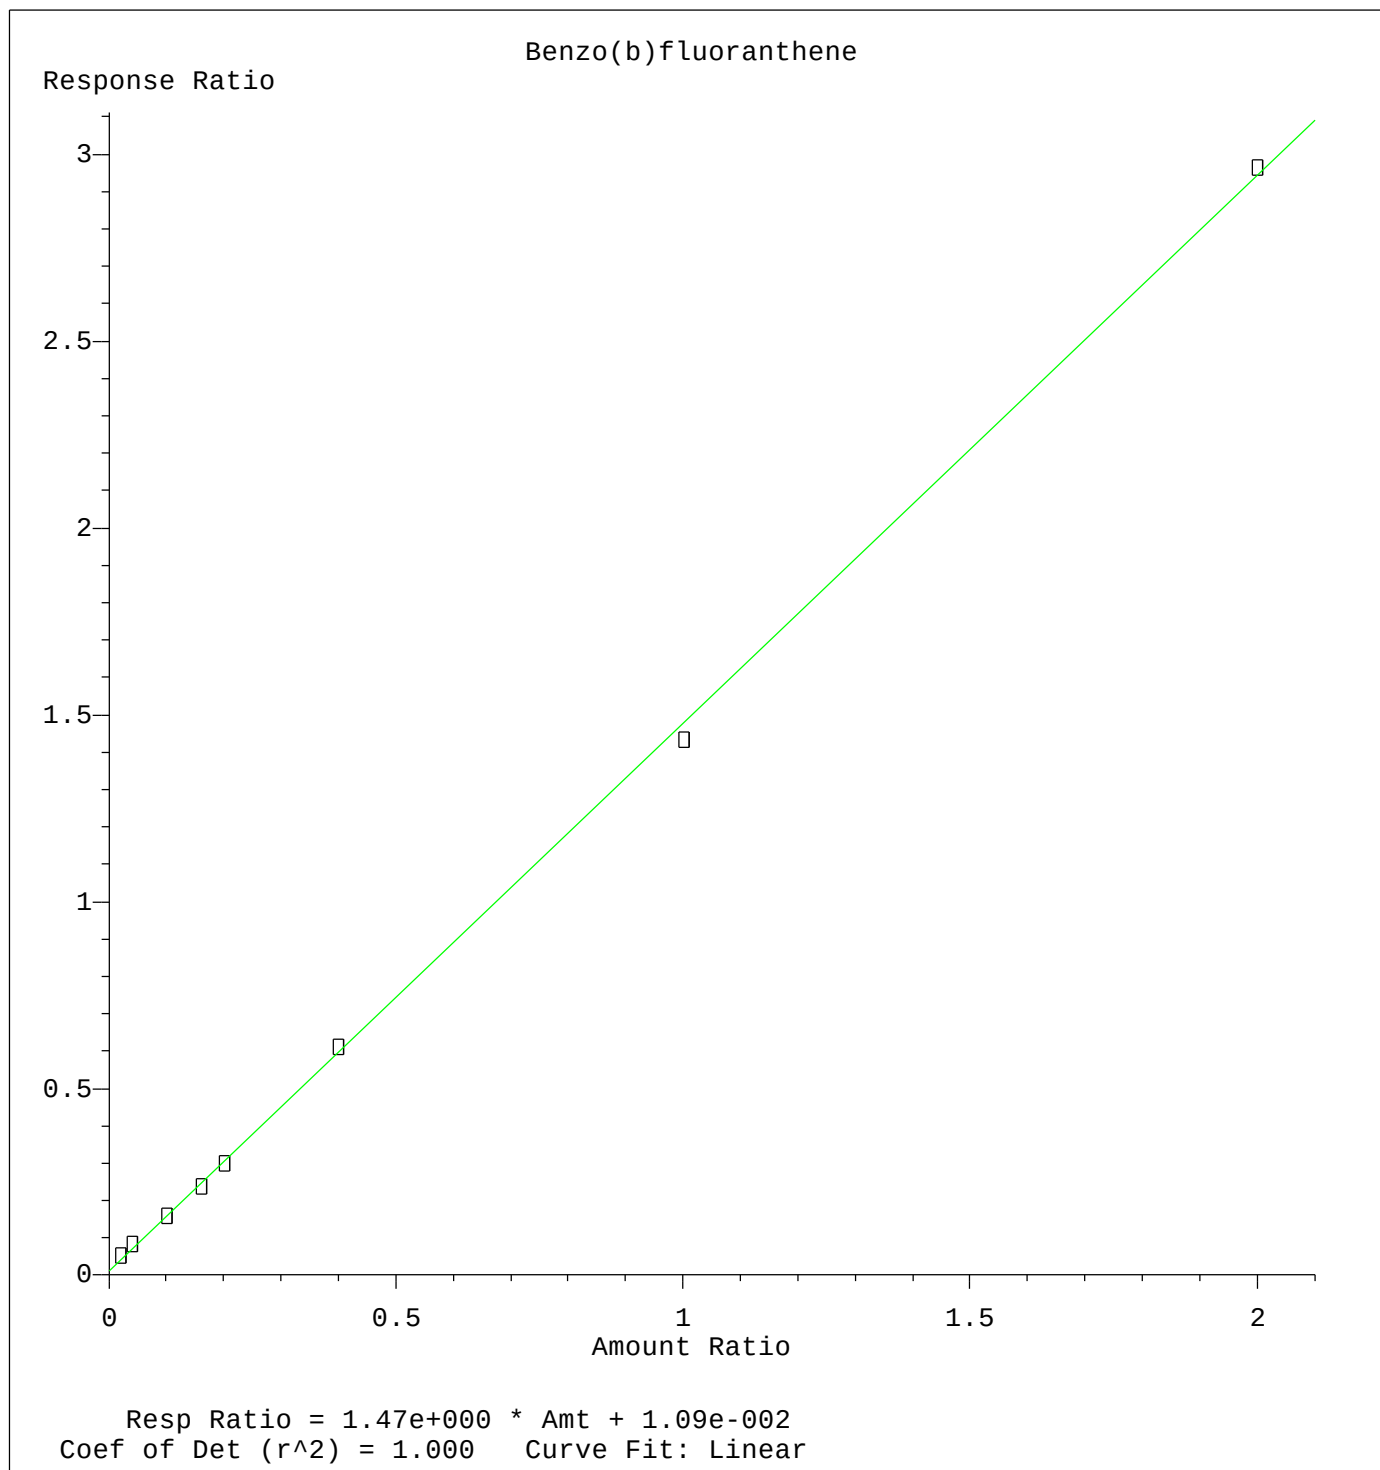

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:27:37 2015

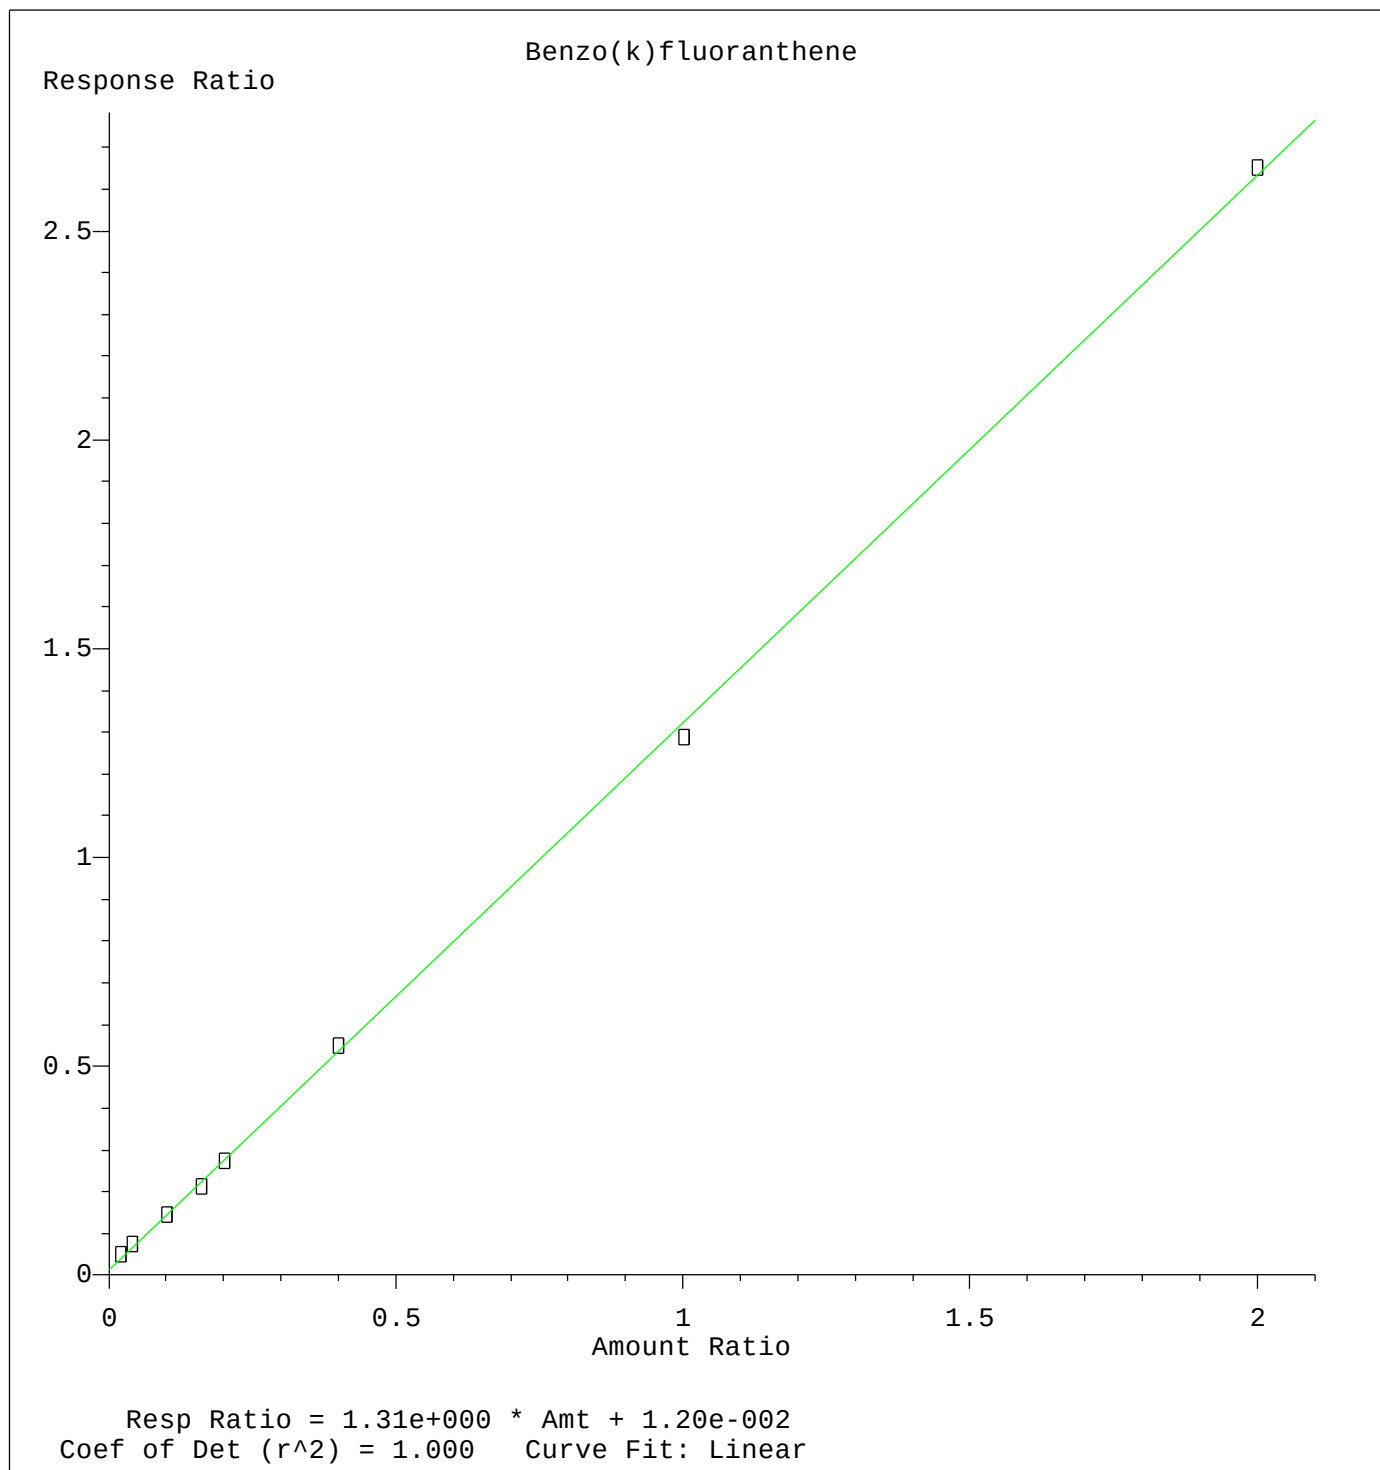

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
Calibration Table Last Updated: Thu Nov 05 10:28:56 2015