


Data Path : Z:\HPCHEM1\BNA M\Data\BM110415\
 Data File : BM003047.D
 Acq On : 04 Nov 2015 17:23
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 05 10:29:18 2015

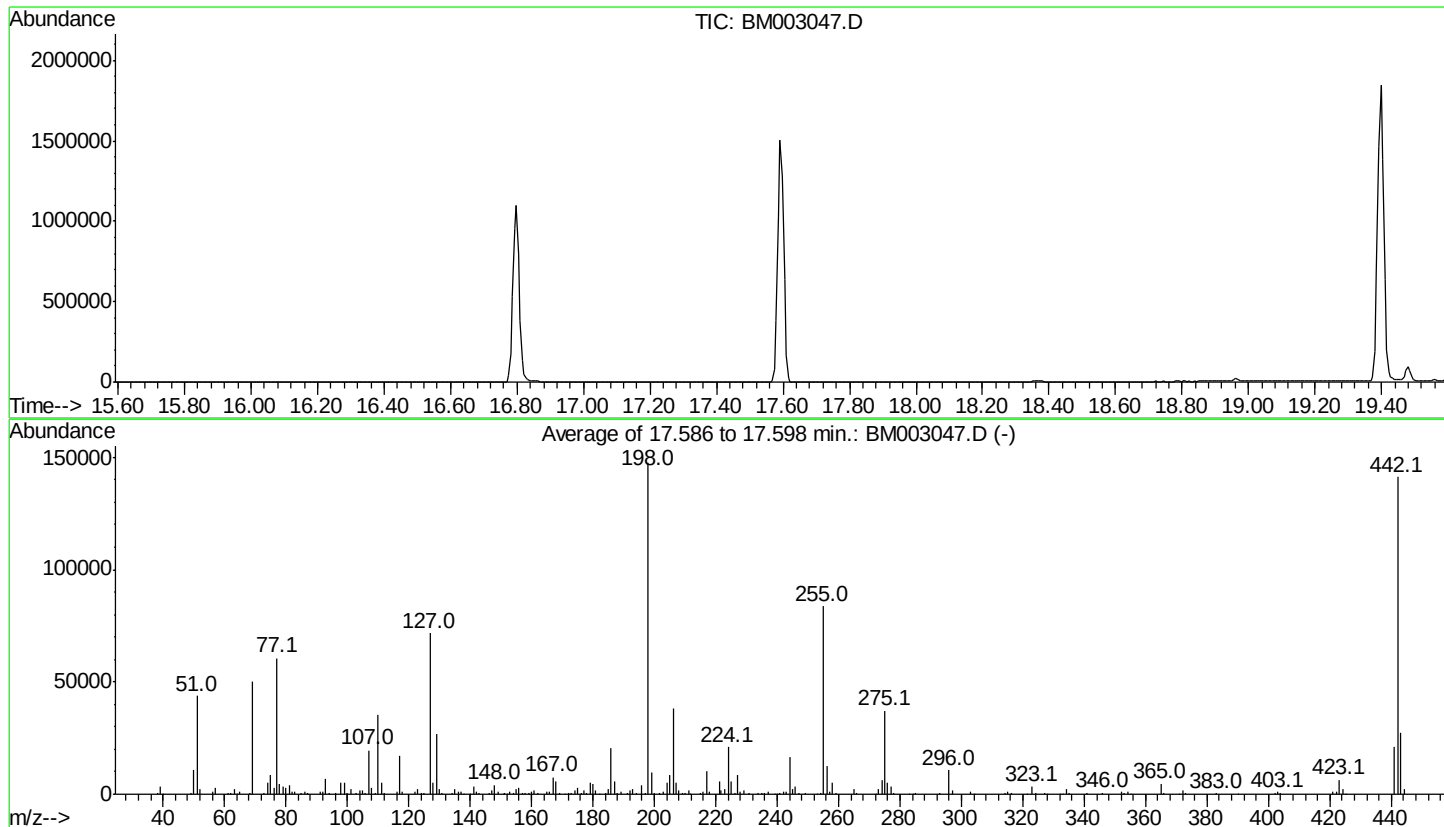

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	43730	PASS
68	69	0.00	2	1.6	824	PASS
69	198	0.00	100	34.0	50128	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	71704	PASS
197	198	0.00	2	0.5	712	PASS
198	198	100	100	100.0	147608	PASS
199	198	5	9	6.7	9906	PASS
275	198	10	60	25.2	37141	PASS
365	198	1	100	3.1	4623	PASS
441	442	0.01	24	15.1	21357	PASS
442	198	50	100	95.6	141176	PASS
443	442	15	24	19.5	27541	PASS