

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110416\
 Data File : BM007758.D
 Acq On : 04 Nov 2016 17:23
 Operator : UM/SJ
 Sample : H5532-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0102

Quant Time: Nov 04 22:16:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 23:14:40 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	963	0.40	ng/ul	0.00
2) Naphthalene-d8	10.54	136	3169	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.38	164	1892	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.23	188	266377	0.40	ng/ul	0.10
16) Chrysene-d12	21.31	240	3539	0.40	ng/ul	-0.01
20) Perylene-d12	23.43	264	247939	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.13	152	1506	0.40	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.38	166	652	0.09	ng/ul#	29
17) Pyrene	19.52	202	798	0.07	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110416\
Data File : BM007758.D
Acq On : 04 Nov 2016 17:23
Operator : UM/SJ
Sample : H5532-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0102

Quant Time: Nov 04 22:16:02 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 23:14:40 2016
Response via : Initial Calibration




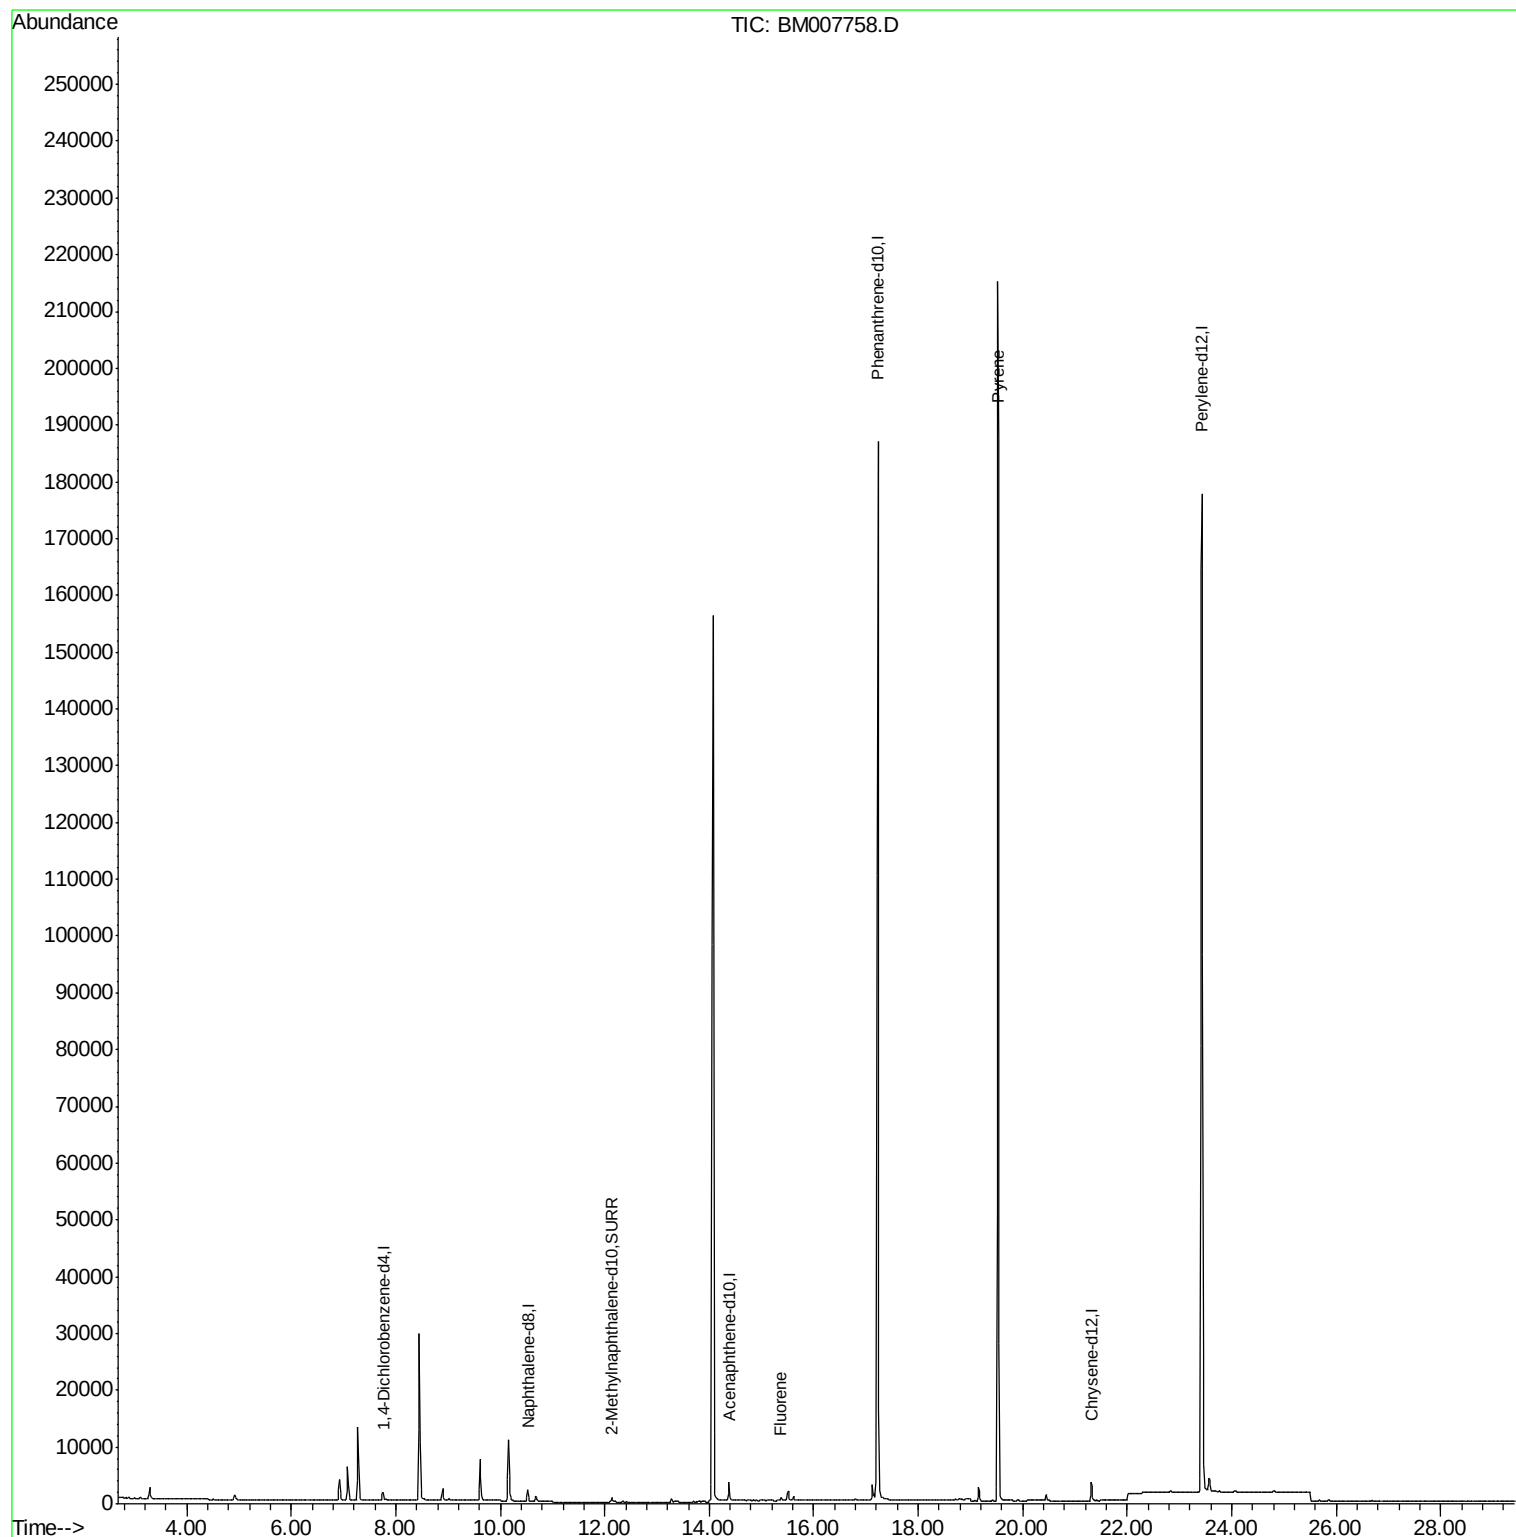


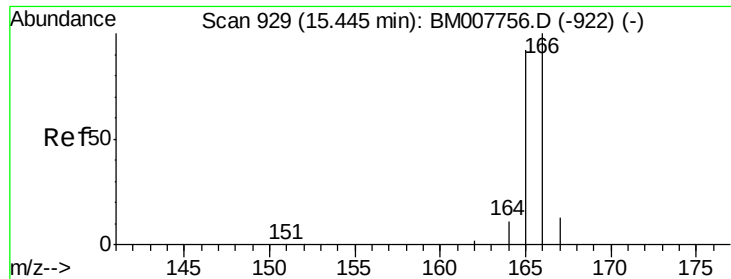

#9
Fluorene
 Concen: 0.09 ng/ul
 RT: 15.38 min Scan# 925
 Delta R.T. -0.07 min
 Lab File: BM007758.D
 Acq: 04 Nov 2016 17:23

Instrument :
 BNA_M
 ClientSampleId :
 H0102

Tgt Ion:166 Resp: 652
 Ion Ratio Lower Upper
 166 100
 165 19.6 73.4 110.2#
 167 38.4 14.6 22.0#

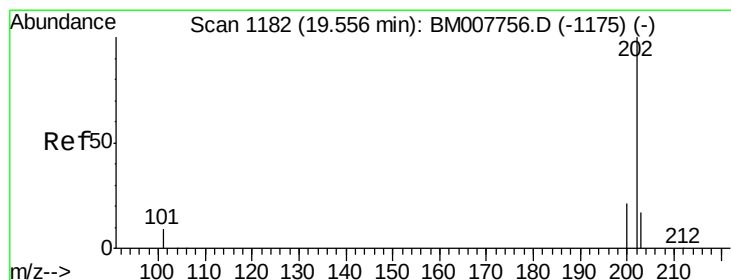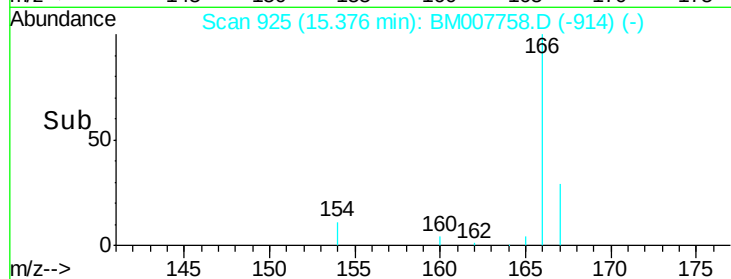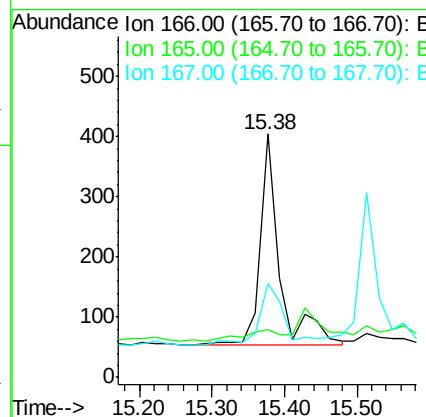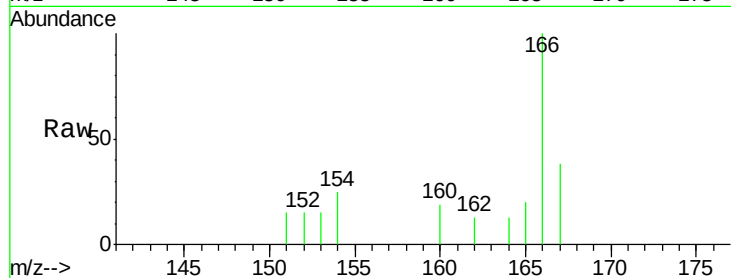

#17
Pyrene
 Concen: 0.07 ng/ul
 RT: 19.52 min Scan# 1179
 Delta R.T. -0.04 min
 Lab File: BM007758.D
 Acq: 04 Nov 2016 17:23

Tgt Ion:202 Resp: 798
 Ion Ratio Lower Upper
 202 100
 200 18.4 18.2 27.4
 203 137.6 15.6 23.4#

