


Data Path : Z:\HPCHEM1\BNA_M\Data\BM110417\
Data File : BM012701.D
Acq On : 04 Nov 2017 11:20
Operator : SJ/JU
Sample : DFTPP41
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP41

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM110417MA.M
Title : SVOA CALIBRATION
Last Update : Tue Nov 07 04:13:22 2017

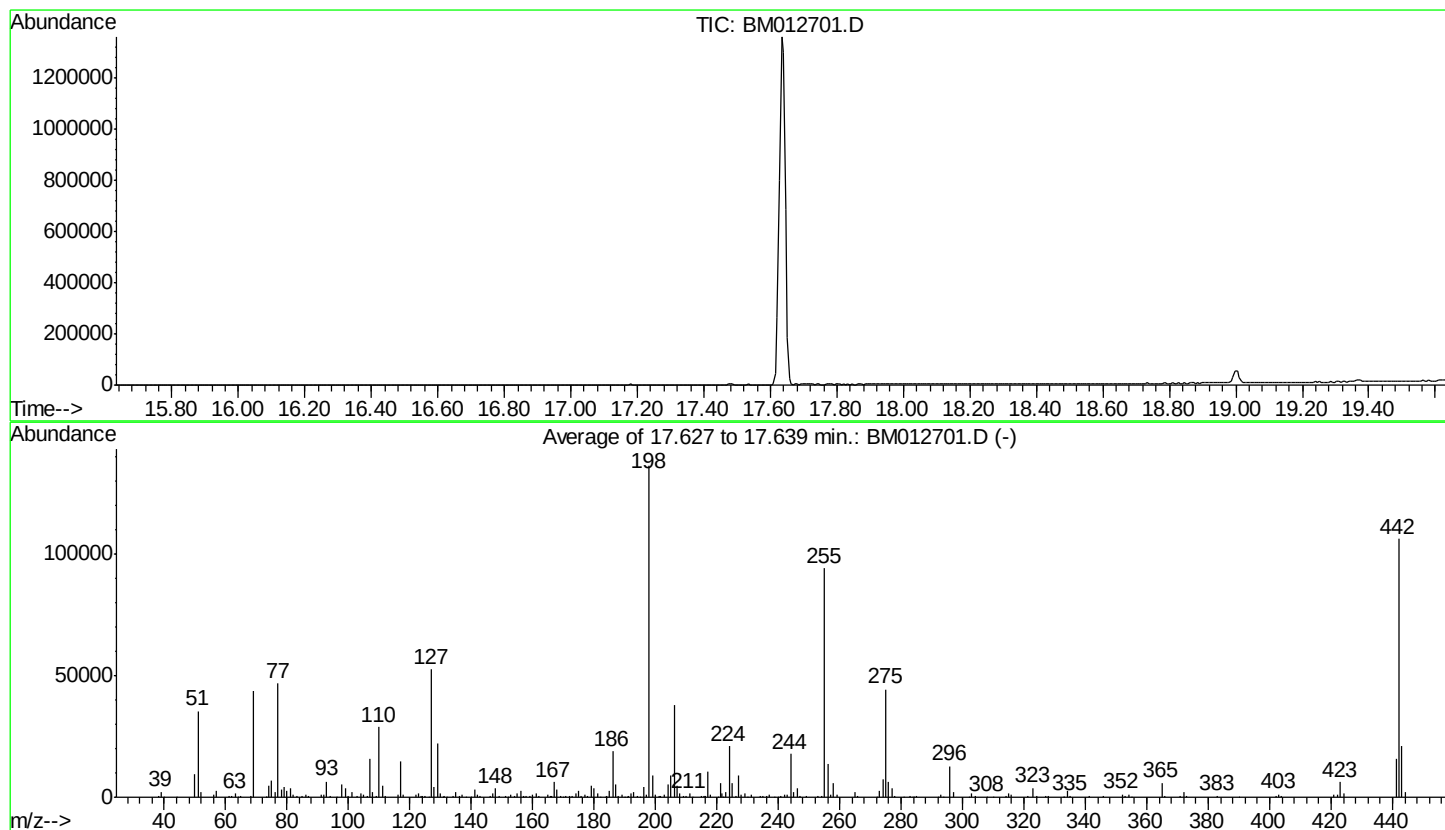

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	35466	PASS
68	69	0.00	2	1.5	651	PASS
69	198	0.00	100	32.2	43938	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.6	52597	PASS
197	198	0.00	2	0.7	1013	PASS
198	198	100	100	100.0	136314	PASS
199	198	5	9	6.7	9103	PASS
275	198	10	60	32.6	44424	PASS
365	198	1	100	4.3	5896	PASS
441	443	0.01	100	75.7	16007	PASS
442	198	50	100	77.9	106256	PASS
443	442	15	24	19.9	21148	PASS

Scan 2467 (17.598 min): BM012701.D
DFTPP41

m/z	Abundance
44.00	523.0
73.10	338.0
207.00	1015.0
281.00	428.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

m/z	Abundance
37.90	407.0
39.00	1815.0
44.00	816.0
50.10	8115.0
51.00	29272.0
52.00	1637.0
56.00	1023.0
57.00	2078.0
60.90	534.0
62.00	614.0
63.00	1121.0
65.00	595.0
68.20	709.0
69.00	35696.0
73.00	602.0
74.00	3576.0
75.00	5765.0
76.00	1819.0
77.00	36688.0
78.00	2561.0
79.00	3290.0
80.00	2388.0
81.00	3125.0
82.00	692.0
83.10	510.0
84.90	588.0
86.00	1110.0
86.90	424.0
91.00	779.0
92.00	810.0
93.00	5446.0
94.10	379.0
98.00	3818.0
98.90	3183.0
99.90	308.0
101.00	1539.0
102.90	618.0
104.00	1197.0
105.00	1083.0
106.10	391.0
107.00	12636.0
107.90	1618.0
109.10	322.0
110.00	22800.0
111.00	3798.0
112.00	504.0
116.00	943.0
117.00	11214.0
118.00	822.0
122.00	609.0
123.00	1290.0
123.80	467.0
125.00	603.0
127.00	40016.0
128.00	3085.0
129.00	17744.0
130.00	1529.0
131.00	381.0
134.00	453.0
135.00	1586.0
135.90	556.0
137.00	943.0
141.00	2157.0
141.90	864.0
143.00	485.0
145.90	471.0
147.00	1337.0
148.00	3059.0
148.90	760.0
151.20	316.0
152.90	881.0
154.00	406.0
155.00	1578.0
156.00	1918.0
156.90	515.0
157.90	404.0
158.90	342.0
159.80	678.0
161.10	938.0
161.90	555.0
164.90	962.0
166.00	664.0
167.00	4554.0
168.00	2682.0
169.00	580.0
172.10	430.0
172.90	428.0
173.90	838.0
175.00	1828.0
176.00	522.0
176.90	993.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

177.90	476.0
179.00	3275.0
180.00	2615.0
181.00	1049.0
183.80	310.0
185.00	1815.0
186.00	13683.0
187.00	3720.0
188.00	462.0
188.90	917.0
190.90	755.0
191.90	1141.0
193.00	1565.0
196.00	3295.0
197.10	668.0
197.90	95344.0
198.90	6897.0
199.90	557.0
201.30	608.0
202.90	653.0
204.00	3348.0
205.00	5786.0
206.00	26736.0
207.00	4894.0
207.90	1003.0
209.10	411.0
209.90	462.0
211.00	1091.0
215.00	398.0
215.90	689.0
216.90	7656.0
217.90	1022.0
221.00	3223.0
221.80	713.0
222.00	699.0
222.90	1821.0
224.00	13572.0
224.90	3674.0
226.00	551.0
227.00	6588.0
227.90	1101.0
228.90	1440.0
231.00	586.0
233.90	387.0
235.00	426.0
237.00	711.0
240.90	346.0
241.90	750.0
243.10	881.0
244.00	11365.0
245.10	1525.0
246.00	2536.0
247.00	422.0
248.90	526.0
255.00	60456.0
256.00	9595.0
256.90	699.0
258.00	3994.0
259.00	557.0
264.90	1438.0
273.00	1801.0
274.00	4897.0
275.00	29608.0
276.00	4183.0
277.00	2547.0
277.90	464.0
281.00	552.0
282.90	395.0
292.90	485.0
296.00	8163.0
296.90	1284.0
303.00	831.0
303.90	380.0
314.00	351.0
315.00	912.0
315.90	497.0
321.00	342.0
323.00	2377.0
324.00	461.0
327.00	428.0
328.00	375.0
334.00	1496.0
335.10	376.0
346.00	455.0
352.10	652.0
353.00	534.0
354.00	663.0
365.00	3609.0
366.00	431.0
372.00	1096.0
373.10	307.0
383.00	400.0
402.10	455.0
403.00	532.0
421.10	460.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

422.00	620.0
423.00	2823.0
424.10	860.0
441.10	8295.0
442.10	56272.0
443.10	10910.0
444.10	1150.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

m/z	Abundance
38.00	389.0
39.00	2733.0
40.00	306.0
44.00	647.0
50.00	11624.0
51.00	43160.0
52.00	2001.0
55.90	1460.0
57.00	2827.0
61.00	680.0
62.10	785.0
63.00	2054.0
64.00	316.0
65.00	991.0
69.00	53752.0
73.20	685.0
74.00	5721.0
75.00	8831.0
76.00	2791.0
77.10	57456.0
78.10	4057.0
79.00	5182.0
80.00	3565.0
81.00	4379.0
82.10	1029.0
83.00	847.0
85.00	1042.0
86.00	1447.0
87.00	554.0
90.90	1329.0
91.90	1103.0
93.00	7750.0
93.90	401.0
96.00	420.0
98.00	6605.0
99.00	4648.0
99.90	303.0
101.00	2669.0
103.00	948.0
104.00	1441.0
105.00	1502.0
106.10	609.0
107.00	18952.0
108.00	2753.0
109.20	621.0
110.00	34160.0
111.00	5949.0
112.10	702.0
115.90	1166.0
117.00	17608.0
118.00	1132.0
122.00	1450.0
122.90	2030.0
124.10	908.0
125.10	994.0
126.10	522.0
127.00	62128.0
128.00	4915.0
129.00	26152.0
130.00	2052.0
131.10	594.0
132.00	341.0
133.90	851.0
135.10	2204.0
135.90	817.0
137.00	1100.0
138.20	387.0
139.90	409.0
140.90	3778.0
142.00	1174.0
142.90	1135.0
145.90	818.0
147.00	1875.0
148.00	4059.0
149.00	839.0
151.10	505.0
151.90	312.0
153.00	1309.0
153.90	622.0
155.00	1869.0
156.00	2967.0
157.10	455.0
157.80	562.0
158.90	565.0
159.90	1196.0
161.00	1618.0
161.90	519.0
165.00	1497.0
165.80	1089.0
167.00	7393.0
168.00	3796.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

169.00	877.0
170.00	369.0
170.90	547.0
171.90	643.0
173.00	877.0
174.00	1782.0
175.00	3467.0
175.90	793.0
177.00	1629.0
178.00	474.0
179.00	5889.0
179.90	4387.0
181.00	2134.0
182.00	317.0
184.10	453.0
185.00	3028.0
186.00	21712.0
187.00	6210.0
188.00	809.0
189.00	1332.0
190.00	319.0
191.10	777.0
191.90	2035.0
193.00	2319.0
194.00	506.0
194.90	308.0
196.00	4548.0
197.10	1179.0
197.90	162304.0
199.00	10323.0
199.90	846.0
201.50	840.0
203.00	1283.0
204.00	6545.0
205.00	9791.0
206.00	45296.0
207.00	6864.0
208.00	1769.0
209.00	789.0
210.00	750.0
211.10	1731.0
212.00	366.0
215.00	550.0
215.80	901.0
216.20	863.0
217.00	12052.0
218.00	1691.0
220.20	500.0
221.00	6719.0
221.80	1795.0
223.00	2808.0
224.00	25384.0
225.00	7013.0
226.00	791.0
227.00	10621.0
228.00	1548.0
228.90	2068.0
230.00	369.0
231.00	942.0
233.90	728.0
235.00	690.0
236.00	623.0
237.00	919.0
238.90	448.0
240.00	400.0
240.90	583.0
242.00	1560.0
243.00	1449.0
244.00	21536.0
245.10	2593.0
246.00	4484.0
247.00	919.0
249.00	744.0
252.90	407.0
254.10	1023.0
255.00	111456.0
256.00	15486.0
257.00	1006.0
258.00	6470.0
259.00	861.0
265.00	2238.0
266.00	386.0
273.00	3334.0
274.00	8744.0
275.00	50928.0
276.00	7096.0
277.00	4144.0
278.00	861.0
281.00	473.0
282.90	423.0
283.90	367.0
285.10	679.0
292.90	952.0
296.00	14708.0
297.00	2439.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

303.00	1618.0
303.90	468.0
308.00	305.0
314.00	587.0
315.00	1564.0
316.00	956.0
321.00	449.0
323.00	3973.0
324.00	810.0
327.10	714.0
328.00	556.0
332.90	544.0
334.00	3192.0
335.10	956.0
341.10	388.0
346.00	940.0
352.00	1305.0
353.00	868.0
354.00	1356.0
355.00	321.0
365.00	6515.0
366.00	797.0
371.00	457.0
372.10	2649.0
373.10	562.0
382.90	600.0
402.10	728.0
403.00	1306.0
403.90	321.0
421.10	952.0
422.00	945.0
423.10	7184.0
424.10	2320.0
441.10	17400.0
442.10	118304.0
443.10	23768.0
444.00	2089.0

Instrument :

BNA_M

ClientSampleId :

DFTPP41

m/z	Abundance
38.10	621.0
39.00	2336.0
39.90	304.0
44.00	428.0
50.00	9246.0
51.00	33968.0
52.10	2038.0
56.00	1223.0
57.00	2567.0
60.90	517.0
62.00	535.0
63.00	1571.0
64.90	779.0
68.10	1244.0
69.00	42368.0
73.10	650.0
74.00	4311.0
75.00	6778.0
76.00	2313.0
77.00	45760.0
78.00	3035.0
79.00	3566.0
80.00	2429.0
81.00	3856.0
81.90	866.0
83.00	885.0
84.90	792.0
86.00	1206.0
87.00	631.0
91.00	814.0
92.00	1206.0
93.00	6365.0
94.00	478.0
96.10	400.0
98.00	5257.0
99.00	3510.0
100.00	316.0
101.00	2219.0
103.10	739.0
104.00	1547.0
105.00	1281.0
105.90	517.0
107.00	15584.0
108.00	2516.0
109.10	431.0
110.00	29792.0
111.00	4804.0
112.00	482.0
116.10	1080.0
117.00	15418.0
118.00	1070.0
122.00	1222.0
123.00	1751.0
123.90	881.0
125.00	794.0
127.00	55648.0
128.00	4536.0
129.00	22480.0
130.00	1704.0
130.80	344.0
132.00	301.0
134.00	670.0
135.00	1861.0
136.00	675.0
137.00	1038.0
139.90	404.0
141.00	3270.0
142.00	1022.0
143.00	622.0
146.00	622.0
146.90	1780.0
148.00	3694.0
149.00	783.0
151.00	458.0
152.00	404.0
153.00	1120.0
154.00	868.0
155.00	1709.0
156.00	3023.0
156.90	752.0
157.90	640.0
159.00	417.0
160.00	927.0
161.00	1453.0
162.00	555.0
165.00	1442.0
166.10	1121.0
167.00	6647.0
168.00	3348.0
168.90	481.0
170.90	315.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

171.90	624.0
172.90	794.0
174.00	1888.0
175.00	2754.0
175.90	848.0
177.00	1280.0
177.80	465.0
179.00	5609.0
180.00	3682.0
181.00	1614.0
184.00	476.0
185.00	3018.0
186.00	21064.0
187.00	5893.0
187.90	749.0
188.90	1282.0
191.00	737.0
191.90	1833.0
193.00	2161.0
193.90	346.0
196.00	4994.0
197.10	1192.0
197.90	151296.0
199.00	10089.0
200.00	1033.0
201.30	903.0
202.90	1110.0
204.00	5694.0
205.00	10589.0
206.00	41088.0
207.00	5771.0
208.00	1863.0
209.00	637.0
210.10	812.0
211.00	1751.0
212.00	313.0
215.00	605.0
216.00	939.0
216.90	11256.0
217.90	1204.0
221.00	7345.0
221.80	1577.0
222.90	2429.0
224.00	24192.0
225.00	6416.0
226.00	629.0
227.00	10326.0
228.00	1272.0
229.00	2050.0
229.90	309.0
231.00	1086.0
234.00	664.0
235.00	648.0
236.10	404.0
237.00	879.0
238.90	370.0
240.90	615.0
242.10	1038.0
243.00	1317.0
244.00	20080.0
245.00	2690.0
246.00	4051.0
246.90	846.0
249.00	649.0
253.00	653.0
254.10	1021.0
255.00	110432.0
256.00	15573.0
257.00	1517.0
258.00	6200.0
259.00	1193.0
265.00	2269.0
265.90	497.0
271.90	426.0
273.00	3571.0
274.00	7963.0
275.00	52736.0
276.00	7248.0
276.90	4812.0
277.90	710.0
281.00	648.0
282.90	582.0
284.10	436.0
285.10	781.0
292.10	372.0
292.90	1077.0
293.90	313.0
296.00	15658.0
297.00	2568.0
302.00	322.0
303.00	1783.0
304.00	534.0
308.00	311.0
310.00	437.0
314.00	826.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

314.90	1577.0
316.00	992.0
321.10	384.0
323.00	4968.0
324.10	764.0
327.00	1126.0
328.00	329.0
333.10	463.0
334.00	3784.0
334.90	605.0
341.00	760.0
346.00	881.0
352.00	1365.0
353.00	980.0
354.10	1827.0
355.00	331.0
365.00	7565.0
365.90	950.0
370.90	460.0
372.00	2524.0
373.10	733.0
383.10	712.0
390.00	397.0
402.10	1175.0
403.00	1495.0
404.00	522.0
421.00	1186.0
422.00	1292.0
423.10	8571.0
424.10	2015.0
441.10	22328.0
442.10	144192.0
443.10	28768.0
444.10	2370.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41