
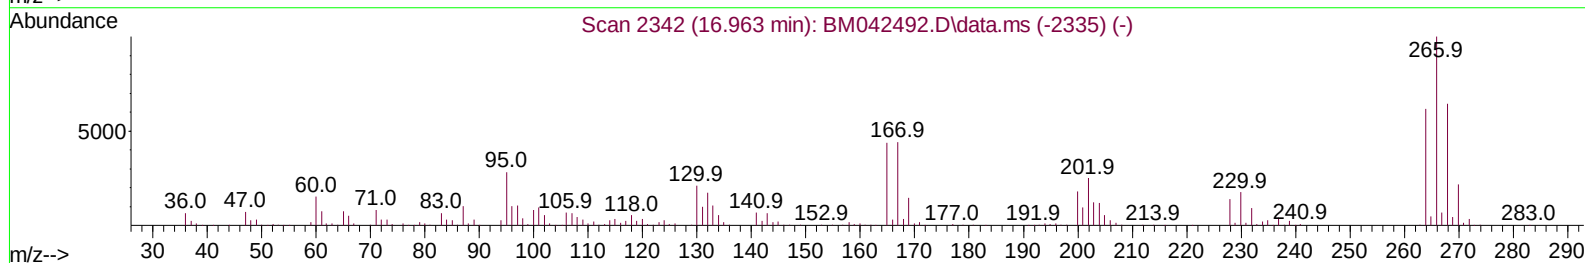
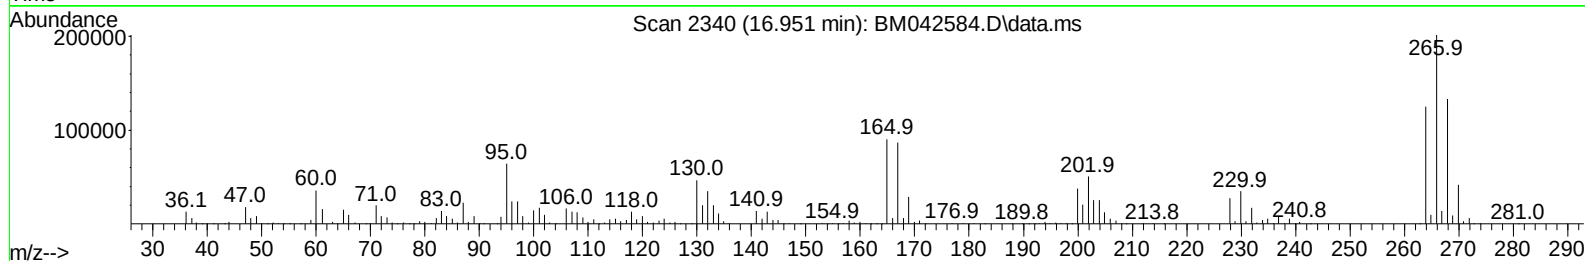


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110423\
Data File : BM042584.D
Acq On : 04 Nov 2023 09:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 03:52:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:52:20 2023
Response via : Initial Calibration

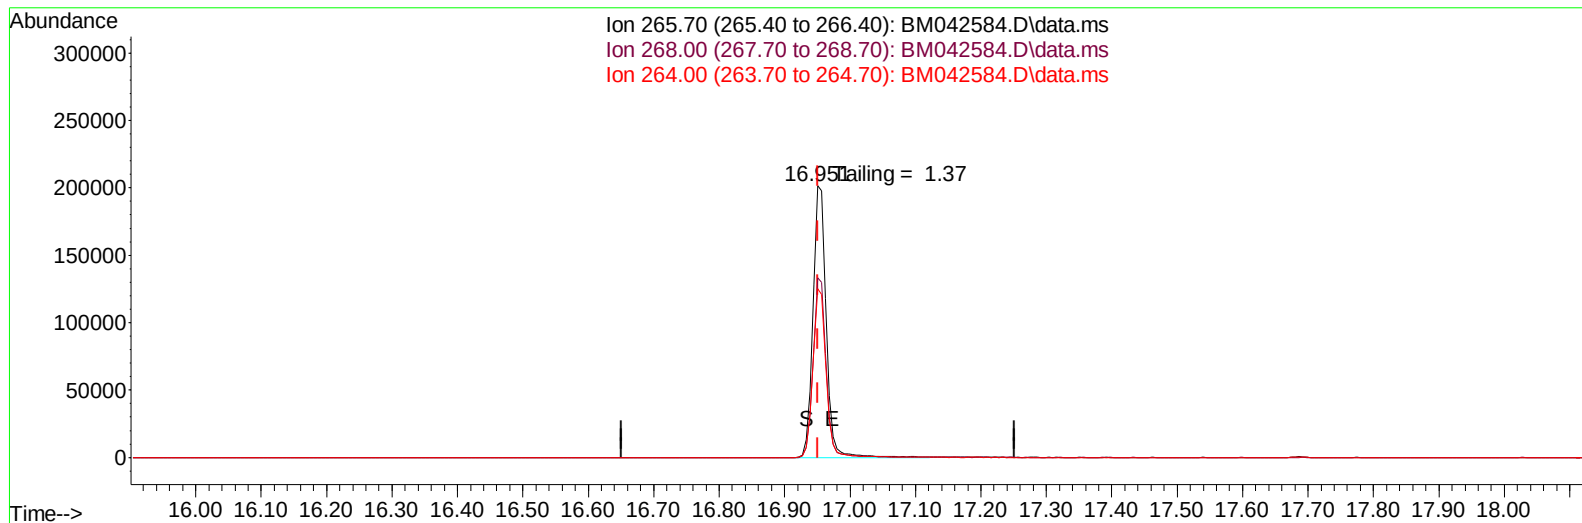

TIC: BM042584.D\data.ms

(70) Pentachlorophenol (C)




16.951min (-0.000) 0.00 ng

response 284216

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	66.03
264.00	61.80	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110423\
Data File : BM042584.D
Acq On : 04 Nov 2023 09:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 03:52:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:52:20 2023
Response via : Initial Calibration

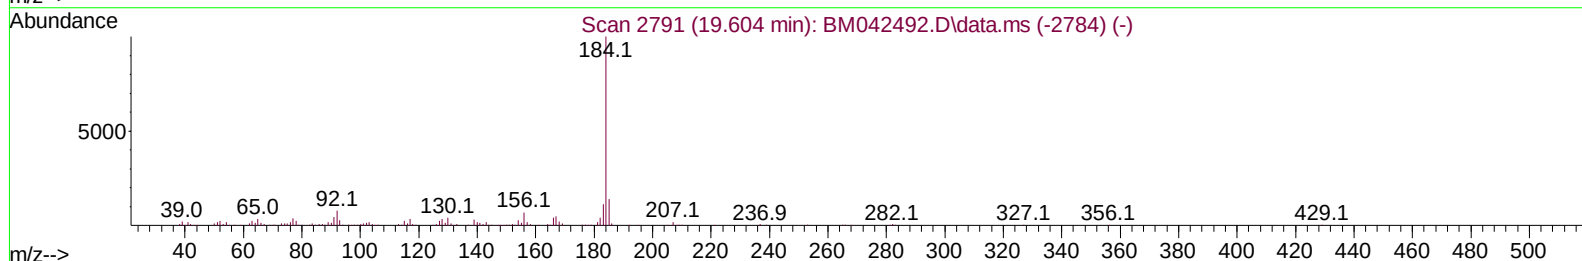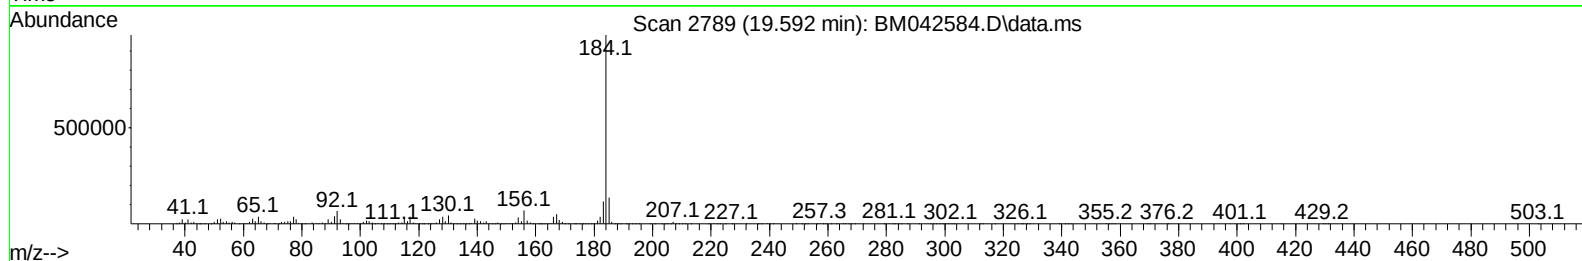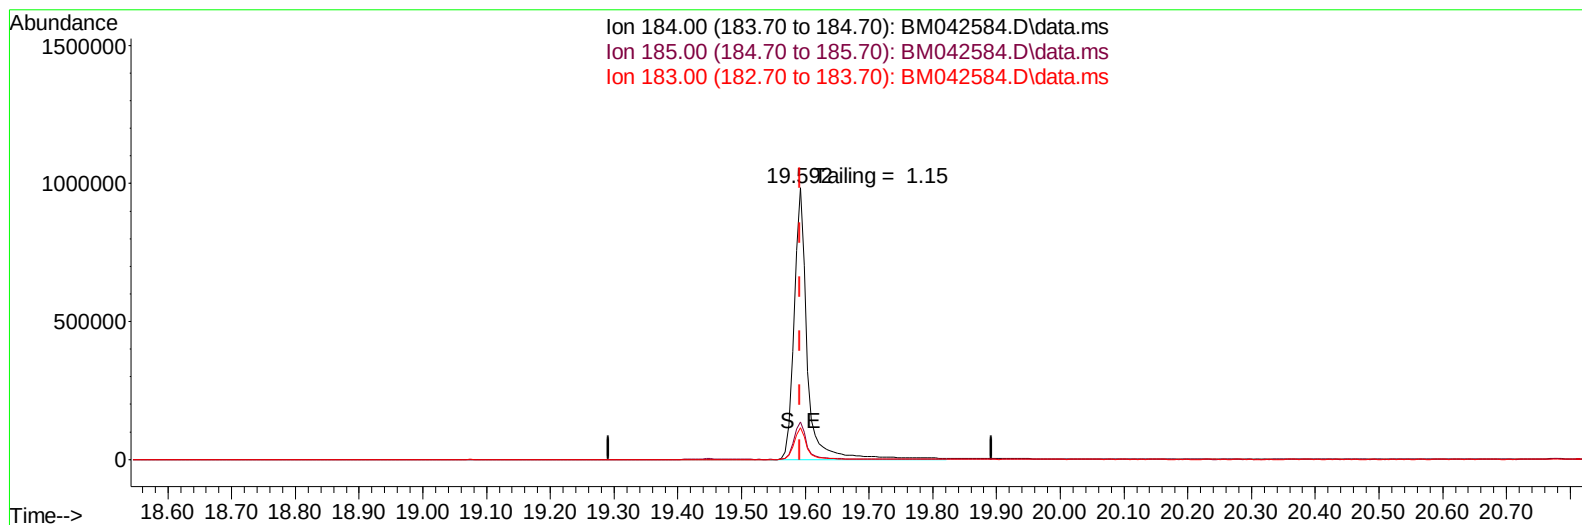

TIC: BM042584.D\data.ms

(77) Benzidine**19.592min (-0.000) 29673.88 ng****response 1416654**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.87
183.00	11.20	11.74
0.00	0.00	0.00