


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110423\
Data File : BM042584.D
Acq On : 04 Nov 2023 09:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 03 15:52:20 2023

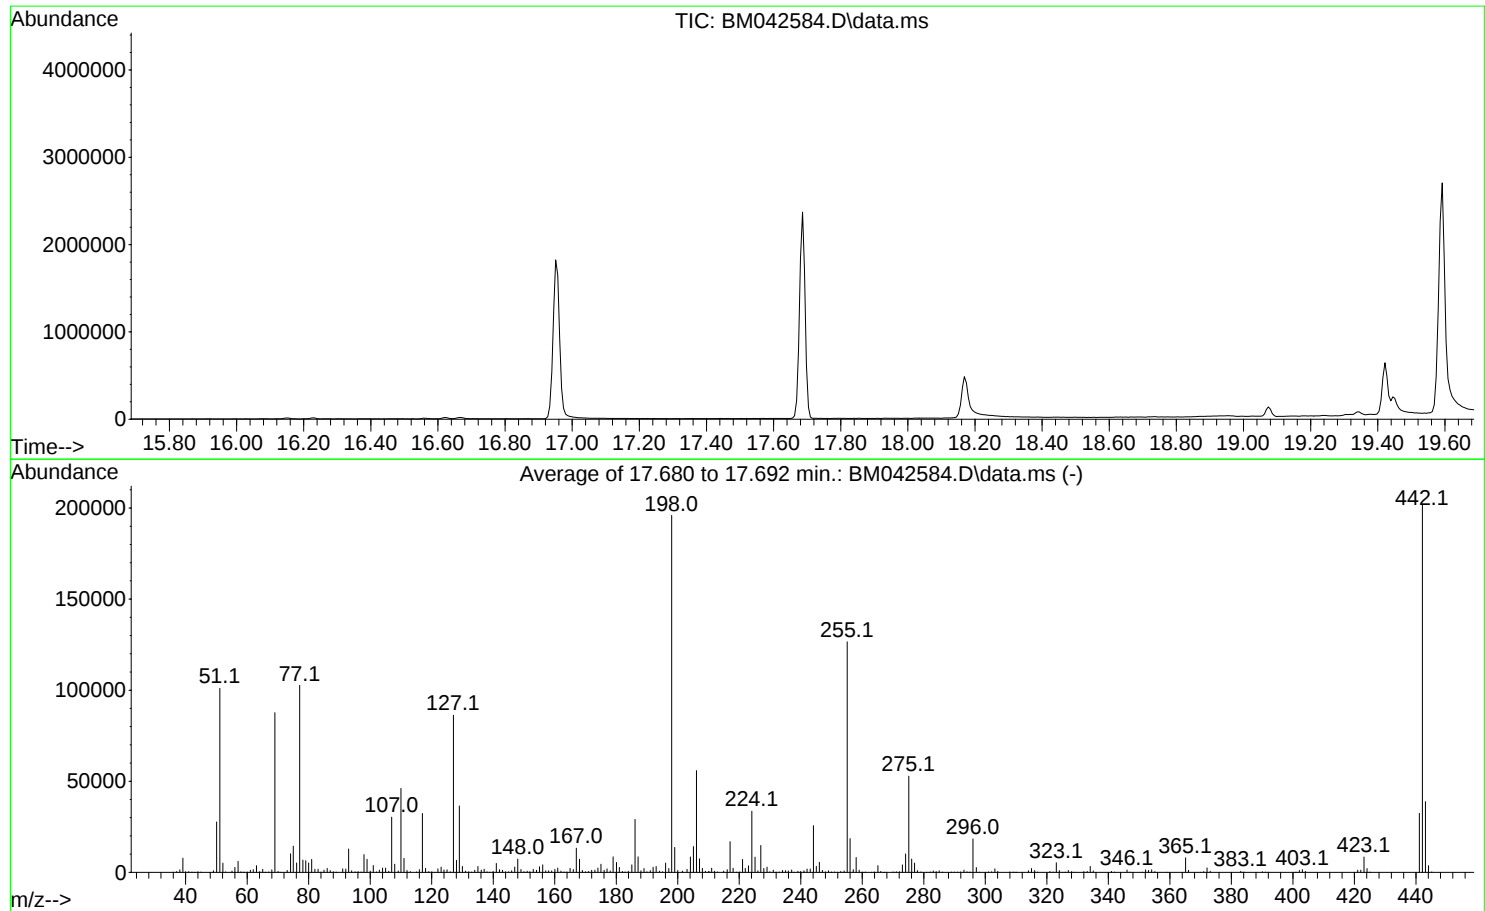




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.6	101048	PASS
68	69	0.00	2	1.6	1401	PASS
69	198	0.00	100	44.7	87646	PASS
70	69	0.00	2	0.6	540	PASS
127	198	10	80	44.0	86253	PASS
197	198	0.00	2	1.1	2111	PASS
198	198	100	100	100.0	195925	PASS
199	198	5	9	7.0	13703	PASS
275	198	10	60	26.9	52781	PASS
365	198	1	100	4.1	7986	PASS
441	198	0.01	100	16.5	32400	PASS
442	442	50	100	100.0	201941	PASS
443	442	15	24	19.2	38808	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110423\
Data File : BM042584.D
Acq On : 04 Nov 2023 09:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 06 03:52:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:52:20 2023
Response via : Initial Calibration

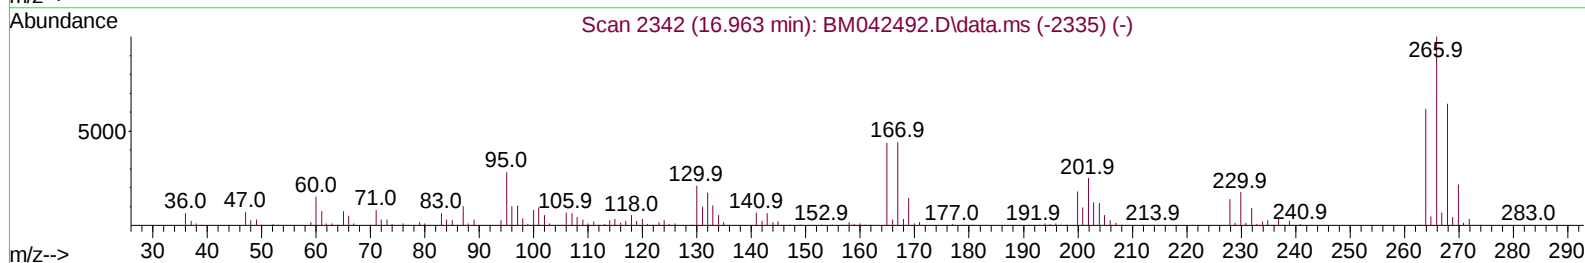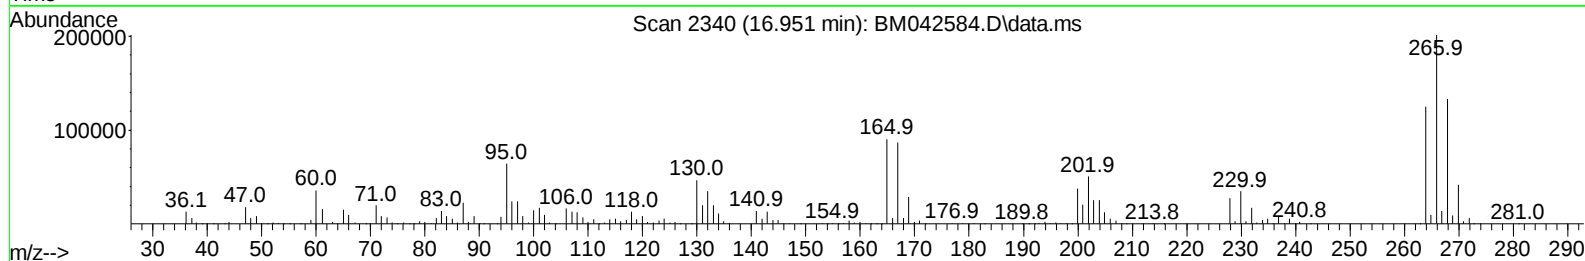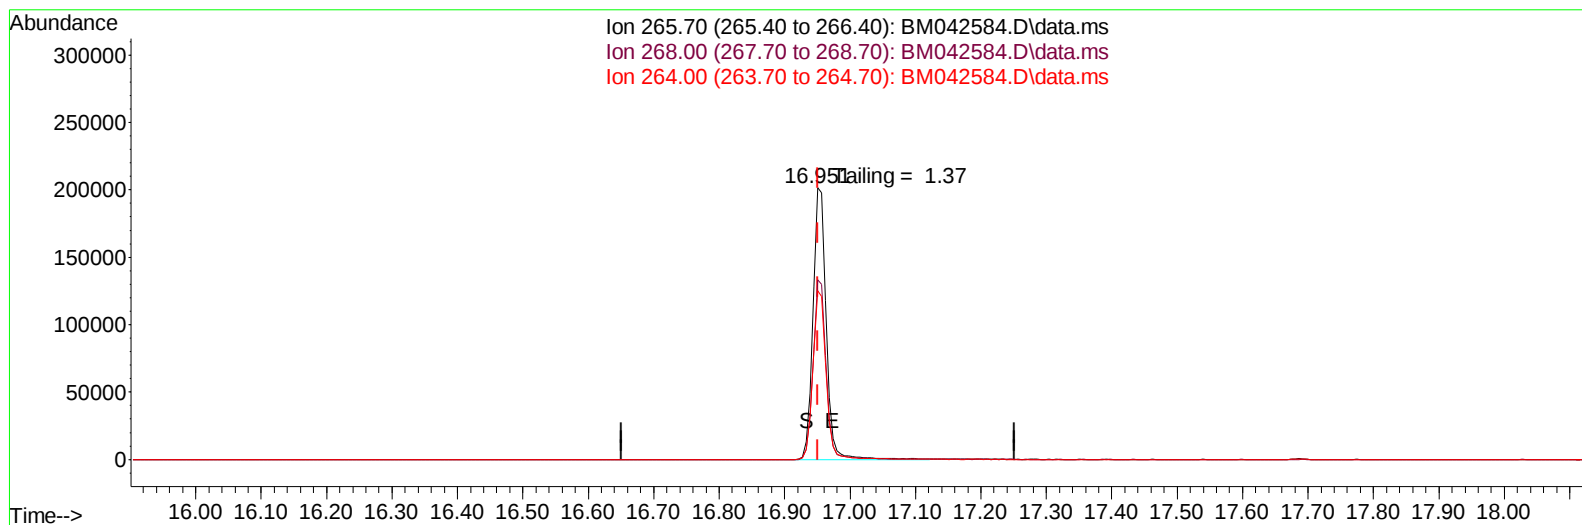

TIC: BM042584.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.000) 0.00 ng




response 284216

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	66.03
264.00	61.80	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110423\
Data File : BM042584.D
Acq On : 04 Nov 2023 09:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 06 03:52:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:52:20 2023
Response via : Initial Calibration

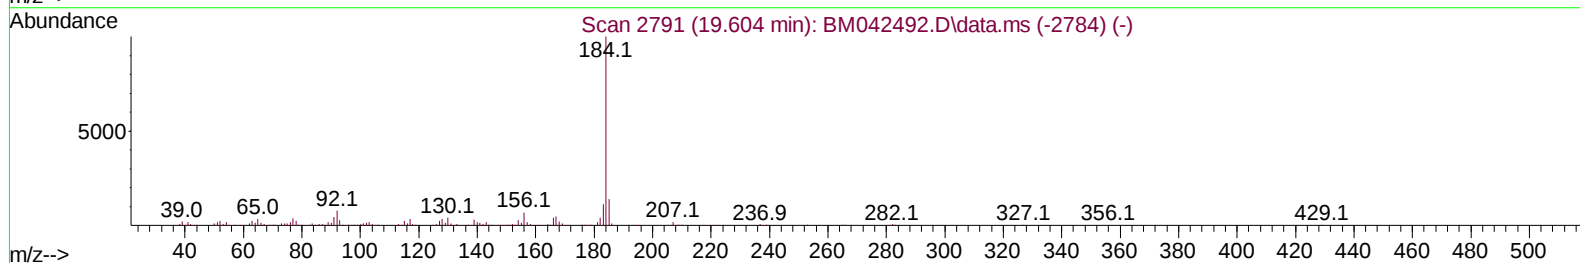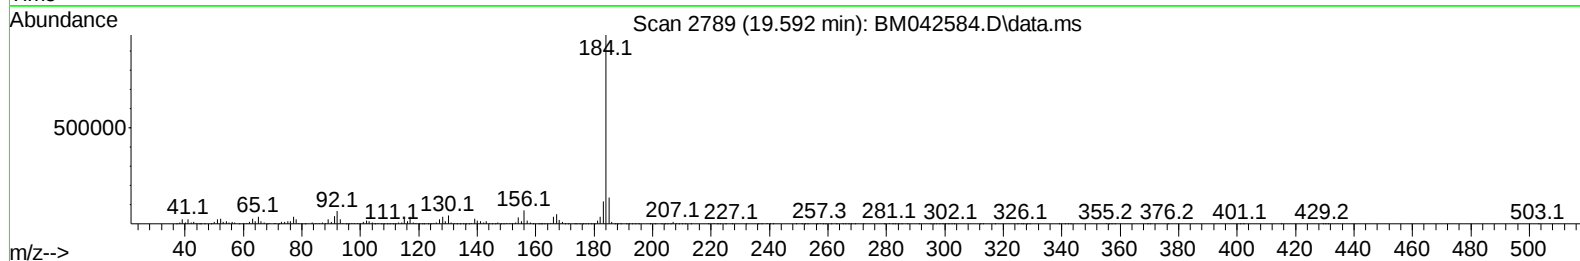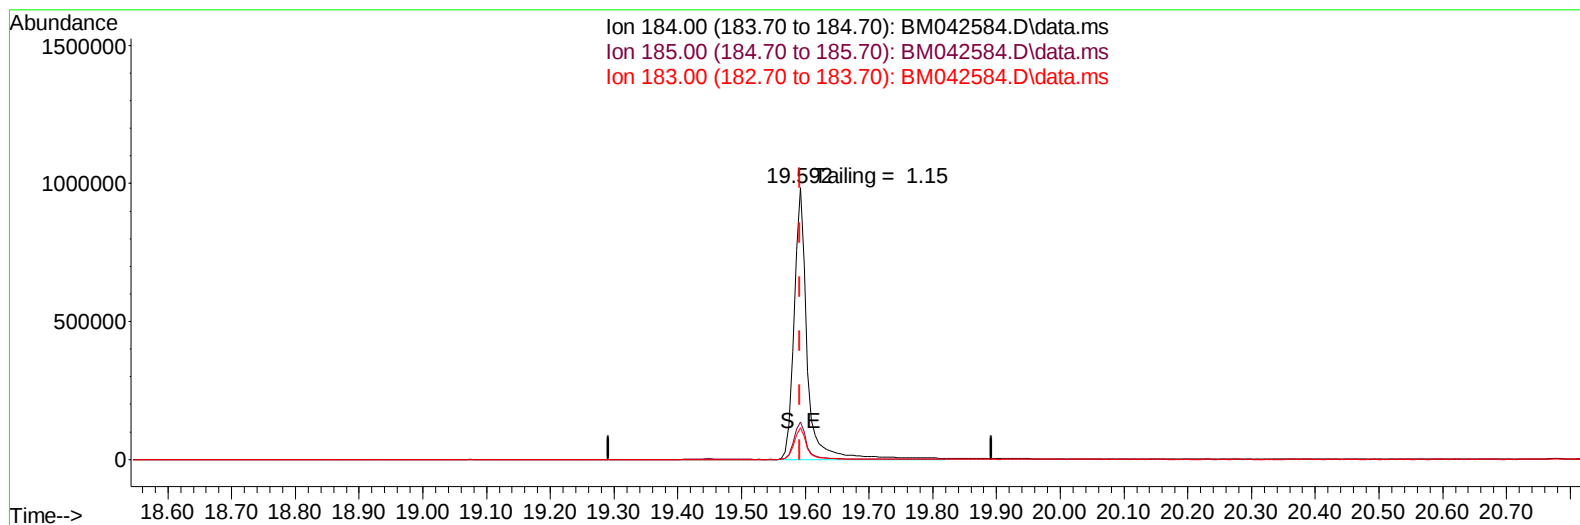

TIC: BM042584.D\data.ms

(77) Benzidine

19.592min (-0.000) 29673.88 ng

response 1416654

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.87
183.00	11.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2023	BNA_M	<u>BM042584.D</u>
Compound Name	Response	Retention Time
DDT	897471	20.78
DDD	12857	20.38
DDE	1332	19.421
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14189	911660	1.56

Instrument :
BNA_M
ClientSampleId :
DFTPP