

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110424\
 Data File : BM048445.D
 Acq On : 05 Nov 2024 02:18
 Operator : RC/JU
 Sample : P4625-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/05/2024
 Supervised By :mohammad ahmed 11/06/2024

Quant Time: Nov 05 02:54:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	5100	0.400	ng/u1	-0.05
4) Naphthalene-d8	10.484	136	15523	0.400	ng/u1	#-0.05
9) Acenaphthene-d10	14.343	164	7805	0.400	ng/u1	-0.02
13) Phenanthrene-d10	17.085	188	15046m	0.400	ng/u1	-0.04
17) Chrysene-d12	21.298	240	10567m	0.400	ng/u1	0.00
23) Perylene-d12	23.510	264	7145m	0.400	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	29616	4.728	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.112	152	6428	0.325	ng/u1	-0.03
18) Fluoranthene-d10	19.117	212	13591	0.507	ng/u1	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.534	128	4930	0.122	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110424\
Data File : BM048445.D
Acq On : 05 Nov 2024 02:18
Operator : RC/JU
Sample : P4625-15
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AC4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/05/2024
Supervised By :mohammad ahmed 11/06/2024


Quant Time: Nov 05 02:54:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

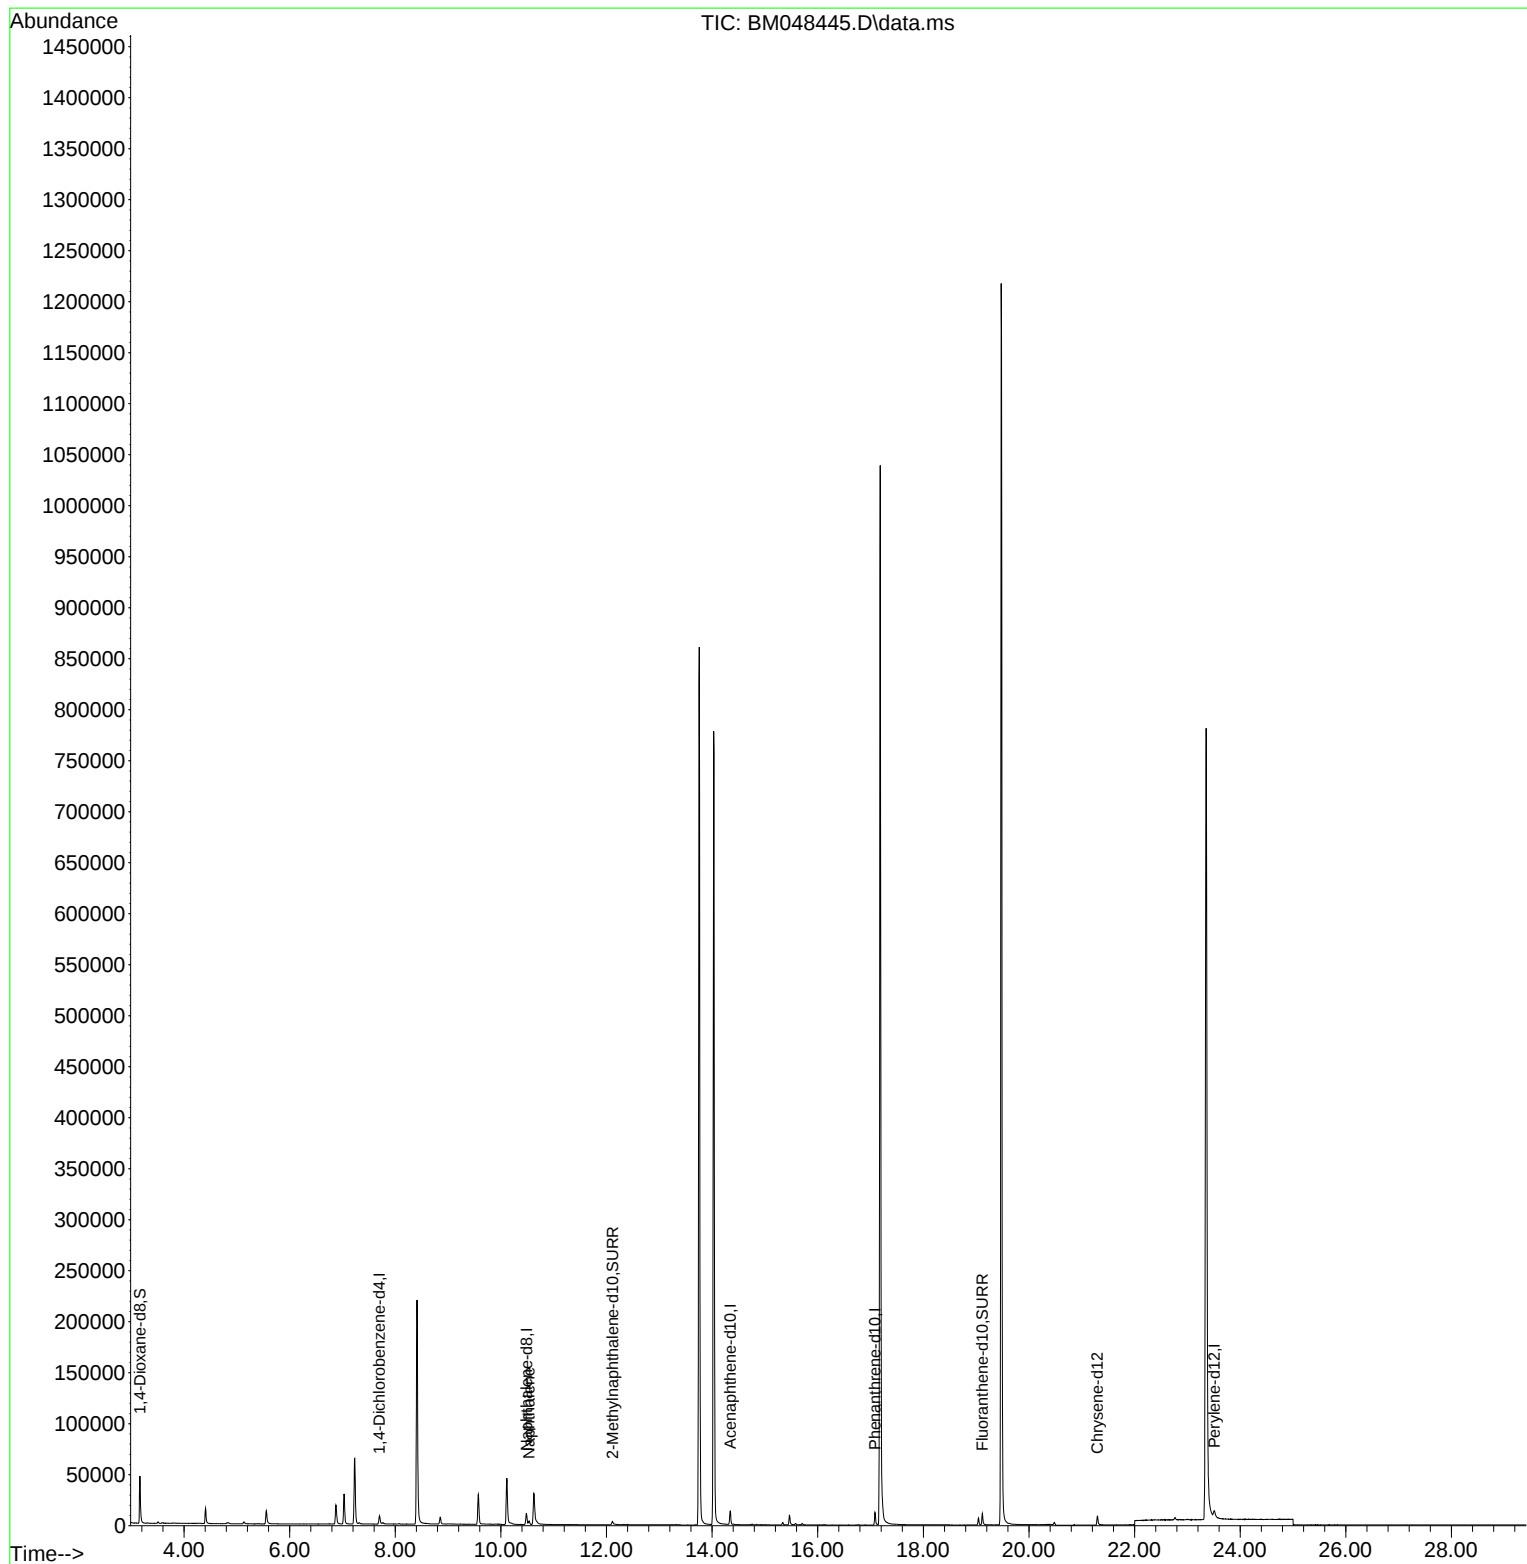

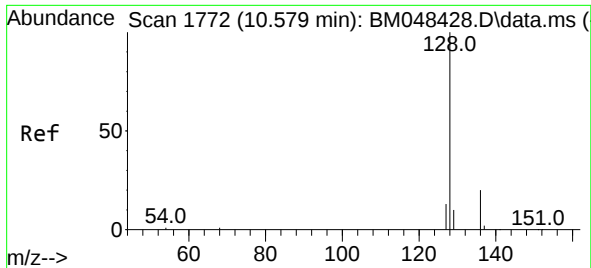

#5
Naphthalene
Concen: 0.122 ng/ul
RT: 10.534 min Scan# 1772
Delta R.T. -0.045 min
Lab File: BM048445.D
Acq: 05 Nov 2024 02:18

Instrument :
BNA_M
ClientSampleId :
C0AC4

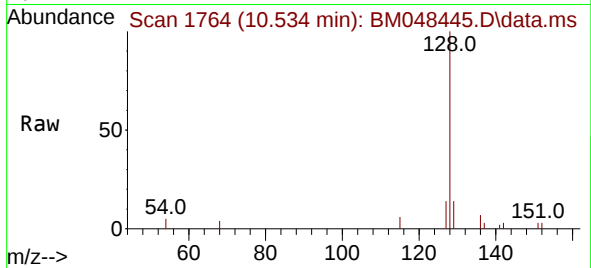

Tgt Ion:128 Resp: 4930
Ion Ratio Lower Upper
128 100
129 14.3 10.6 15.8
127 14.2 11.4 17.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/05/2024
Supervised By :mohammad ahmed 11/06/2024

