

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110424\
 Data File : BM048449.D
 Acq On : 05 Nov 2024 05:18
 Operator : RC/JU
 Sample : P4625-17
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/05/2024
 Supervised By :mohammad ahmed 11/06/2024

Quant Time: Nov 05 05:59:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 05 05:12:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	5681	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.479	136	17647	0.400	ng/ul	-0.05
9) Acenaphthene-d10	14.339	164	9370	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.085	188	18658m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.292	240	12914m	0.400	ng/ul	0.00
23) Perylene-d12	23.508	264	9086m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	36661	5.255	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.101	152	9226	0.411	ng/ul	-0.04
18) Fluoranthene-d10	19.117	212	18298	0.558	ng/ul	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.529	128	2037	0.044	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110424\
Data File : BM048449.D
Acq On : 05 Nov 2024 05:18
Operator : RC/JU
Sample : P4625-17
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AC8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/05/2024
Supervised By :mohammad ahmed 11/06/2024


Quant Time: Nov 05 05:59:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 05 05:12:02 2024
Response via : Initial Calibration

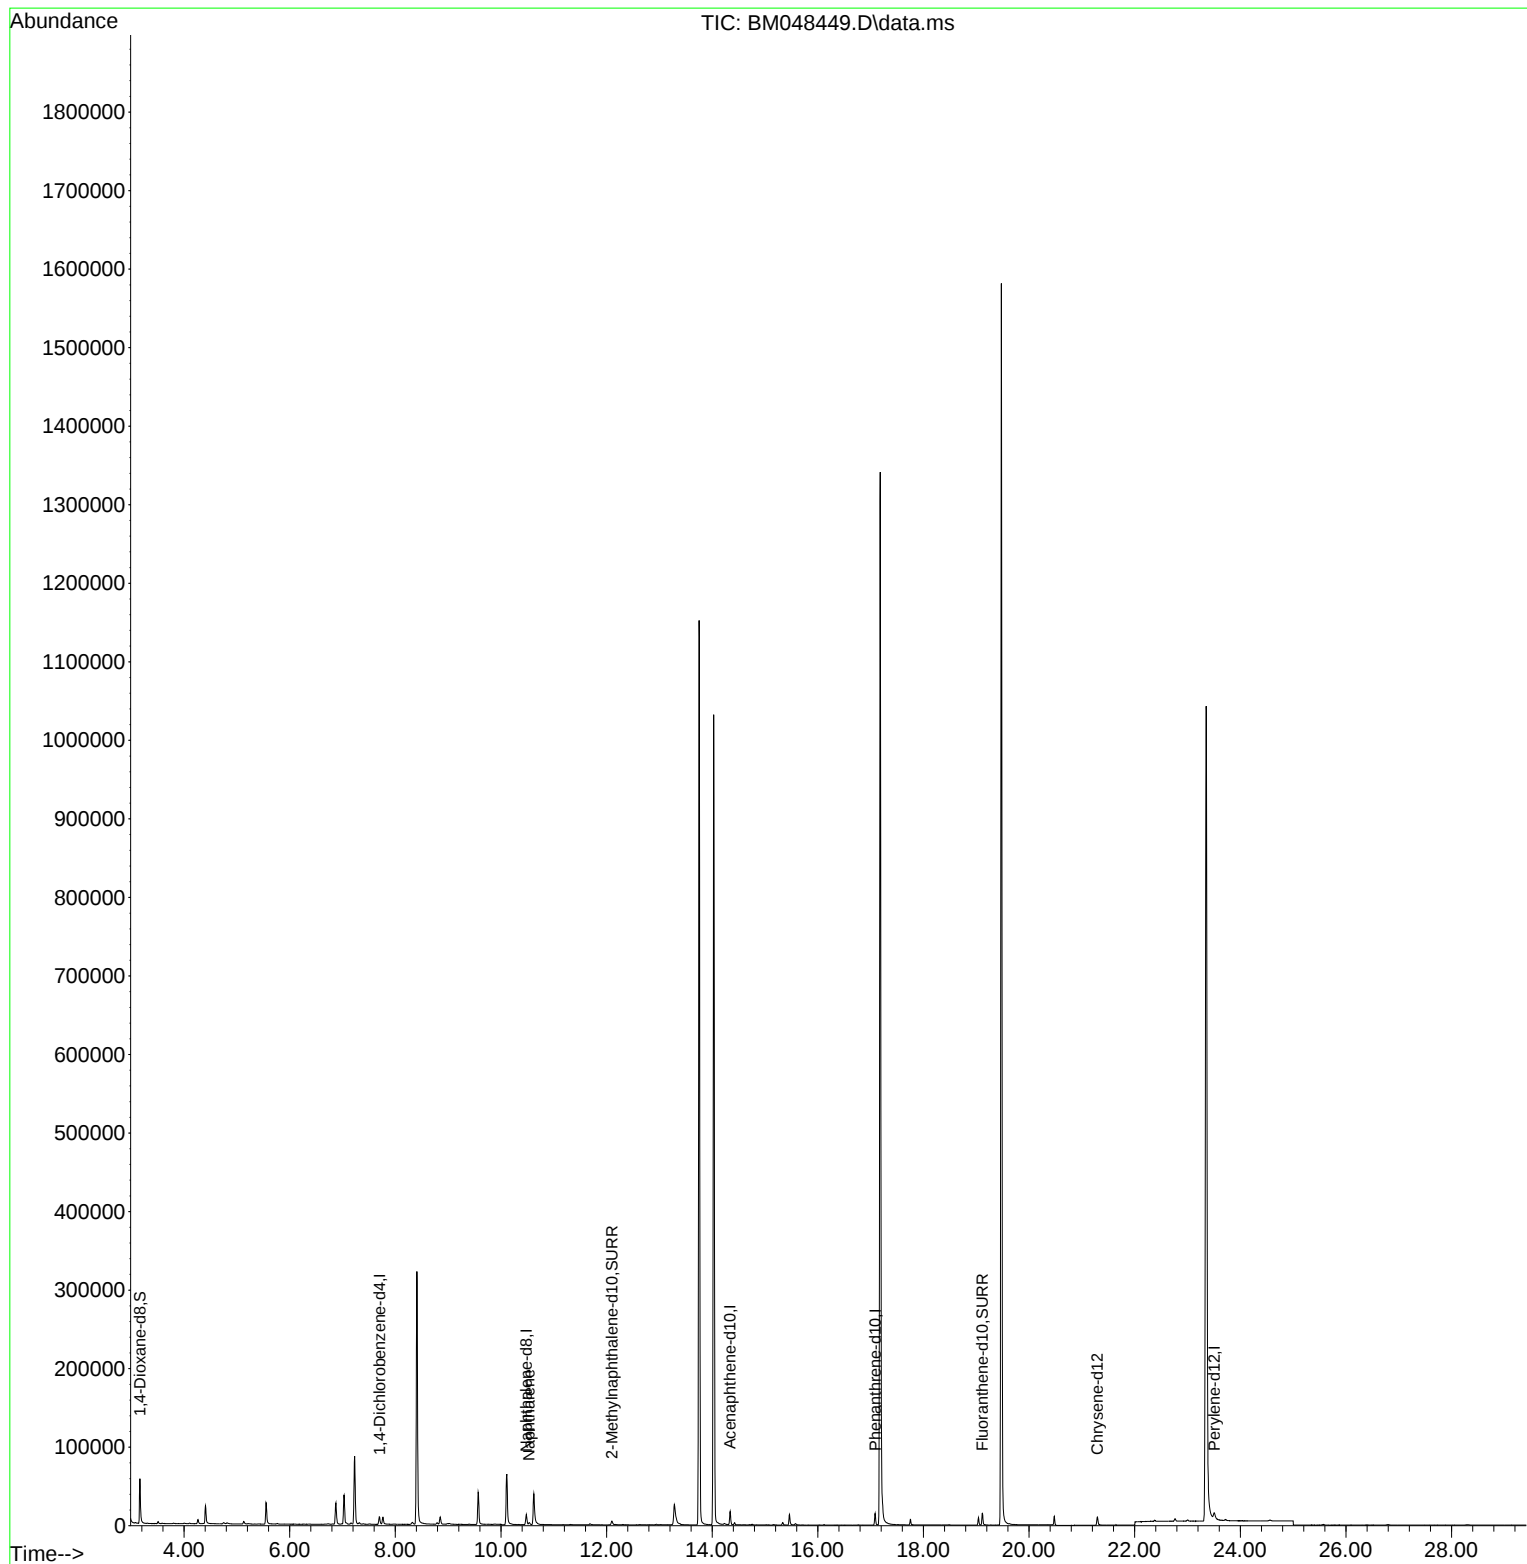

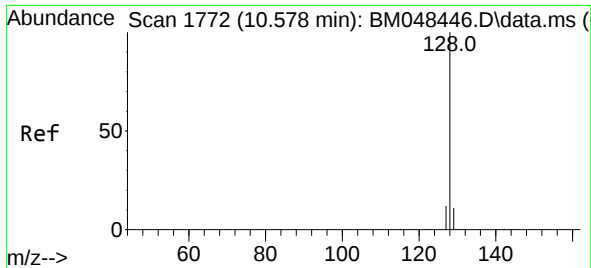

#5
Naphthalene
Concen: 0.044 ng/ul
RT: 10.529 min Scan# 1772
Delta R.T. -0.051 min
Lab File: BM048449.D
Acq: 05 Nov 2024 05:18

Instrument :
BNA_M
ClientSampleId :
C0AC8

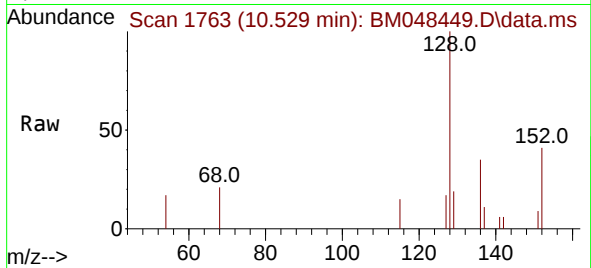

Tgt Ion:128 Resp: 2037
Ion Ratio Lower Upper
128 100
129 19.3 10.6 15.8
127 16.9 11.4 17.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/05/2024
Supervised By :mohammad ahmed 11/06/2024

