

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110424\
 Data File : BM048459.D
 Acq On : 05 Nov 2024 15:37
 Operator : RC/JU
 Sample : P4625-17
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/05/2024
 Supervised By :mohammad ahmed 11/06/2024

Quant Time: Nov 05 16:34:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 05 05:12:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	3751	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.480	136	11725	0.400	ng/ul	-0.05
9) Acenaphthene-d10	14.340	164	6367	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.086	188	12368m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.298	240	9294m	0.400	ng/ul	0.00
23) Perylene-d12	23.507	264	6027m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	21253	4.613	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.108	152	4638	0.311	ng/ul	-0.03
18) Fluoranthene-d10	19.118	212	9934	0.421	ng/ul	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.530	128	1174	0.038	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110424\
Data File : BM048459.D
Acq On : 05 Nov 2024 15:37
Operator : RC/JU
Sample : P4625-17
Misc :
ALS Vial : 41 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AC8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/05/2024
Supervised By :mohammad ahmed 11/06/2024


Quant Time: Nov 05 16:34:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 05 05:12:02 2024
Response via : Initial Calibration

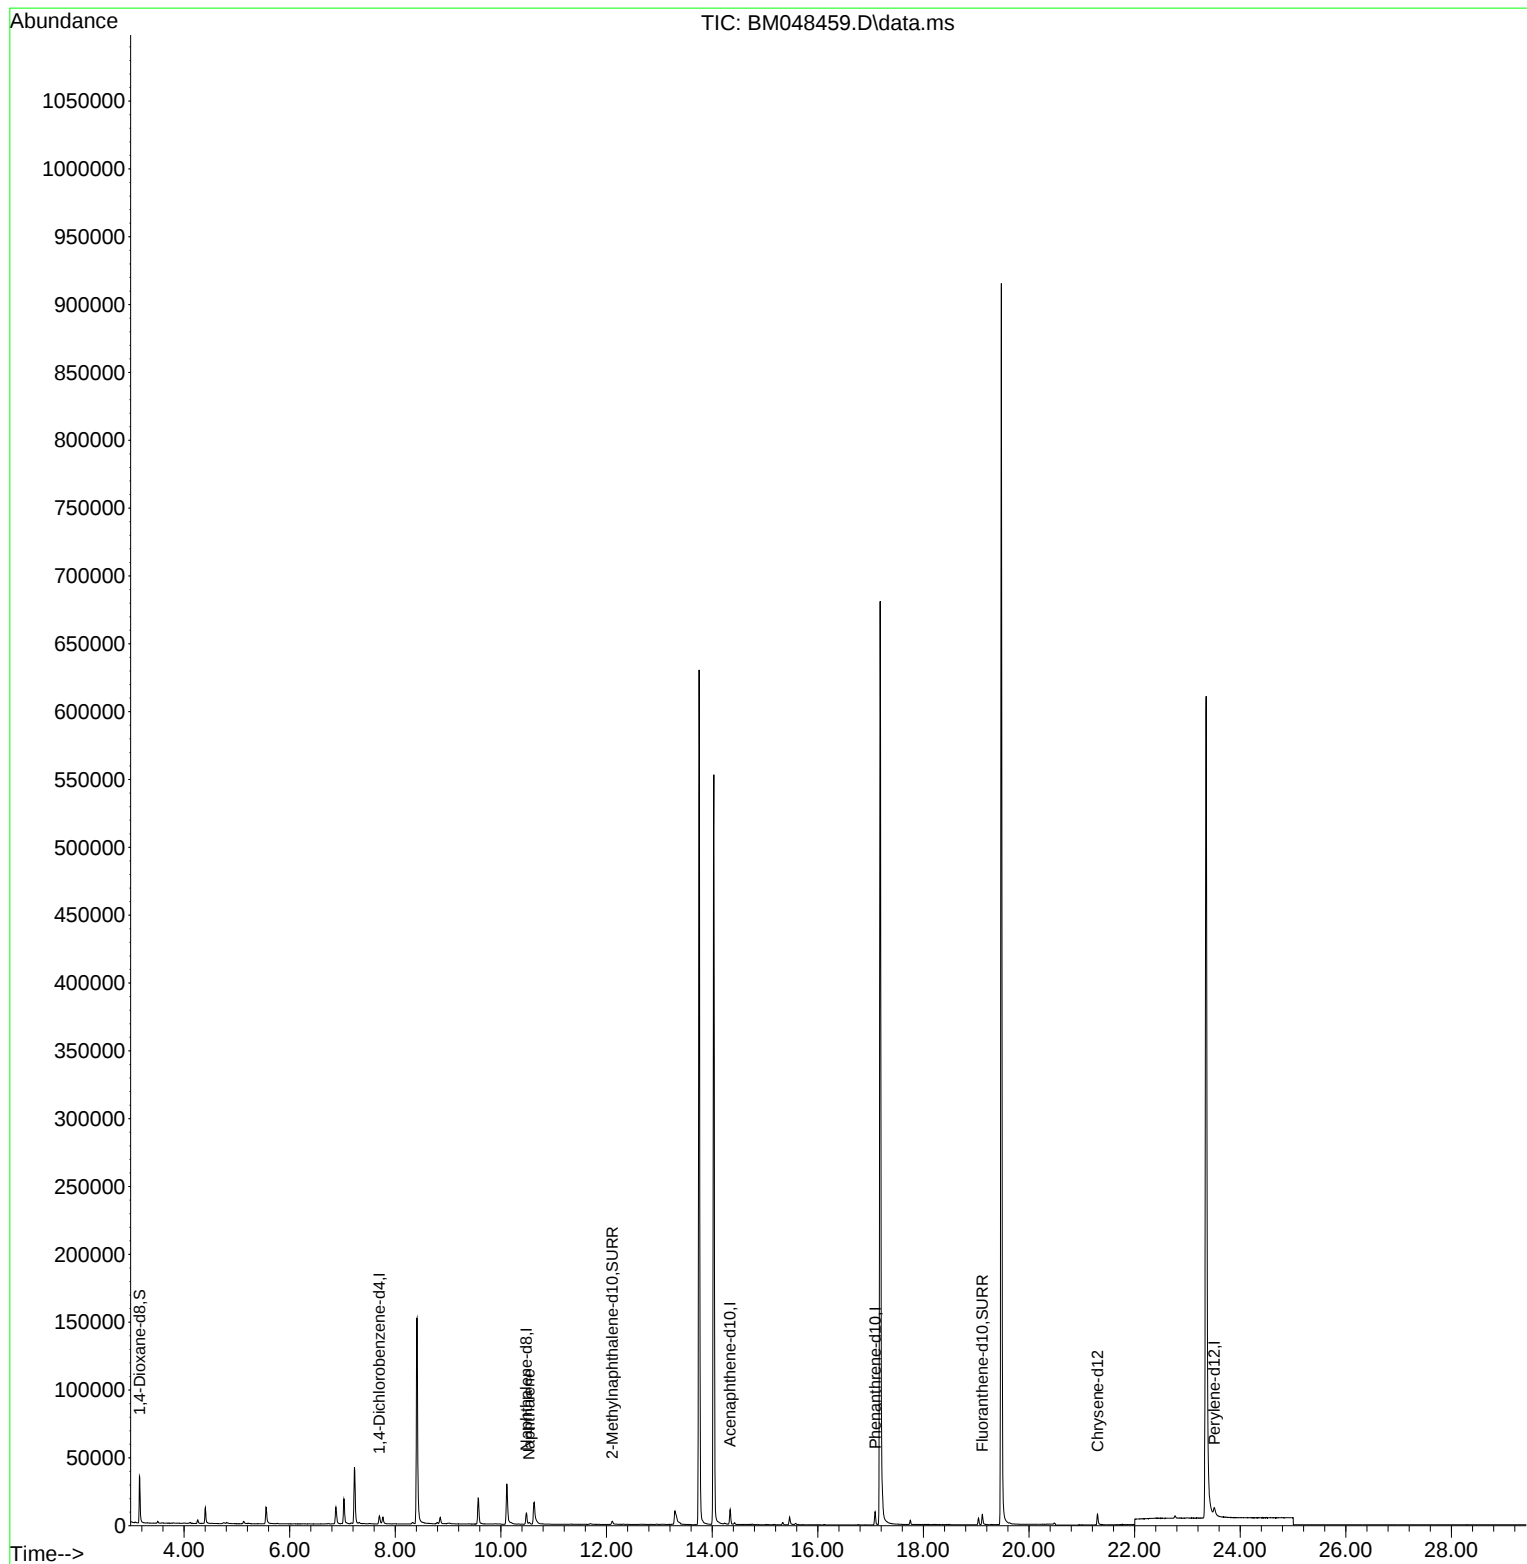

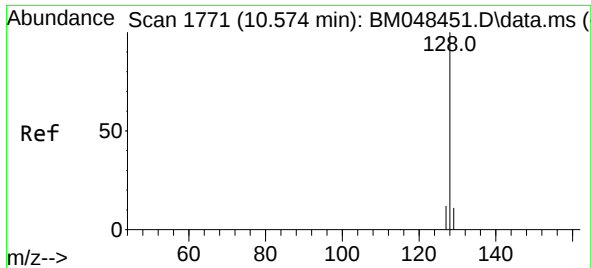

#5
Naphthalene
Concen: 0.038 ng/ul
RT: 10.530 min Scan# 1174
Delta R.T. -0.050 min
Lab File: BM048459.D
Acq: 05 Nov 2024 15:37

Instrument :
BNA_M
ClientSampleId :
C0AC8

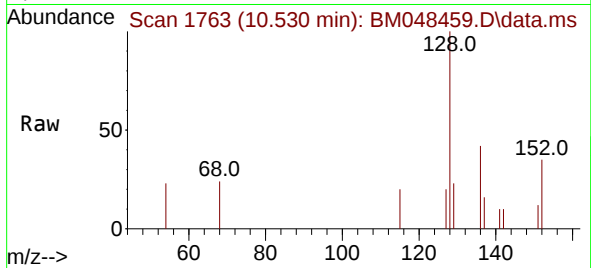

Tgt Ion:128 Resp: 1174
Ion Ratio Lower Upper
128 100
129 23.4 10.6 15.8
127 20.1 11.4 17.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/05/2024
Supervised By :mohammad ahmed 11/06/2024

