


Data Path : Z:\HPCHEM1\BNA M\DATA\BM110515\
 Data File : BM003058.D
 Acq On : 05 Nov 2015 10:42
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM110415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 05 10:29:18 2015

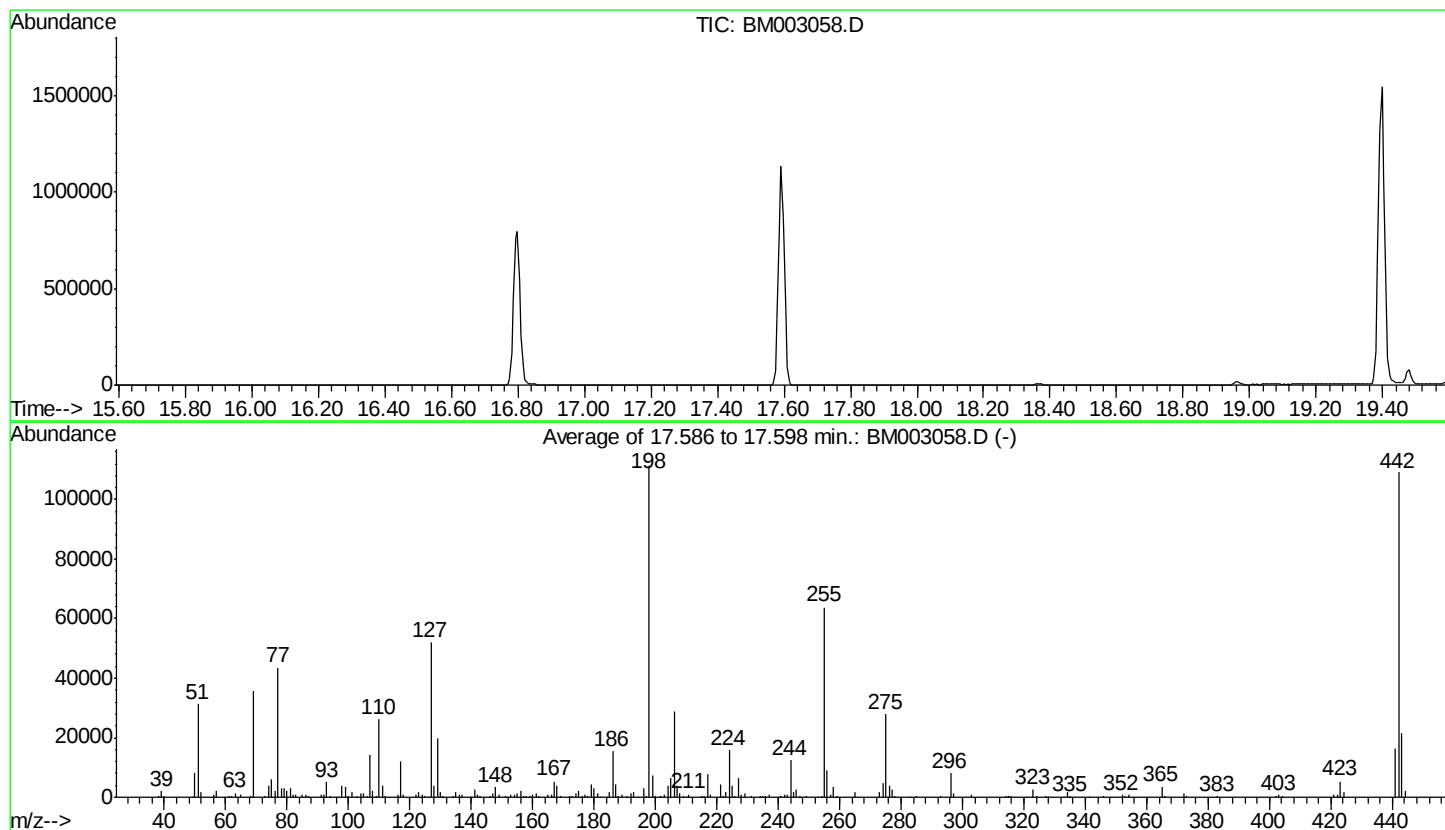

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	31274	PASS
68	69	0.00	2	1.8	628	PASS
69	198	0.00	100	32.1	35784	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	51970	PASS
197	198	0.00	2	0.4	480	PASS
198	198	100	100	100.0	111389	PASS
199	198	5	9	6.7	7516	PASS
275	198	10	60	24.9	27784	PASS
365	198	1	100	3.2	3549	PASS
441	442	0.01	24	14.8	16197	PASS
442	198	50	100	98.1	109280	PASS
443	442	15	24	19.5	21360	PASS