

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110517\
 Data File : BM012744.D
 Acq On : 05 Nov 2017 18:06
 Operator : SJ/JU
 Sample : PB103865BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Quant Time: Nov 06 06:46:05 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 06 06:44:10 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	73666	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	323378	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	229691	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	602514	20.00	ng/ul	0.00
77) Chrysene-d12	21.37	240	774938	20.00	ng/ul	0.00
85) Perylene-d12	23.66	264	720845	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	9014	6.61	ng/uL	0.00
5) Phenol-d5	6.99	99	186714	34.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	106941	36.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	162156	35.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	170077	35.95	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	84031	35.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	102262	37.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	183195	32.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	252326	46.65	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	734724	38.65	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	826463	35.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	120230	39.48	ng/ul	0.00
57) Fluorene-d10	15.44	176	607978	37.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	97400	24.49	ng/ul	0.00
70) Anthracene-d10	17.29	188	1079345	37.08	ng/ul	0.00
78) Pyrene-d10	19.59	212	1312537	36.50	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.52	264	1346081	39.49	ng/ul	0.00

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.52	70	3742	1.09	ng/ul#	1
45) 2,6-Dinitrotoluene	13.86	165	5112	1.35	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110517\
Data File : BM012744.D
Acq On : 05 Nov 2017 18:06
Operator : SJ/JU
Sample : PB103865BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Quant Time: Nov 06 06:46:05 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 06 06:44:10 2017
Response via : Initial Calibration

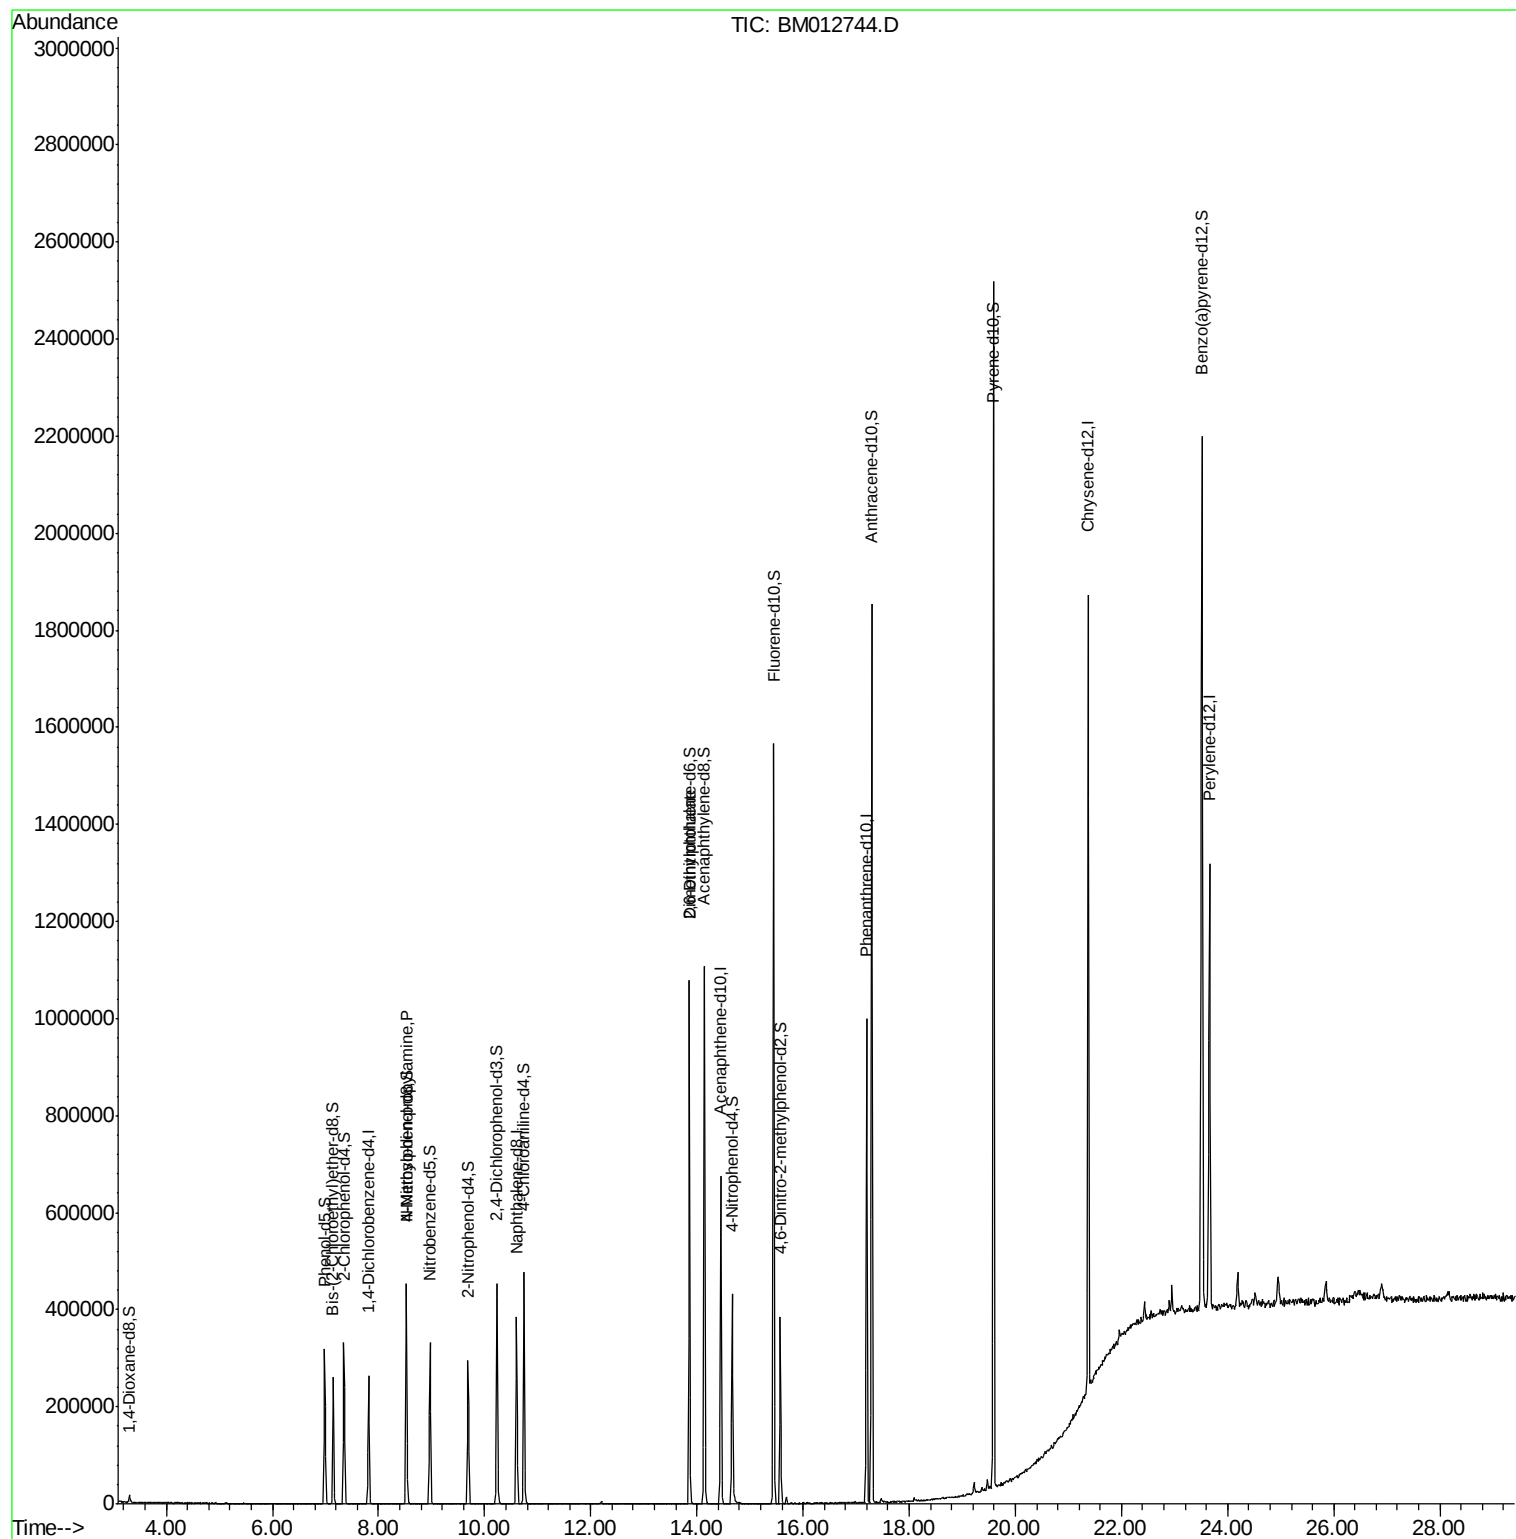

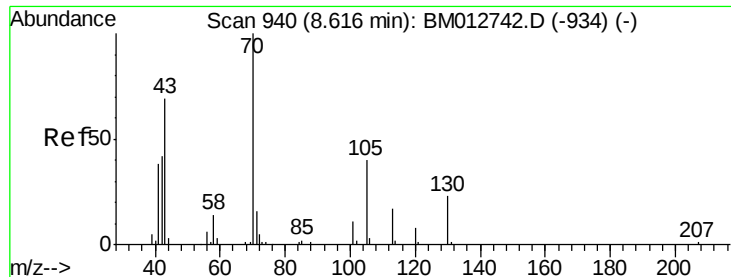

#15

N-Nitroso-di-n-propylamine

Concen: 1.09 ng/ul

RT: 8.52 min Scan# 924

Delta R.T. -0.09 min

Lab File: BM012744.D

Acq: 05 Nov 2017 18:06

Instrument :

BNA_M

ClientSampleId :

SBLK65

Tot Ion: 70 Resp: 3742


Ion Ratio Lower Upper

70 100

42 288.7 35.4 53.0#

101 0.0 8.4 12.6#

130 0.0 18.2 27.4#



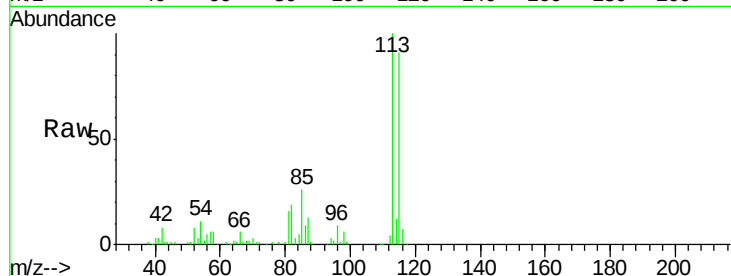


Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

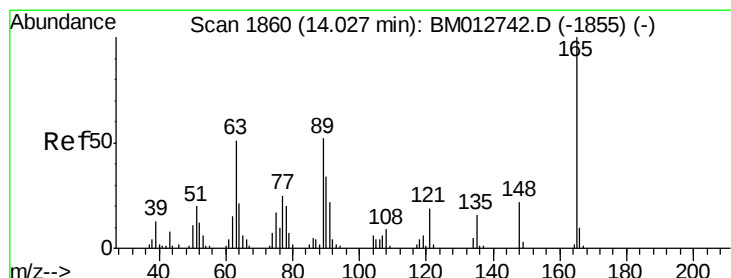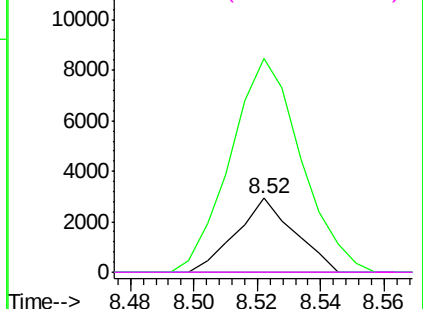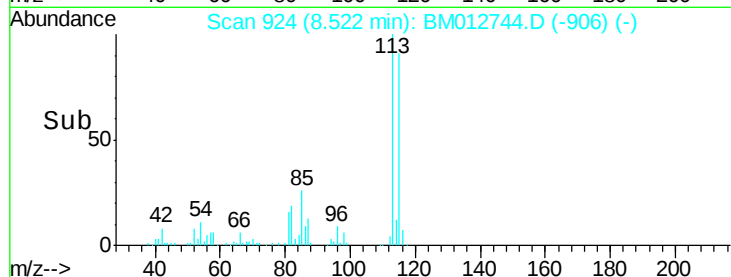

#45

2,6-Dinitrotoluene

Concen: 1.35 ng/ul

RT: 13.86 min Scan# 1832

Delta R.T. -0.16 min

Lab File: BM012744.D

Acq: 05 Nov 2017 18:06


Tgt Ion:165 Resp: 5112

Ion Ratio Lower Upper

165 100

89 0.0 42.4 63.6#

121 17.5 16.6 24.8

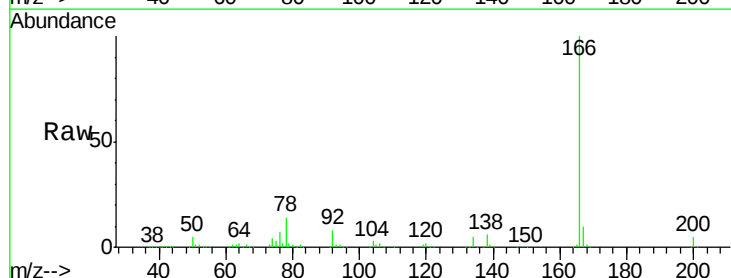

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

