

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110517\
 Data File : BM012747.D
 Acq On : 05 Nov 2017 19:53
 Operator : SJ/JU
 Sample : I6154-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDEE7

Quant Time: Nov 06 06:46:37 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 06 06:44:10 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	117488	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	510191	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	355287	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	898198	20.00	ng/ul	0.00
77) Chrysene-d12	21.37	240	879549	20.00	ng/ul	0.00
85) Perylene-d12	23.66	264	727902	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	15971	7.34	ng/uL	0.00
5) Phenol-d5	6.99	99	60710	6.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	161387	34.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	200059	27.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	130141	17.25	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	131515	34.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	159906	37.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	267248	30.22	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	463	0.05	ng/ul	-0.13
43) Dimethylphthalate-d6	13.86	166	1109438	37.74	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	1249491	34.36	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	33960	7.21	ng/ul	0.00
57) Fluorene-d10	15.44	176	946838	37.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	162705	27.44	ng/ul	0.00
70) Anthracene-d10	17.29	188	1596226	36.78	ng/ul	0.00
78) Pyrene-d10	19.59	212	1737543	42.57	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.51	264	1339184	38.91	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) 2,6-Dinitrotoluene	13.86	165	8912	1.53	ng/ul#	43




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110517\
Data File : BM012747.D
Acq On : 05 Nov 2017 19:53
Operator : SJ/JU
Sample : I6154-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDEE7

Quant Time: Nov 06 06:46:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 06 06:44:10 2017
Response via : Initial Calibration

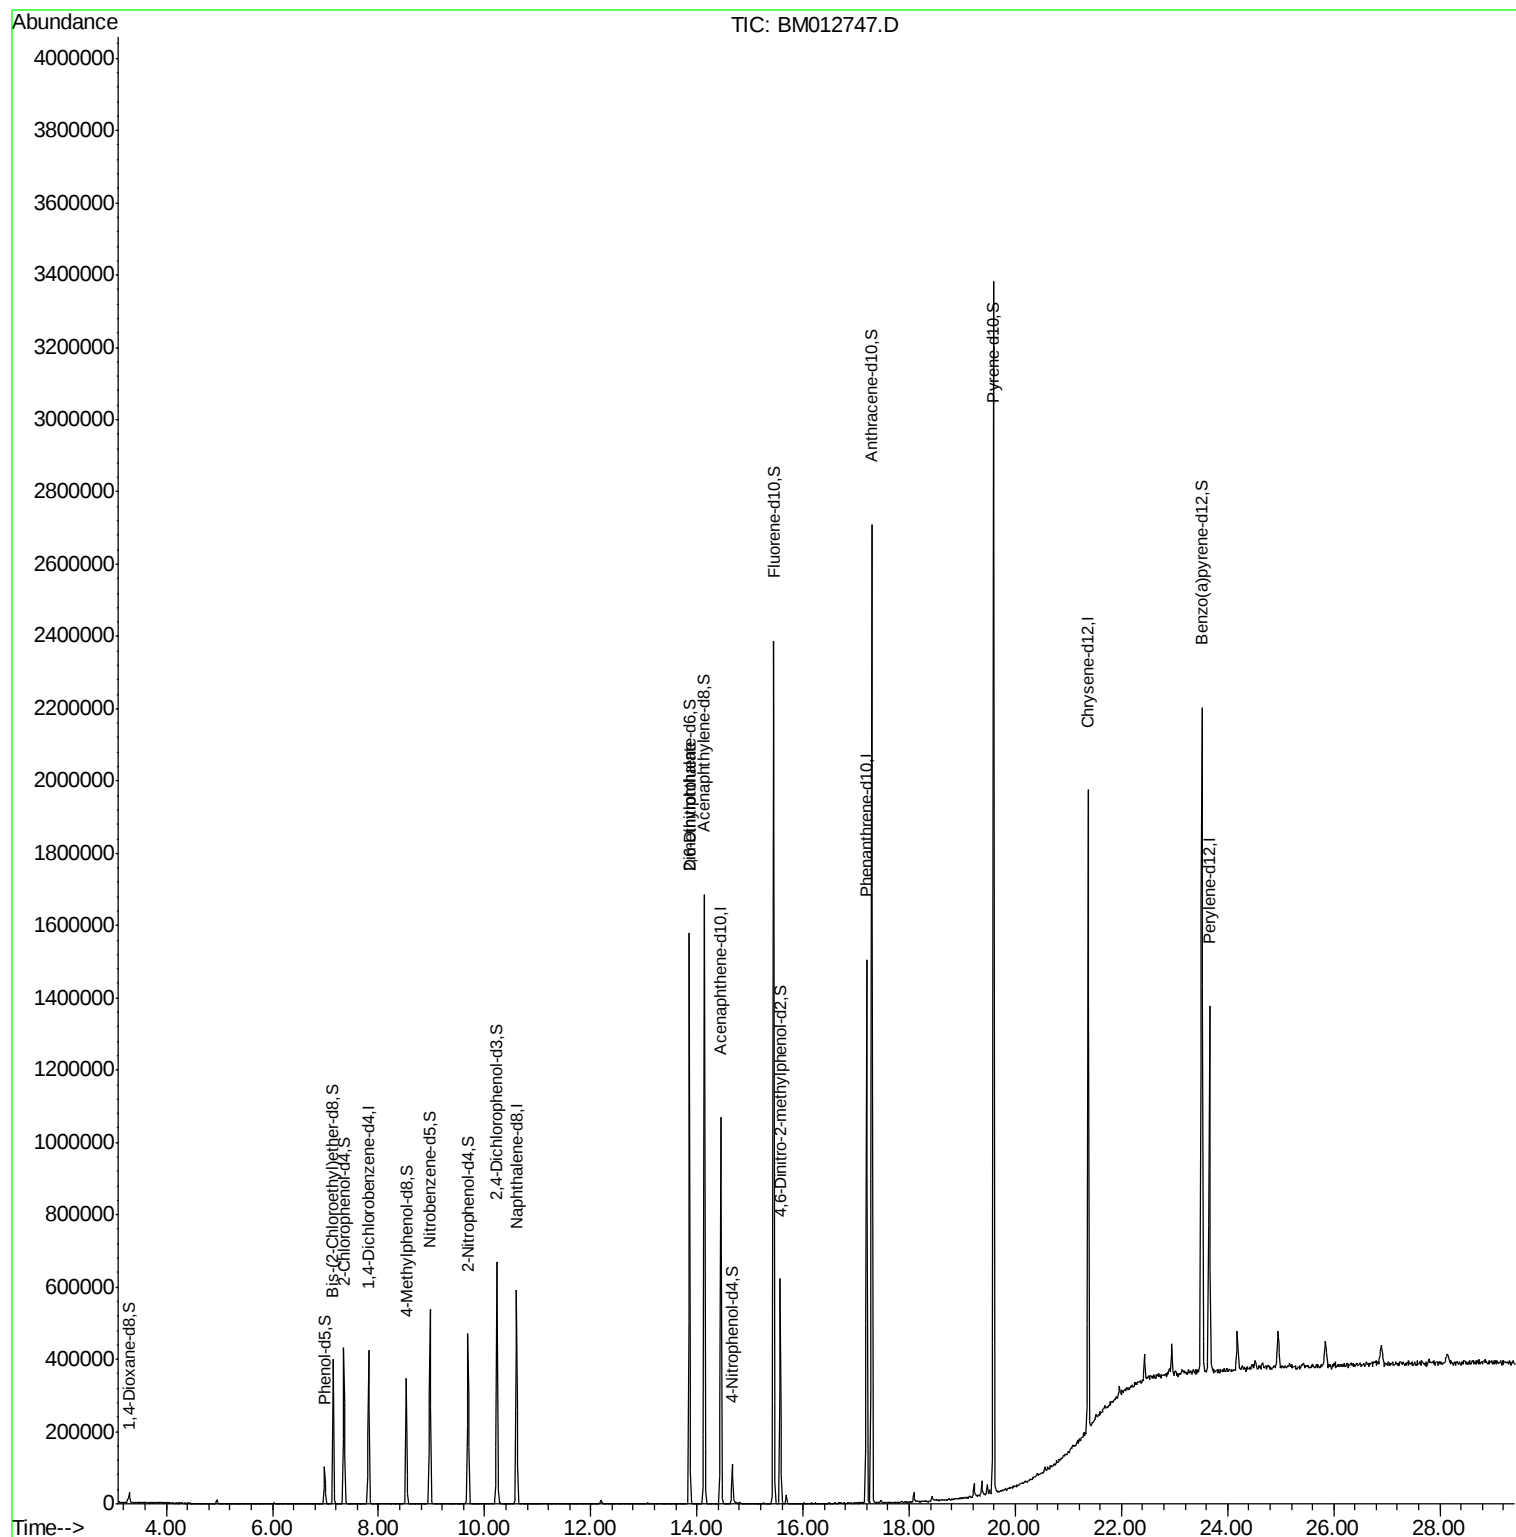

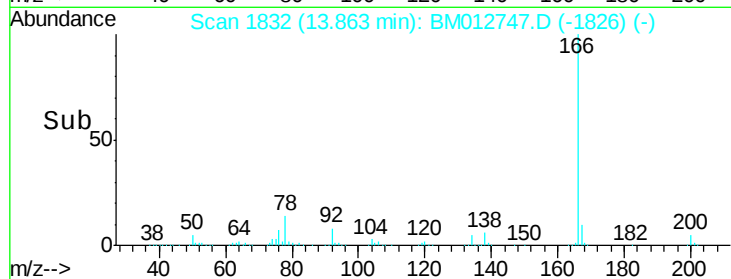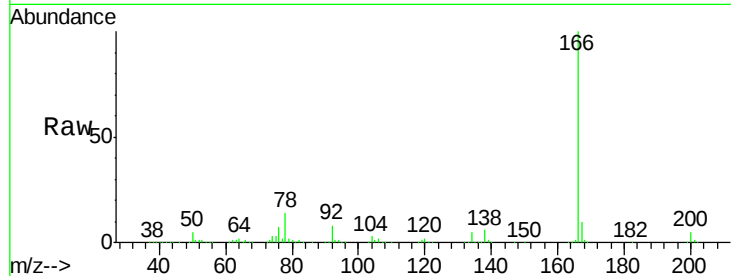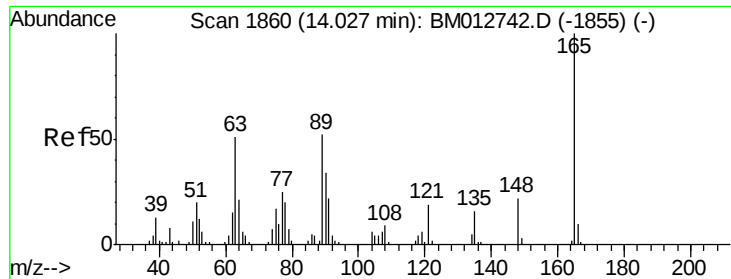

#45

2,6-Dinitrotoluene

Concen: 1.53 ng/ul

RT: 13.86 min Scan# 1832

Delta R.T. -0.16 min

Lab File: BM012747.D

Acq: 05 Nov 2017 19:53

Instrument :

BNA_M

ClientSampleId :

BDEE7

Tot Ion:165 Resp: 8912

Ion Ratio Lower Upper

165 100

89 0.0 42.4 63.6#

121 16.0 16.6 24.8#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

