


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110620\
Data File : BM027726.D
Acq On : 06 Nov 2020 09:01
Operator : JU/CG
Sample : DFTPP85
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP861

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 06 11:00:57 2020

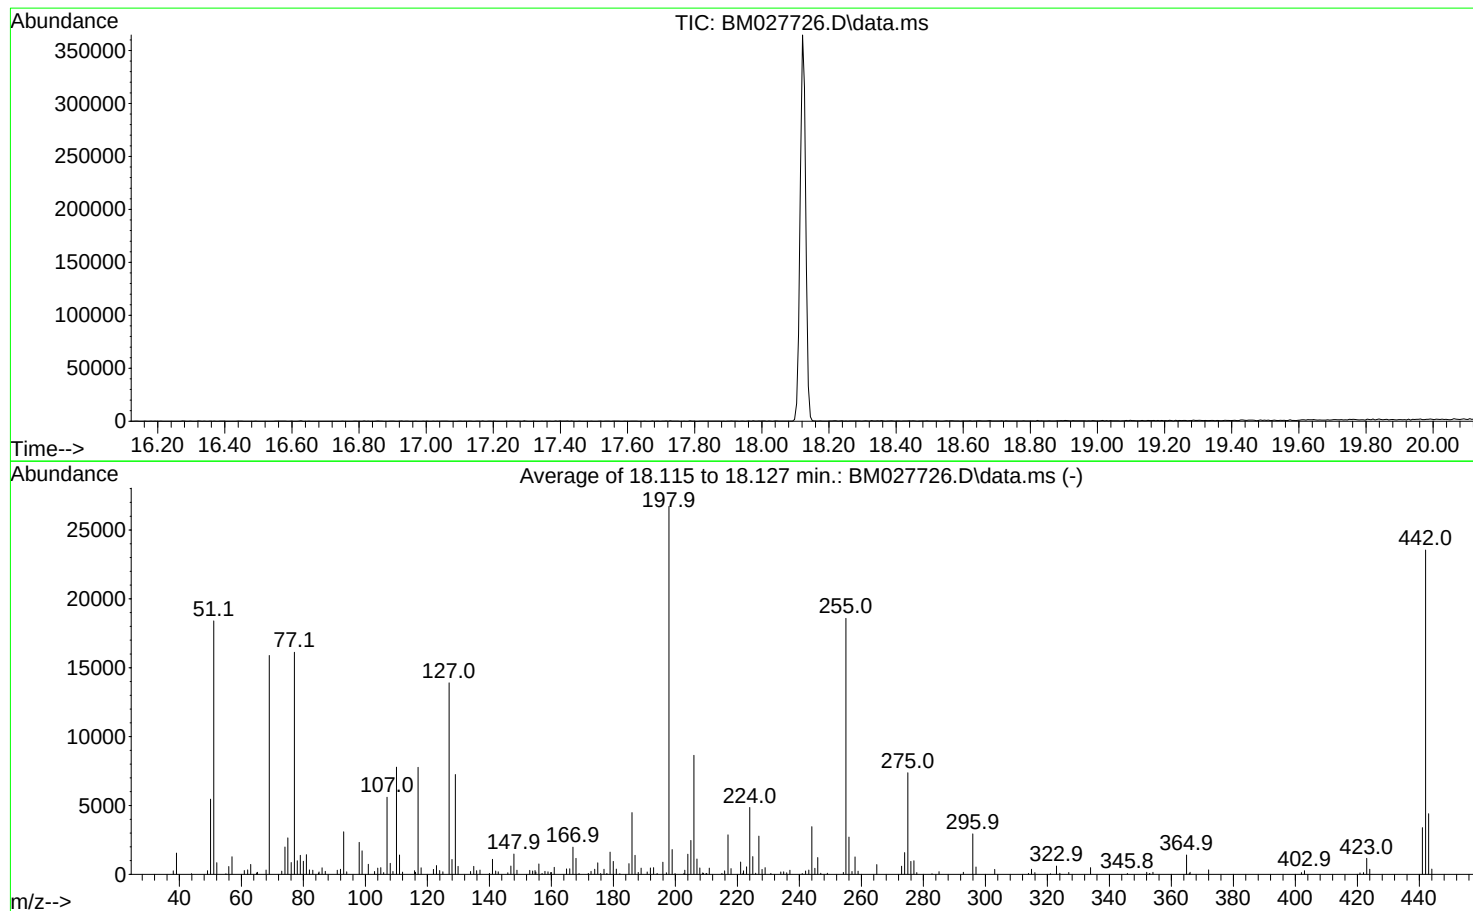

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.9	18403	PASS
68	69	0.00	2	1.9	309	PASS
69	198	0.00	100	59.5	15889	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.1	13904	PASS
197	198	0.00	2	0.4	114	PASS
198	198	100	100	100.0	26704	PASS
199	198	5	9	6.7	1801	PASS
275	198	10	60	27.6	7379	PASS
365	198	1	100	5.3	1407	PASS
441	198	0.01	100	12.7	3393	PASS
442	198	50	100	88.2	23549	PASS
443	442	15	24	18.7	4402	PASS

m/z	Abundance
206.90	217.0

Instrument :
BNA_M
ClientSampleId :
DFTPP861

m/z	Abundance
38.00	182.0
39.00	1413.0
49.10	202.0
50.00	4955.0
51.10	17088.0
52.00	764.0
55.00	154.0
55.90	598.0
57.00	1070.0
61.00	245.0
62.00	197.0
63.00	704.0
65.20	188.0
68.00	333.0
69.00	13909.0
73.00	264.0
74.00	1725.0
75.00	2287.0
76.00	811.0
77.10	13925.0
78.00	858.0
79.00	1356.0
80.00	741.0
81.00	1280.0
82.00	206.0
83.10	196.0
84.90	265.0
86.00	463.0
87.10	194.0
91.10	176.0
91.90	356.0
93.00	2738.0
94.00	189.0
98.00	2129.0
99.00	1818.0
100.90	661.0
103.00	179.0
104.00	397.0
104.90	420.0
106.00	198.0
107.00	4537.0
108.00	582.0
109.00	206.0
110.00	6897.0
111.00	1014.0
112.00	184.0
115.80	215.0
116.20	191.0
117.00	6516.0
117.90	268.0
121.90	271.0
122.90	545.0
124.00	298.0
127.00	11208.0
127.90	667.0
129.00	6080.0
129.90	418.0
133.90	204.0
135.00	472.0
135.80	207.0
137.00	325.0
141.00	768.0
142.00	188.0
142.80	156.0
147.00	479.0
147.90	1212.0
148.90	286.0
153.00	211.0
154.00	153.0
154.70	324.0
155.90	494.0
157.90	163.0
159.00	165.0
159.80	150.0
160.90	424.0
164.80	361.0
165.90	364.0
166.90	1420.0
168.00	973.0
172.90	196.0
174.10	306.0
175.00	736.0
177.00	282.0
178.90	982.0
180.00	718.0
181.00	351.0
185.00	660.0
186.00	3530.0
187.00	1091.0
189.00	380.0
192.00	359.0
192.90	296.0

Instrument :
BNA_M
ClientSampleId :
DFTPP861

196.00	507.0
197.90	19832.0
199.00	1299.0
202.80	199.0
203.10	189.0
204.00	1256.0
205.00	1800.0
206.00	5875.0
207.00	1146.0
208.00	363.0
209.90	168.0
210.90	311.0
215.90	185.0
217.00	2719.0
217.90	251.0
221.10	852.0
221.80	244.0
222.90	322.0
224.00	3555.0
224.90	953.0
227.00	2180.0
227.90	280.0
229.00	241.0
235.00	151.0
236.90	305.0
240.90	158.0
242.10	150.0
243.00	237.0
244.00	2513.0
245.00	301.0
245.90	918.0
255.00	13387.0
256.00	1800.0
257.10	200.0
258.00	872.0
258.90	269.0
264.90	386.0
272.90	430.0
273.90	904.0
275.00	5371.0
275.90	672.0
277.00	845.0
285.10	196.0
296.00	1630.0
296.90	403.0
303.10	349.0
314.80	307.0
323.00	340.0
334.00	222.0
352.90	188.0
364.90	779.0
366.10	219.0
372.00	191.0
402.80	151.0
423.00	691.0
424.10	263.0
441.00	1783.0
442.00	13655.0
443.00	2755.0
444.00	187.0

Instrument :
BNA_M
ClientSampleId :
DFTPP861

m/z	Abundance
38.00	400.0
39.10	1843.0
43.90	156.0
48.90	224.0
49.20	195.0
50.00	6416.0
51.10	21592.0
52.00	1010.0
56.00	579.0
57.00	1432.0
61.00	351.0
62.00	486.0
63.00	853.0
65.10	277.0
68.00	324.0
69.00	19128.0
73.00	250.0
74.00	2389.0
75.00	3094.0
76.10	1028.0
77.10	19328.0
78.10	1326.0
79.00	1562.0
80.00	1185.0
80.90	1801.0
82.00	488.0
83.00	379.0
85.10	223.0
86.00	501.0
87.00	227.0
90.90	471.0
92.00	410.0
93.00	3637.0
93.90	194.0
98.00	2876.0
98.90	1772.0
101.00	807.0
102.90	245.0
104.00	511.0
105.00	546.0
105.80	171.0
107.00	6730.0
108.00	986.0
108.90	177.0
110.00	8946.0
111.00	1789.0
112.00	305.0
115.90	586.0
117.00	9263.0
118.00	658.0
122.00	501.0
123.00	812.0
123.90	257.0
125.00	321.0
127.00	17344.0
128.00	1409.0
129.00	8529.0
129.90	855.0
134.00	217.0
135.00	745.0
135.90	346.0
136.90	424.0
140.00	197.0
141.00	1318.0
142.10	262.0
142.90	238.0
145.90	194.0
146.90	806.0
147.90	1669.0
148.90	369.0
152.90	438.0
153.90	325.0
155.00	541.0
156.00	965.0
157.00	201.0
157.80	314.0
158.90	232.0
160.00	407.0
160.90	533.0
164.90	432.0
166.00	432.0
167.00	2506.0
168.00	1419.0
168.90	190.0
171.90	221.0
172.80	238.0
173.90	371.0
174.90	906.0
176.90	387.0
178.90	2013.0
180.00	1074.0
180.90	372.0

Instrument :
BNA_M
ClientSampleId :
DFTPP861

182.10	152.0
185.00	947.0
186.00	5767.0
187.00	1387.0
188.00	238.0
188.90	532.0
190.90	211.0
191.90	616.0
192.90	652.0
194.10	195.0
195.90	1099.0
197.10	342.0
198.00	31928.0
199.00	2149.0
199.90	173.0
203.00	390.0
204.00	1530.0
205.00	2789.0
206.00	10502.0
206.90	1419.0
207.90	653.0
208.80	324.0
210.10	194.0
211.00	698.0
215.90	314.0
216.90	2983.0
217.90	482.0
221.00	988.0
222.00	464.0
223.00	765.0
224.00	5637.0
224.90	1616.0
225.90	257.0
227.00	3006.0
227.90	470.0
228.90	651.0
230.80	226.0
234.00	157.0
234.90	232.0
236.00	171.0
237.00	377.0
242.00	320.0
243.10	425.0
244.00	3892.0
245.00	559.0
246.00	1508.0
246.90	246.0
249.00	256.0
254.20	212.0
255.00	21456.0
256.00	3210.0
256.90	223.0
257.90	1579.0
259.00	216.0
264.90	1061.0
273.00	682.0
274.00	1850.0
275.00	8787.0
276.00	1316.0
276.90	958.0
277.90	151.0
282.80	153.0
285.00	211.0
292.90	271.0
296.00	3276.0
296.90	623.0
302.90	333.0
314.90	462.0
315.90	215.0
321.00	153.0
323.00	825.0
327.00	257.0
333.90	633.0
345.80	213.0
352.10	232.0
353.10	150.0
354.10	219.0
364.90	1828.0
365.80	209.0
372.10	473.0
402.00	184.0
402.90	226.0
420.90	165.0
422.00	210.0
423.00	1180.0
423.90	412.0
441.00	4018.0
442.00	27856.0
443.00	5106.0
444.10	375.0

Instrument :
BNA_M
ClientSampleId :
DFTPP861

m/z	Abundance
38.00	194.0
39.10	1388.0
49.00	174.0
50.10	5010.0
51.10	16528.0
52.10	773.0
55.90	514.0
56.90	1330.0
60.90	229.0
62.00	284.0
63.00	619.0
64.90	306.0
67.90	271.0
69.00	14631.0
73.00	168.0
74.10	1842.0
75.00	2579.0
76.00	732.0
77.10	15100.0
78.00	774.0
79.00	1236.0
80.00	917.0
81.00	1222.0
81.90	270.0
83.00	326.0
85.00	314.0
86.00	453.0
87.00	257.0
90.90	277.0
91.90	349.0
93.00	2909.0
94.00	168.0
98.00	1960.0
99.00	1524.0
101.00	742.0
102.90	196.0
104.00	470.0
104.90	489.0
107.00	5526.0
108.00	828.0
108.80	259.0
110.00	7514.0
111.00	1403.0
116.10	252.0
117.00	7529.0
118.00	509.0
121.90	317.0
123.00	568.0
123.90	283.0
125.00	251.0
127.00	13160.0
127.90	1151.0
129.00	7122.0
129.90	471.0
133.80	211.0
134.90	525.0
136.00	242.0
137.00	196.0
141.00	1194.0
142.00	297.0
142.80	171.0
146.00	154.0
146.90	532.0
147.90	1539.0
148.90	244.0
153.10	218.0
154.00	273.0
154.80	529.0
156.00	800.0
158.00	194.0
158.80	156.0
159.80	246.0
160.90	569.0
165.00	387.0
165.90	432.0
167.00	1989.0
167.90	1098.0
172.70	240.0
174.00	454.0
175.00	853.0
175.90	169.0
176.90	450.0
177.90	224.0
179.00	1849.0
179.90	1022.0
181.00	435.0
185.00	717.0
186.00	4166.0
187.00	1652.0
188.00	166.0
188.90	457.0
190.90	306.0

Instrument :
BNA_M
ClientSampleId :
DFTPP861

191.90	425.0
193.00	517.0
195.90	1043.0
198.00	28352.0
198.90	1954.0
203.00	335.0
204.00	1611.0
205.00	2790.0
206.00	9556.0
207.10	1423.0
207.80	395.0
209.00	255.0
210.90	339.0
215.00	198.0
215.90	285.0
216.90	2918.0
218.00	508.0
221.00	848.0
222.00	299.0
223.00	557.0
224.00	5380.0
225.00	1316.0
226.90	3129.0
228.00	321.0
228.90	572.0
234.00	357.0
234.90	181.0
235.80	192.0
237.00	242.0
241.90	273.0
243.00	275.0
244.00	3963.0
245.00	476.0
246.00	1244.0
254.20	223.0
255.00	20920.0
256.00	3100.0
256.90	198.0
258.00	1364.0
259.00	228.0
265.00	670.0
272.90	654.0
274.00	1972.0
275.00	7980.0
275.90	829.0
276.90	1169.0
277.90	245.0
285.10	193.0
292.90	175.0
295.90	3901.0
297.00	580.0
303.00	385.0
313.90	209.0
315.00	333.0
316.00	153.0
322.90	651.0
324.00	238.0
326.80	178.0
334.00	615.0
352.00	239.0
354.00	221.0
364.90	1614.0
366.00	240.0
371.90	308.0
401.90	215.0
403.00	410.0
420.80	156.0
422.00	176.0
423.00	1612.0
424.00	433.0
441.00	4379.0
442.00	29136.0
443.00	5344.0
444.00	589.0

Instrument :
BNA_M
ClientSampleId :
DFTPP861