




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110624\
Data File : BM048480.D
Acq On : 06 Nov 2024 16:55
Operator : RC/JU
Sample : P4634-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0PI6

Manual IntegrationsAPPROVED

Quant Time: Nov 06 17:36:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 14:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :mohammad ahmed 11/11/2024

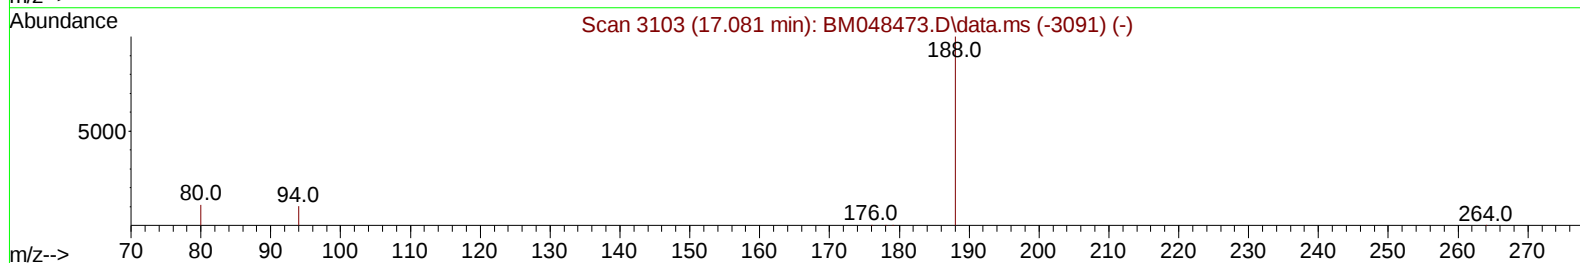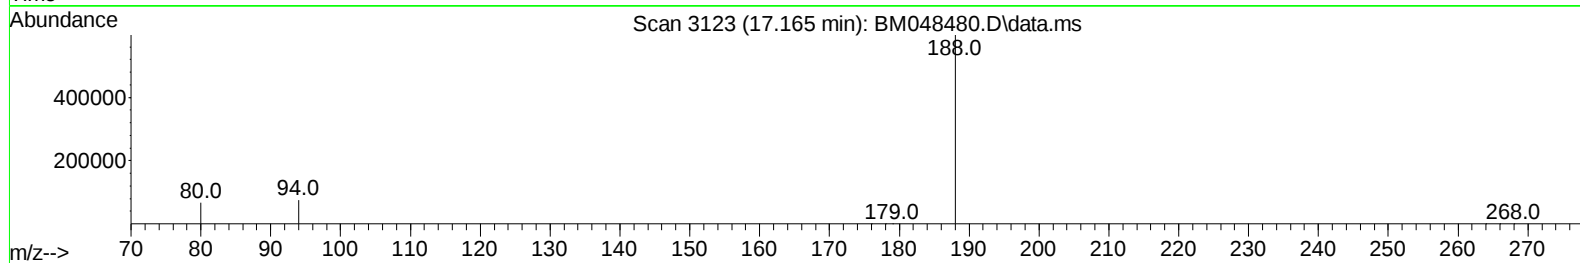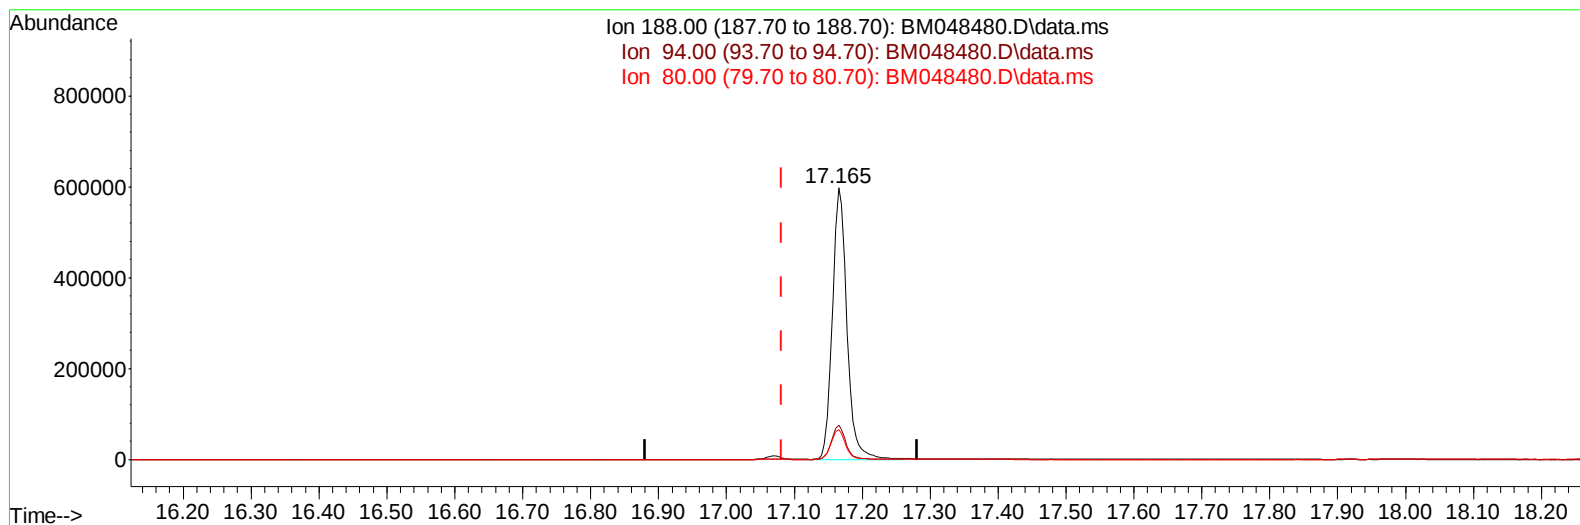

TIC: BM048480.D\data.ms

(13) Phenanthrene-d10 (I)

17.165min (+ 0.084) 0.40 ng/u1

response 885649

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	12.58
80.00	12.60	11.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110624\
Data File : BM048480.D
Acq On : 06 Nov 2024 16:55
Operator : RC/JU
Sample : P4634-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0PI6

Manual IntegrationsAPPROVED

Quant Time: Nov 06 17:36:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 14:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :mohammad ahmed 11/11/2024

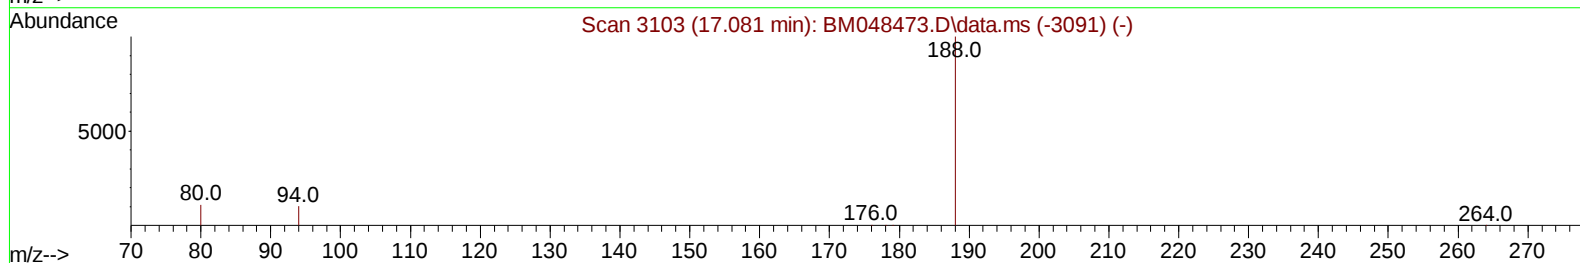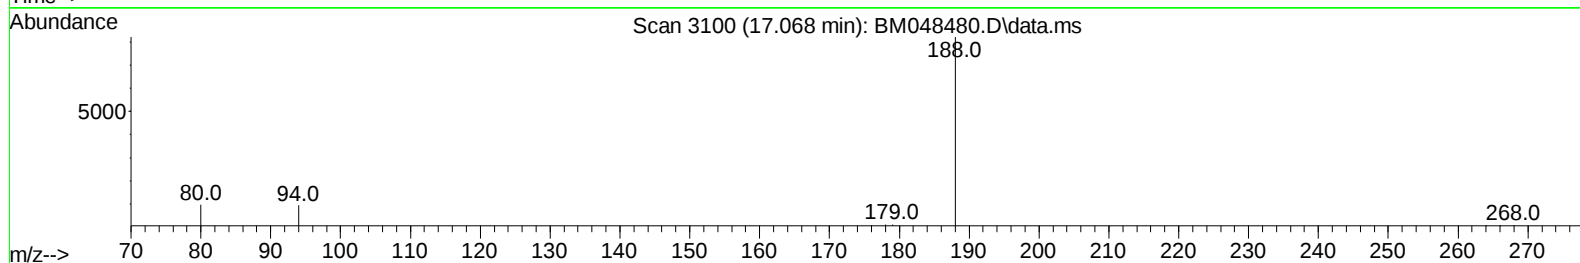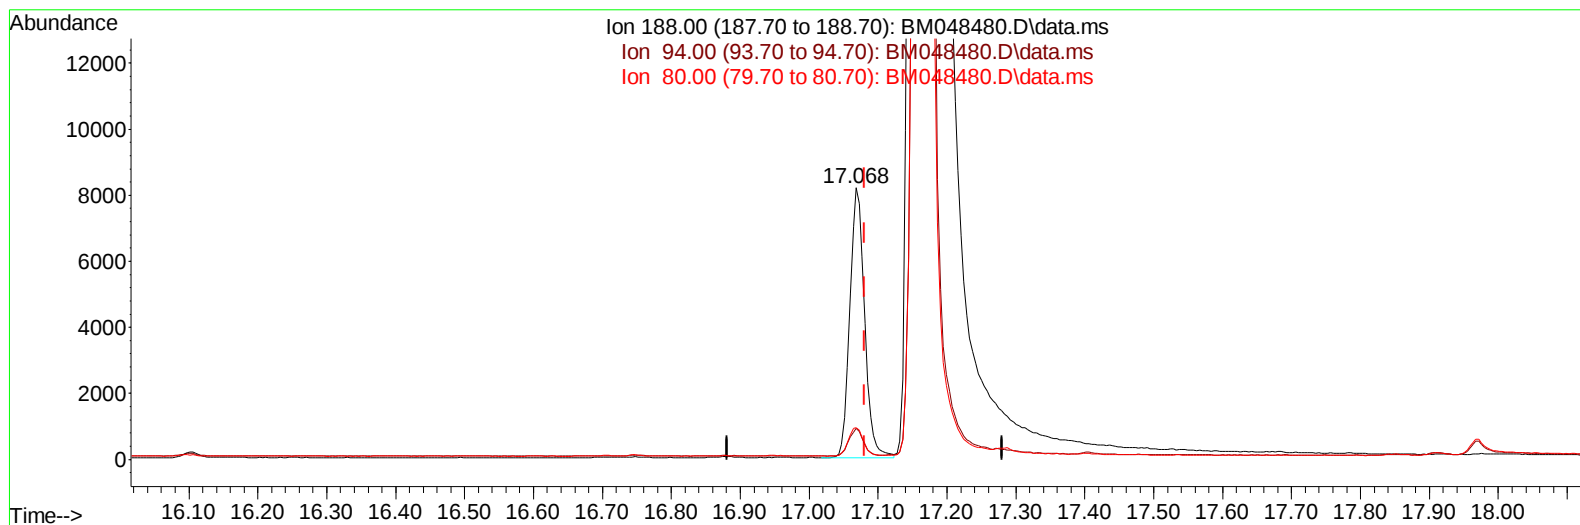

TIC: BM048480.D\data.ms

(13) Phenanthrene-d10 (I)

17.068min (-0.013) 0.40 ng/ul m

response 12143

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	11.35
80.00	12.60	11.74
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110624\
Data File : BM048480.D
Acq On : 06 Nov 2024 16:55
Operator : RC/JU
Sample : P4634-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0PI6

Manual IntegrationsAPPROVED

Quant Time: Nov 06 17:36:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 14:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :mohammad ahmed 11/11/2024

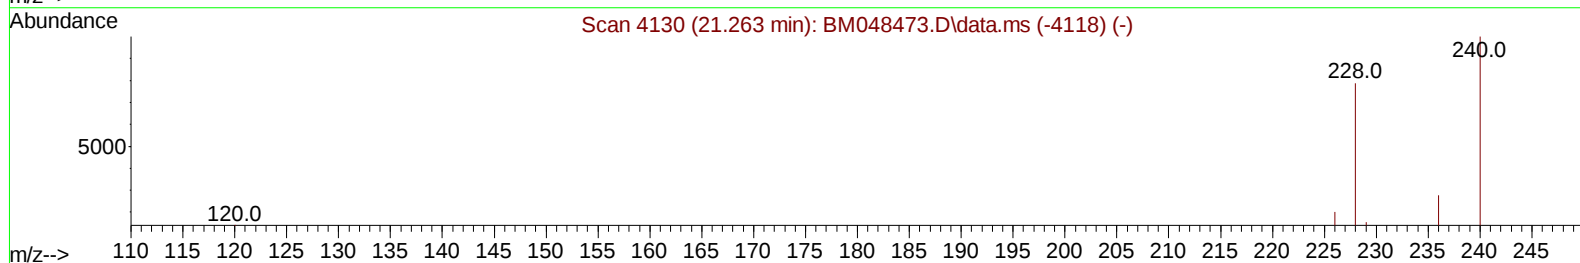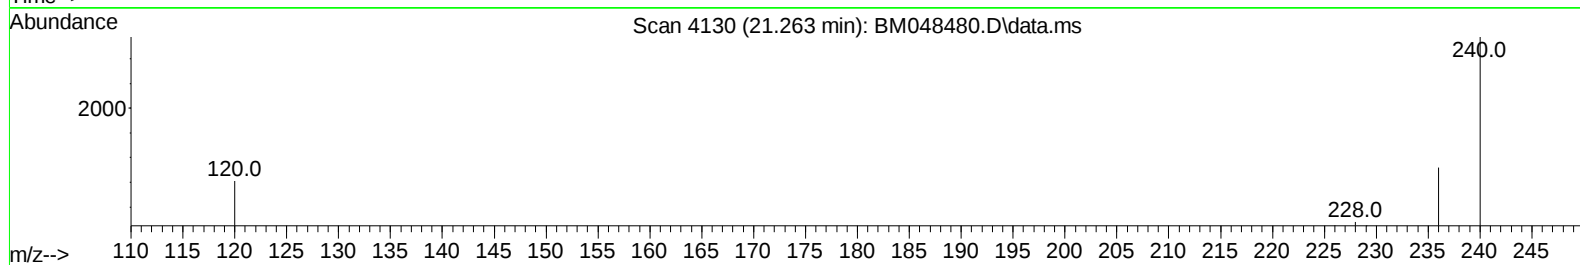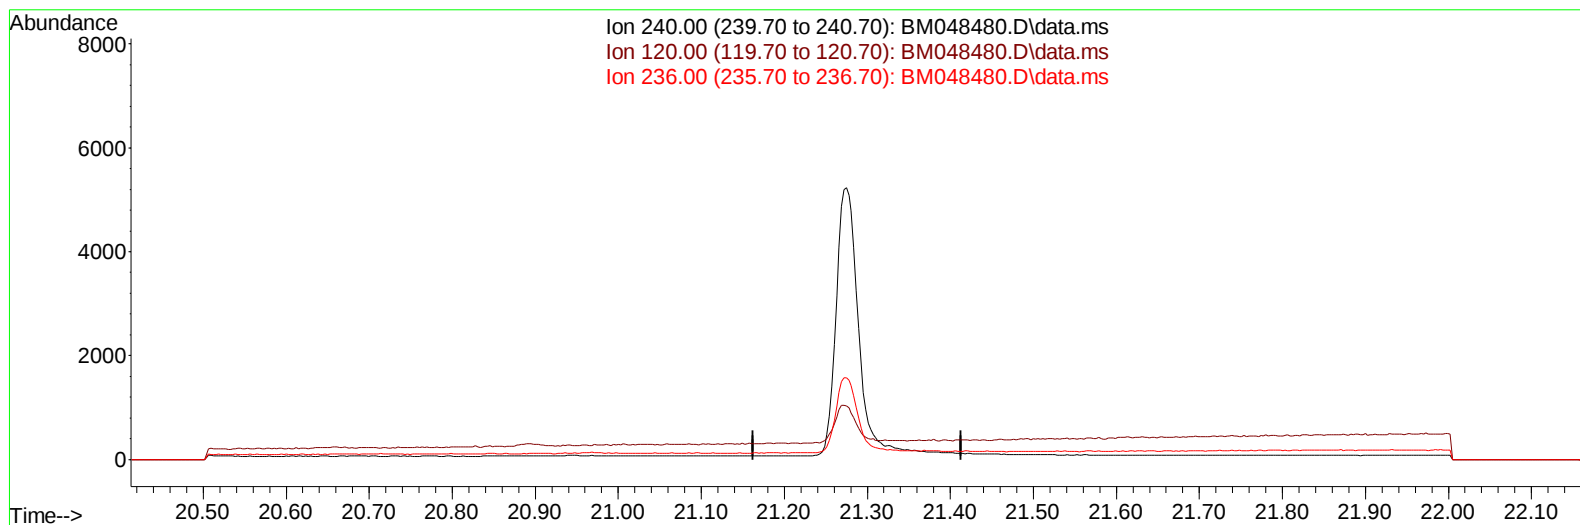

TIC: BM048480.D\data.ms

(17) Chrysene-d12

21.263min (-21.263) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.50	0.00#
236.00	29.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110624\
Data File : BM048480.D
Acq On : 06 Nov 2024 16:55
Operator : RC/JU
Sample : P4634-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0PI6

Manual IntegrationsAPPROVED

Quant Time: Nov 06 17:36:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 14:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :mohammad ahmed 11/11/2024

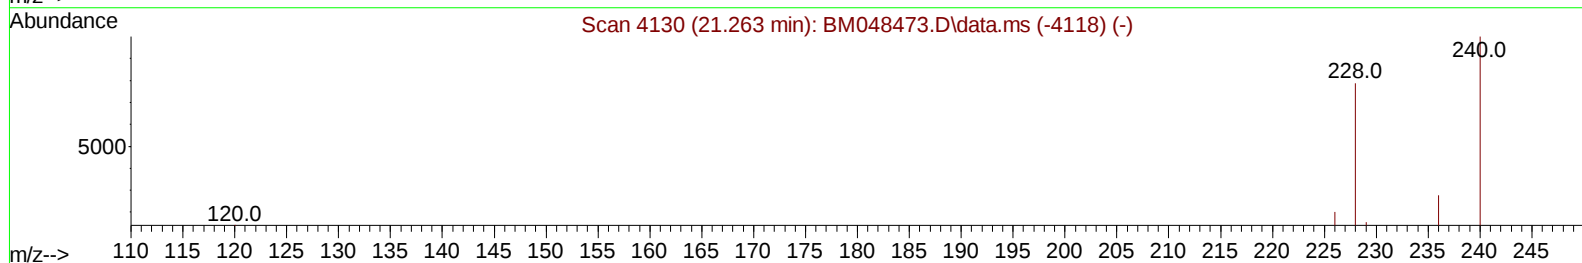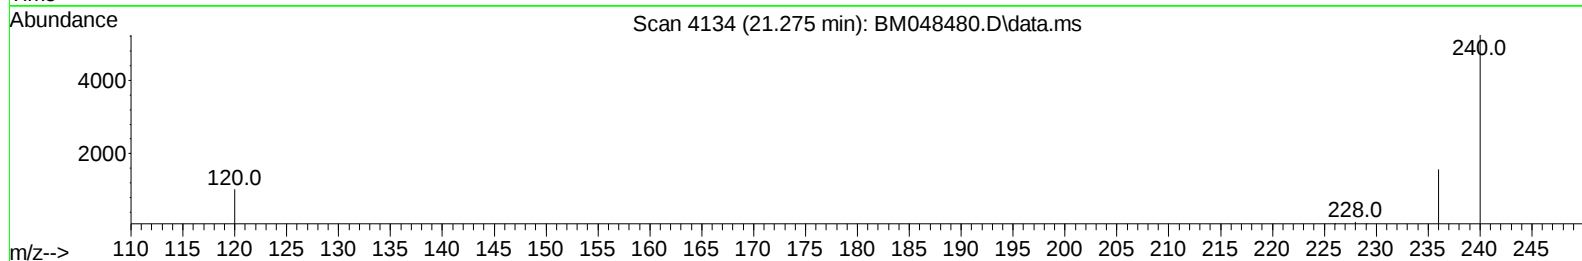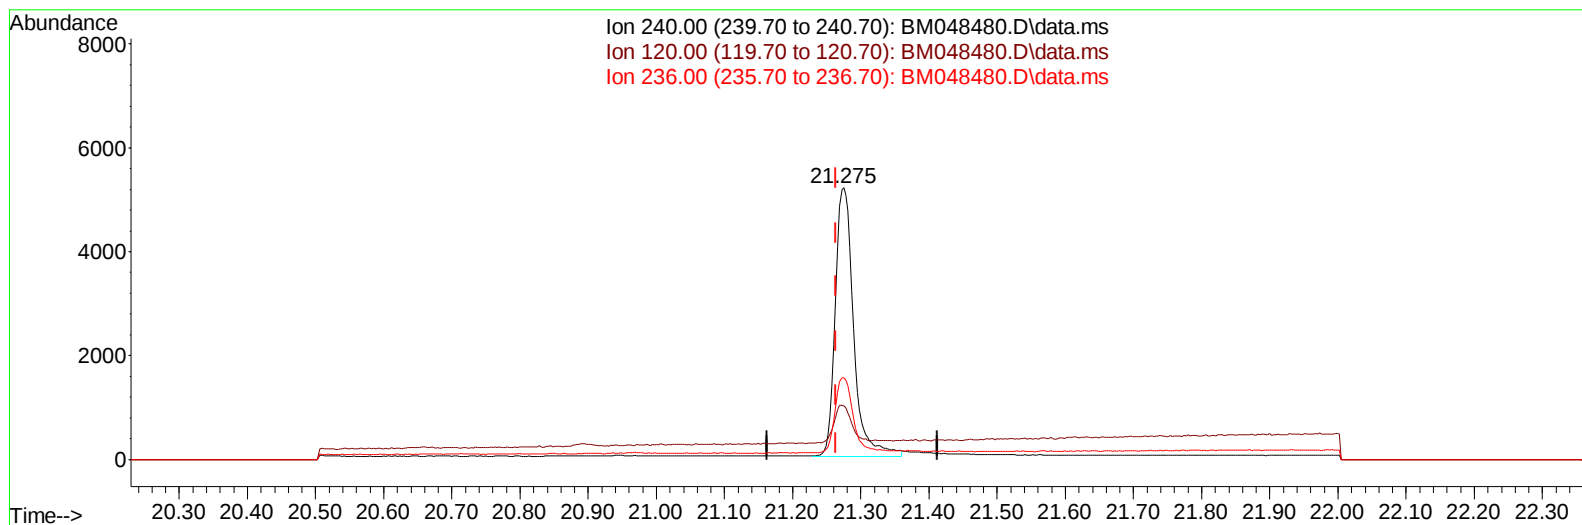

TIC: BM048480.D\data.ms

(17) Chrysene-d12

21.275min (+ 0.012) 0.40 ng/ul m

response 9762

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	19.70
236.00	29.90	30.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110624\
Data File : BM048480.D
Acq On : 06 Nov 2024 16:55
Operator : RC/JU
Sample : P4634-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0PI6

Manual IntegrationsAPPROVED

Quant Time: Nov 06 17:36:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 14:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :mohammad ahmed 11/11/2024

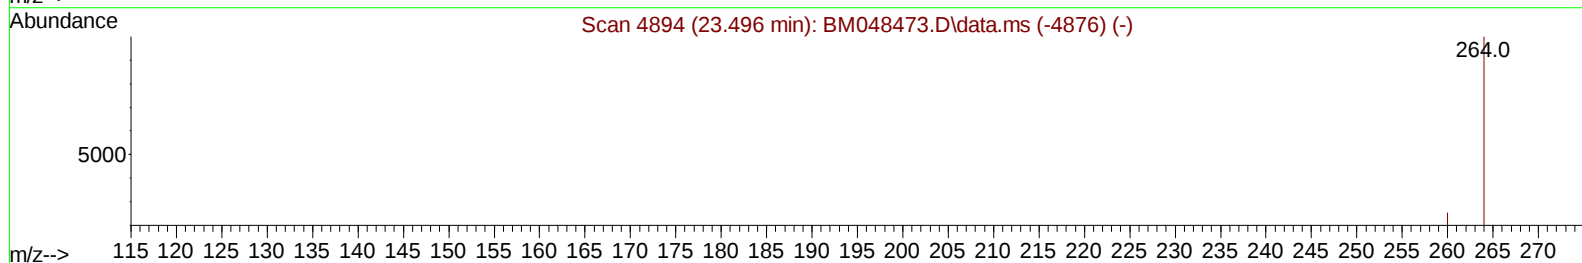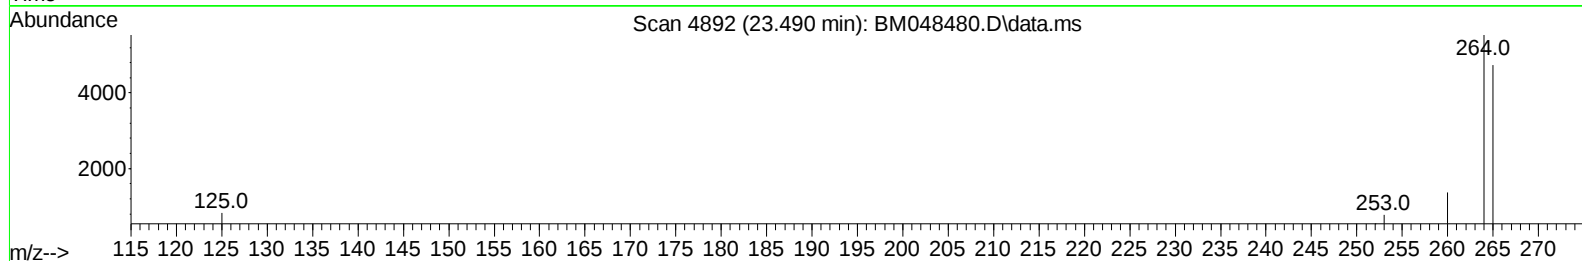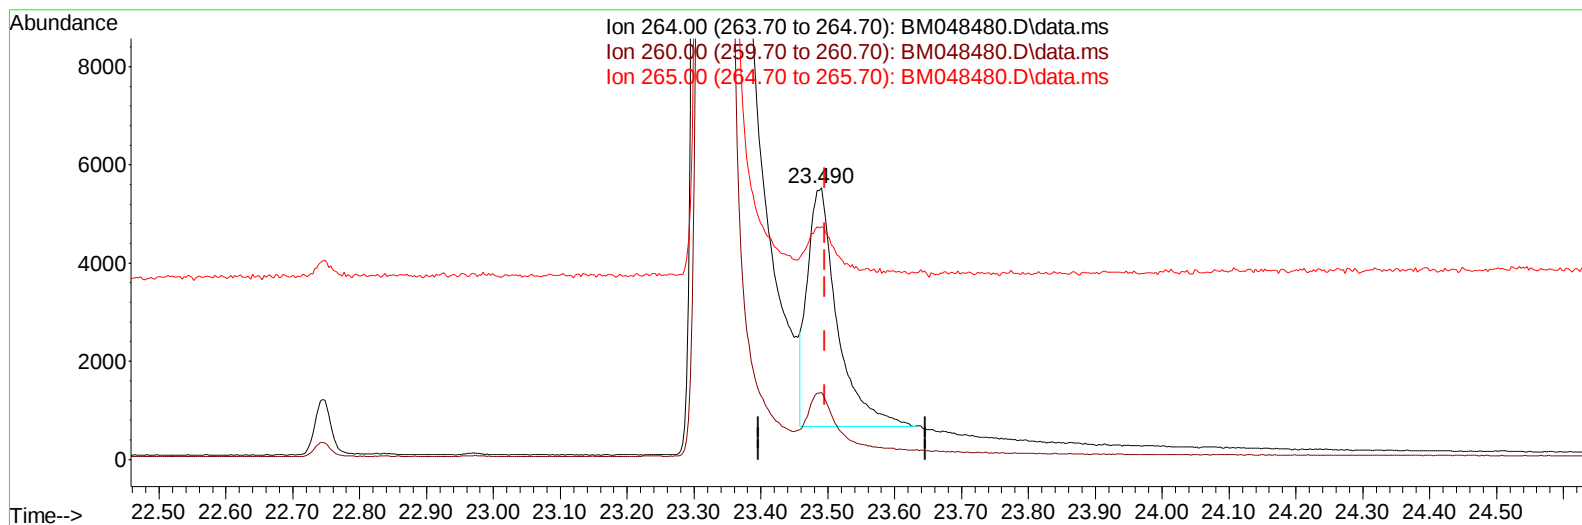

TIC: BM048480.D\data.ms

(23) Perylene-d12 (I)

23.490min (-0.006) 0.40 ng/u1

response 15097

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.77
265.00	119.80	85.64#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110624\
Data File : BM048480.D
Acq On : 06 Nov 2024 16:55
Operator : RC/JU
Sample : P4634-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0PI6

Manual IntegrationsAPPROVED

Quant Time: Nov 06 17:36:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 14:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :mohammad ahmed 11/11/2024

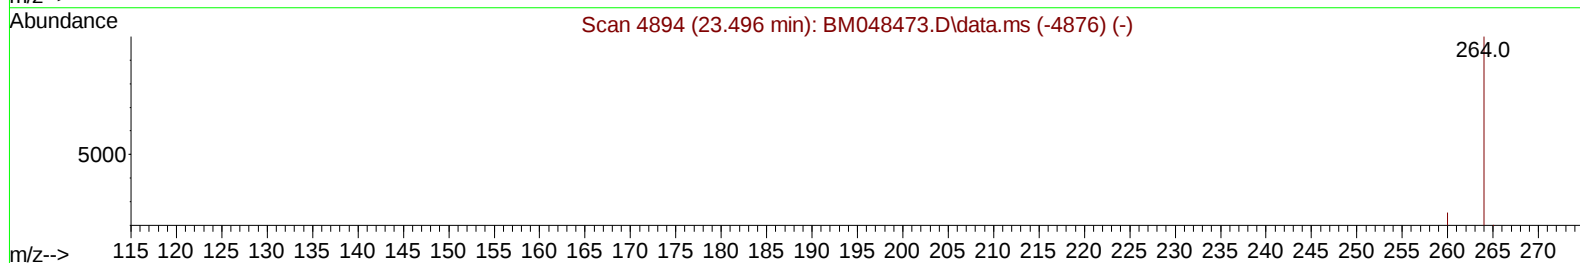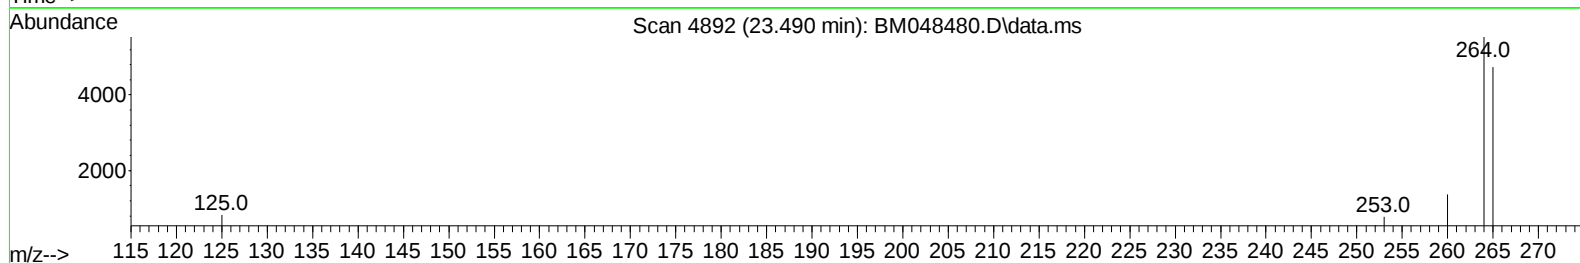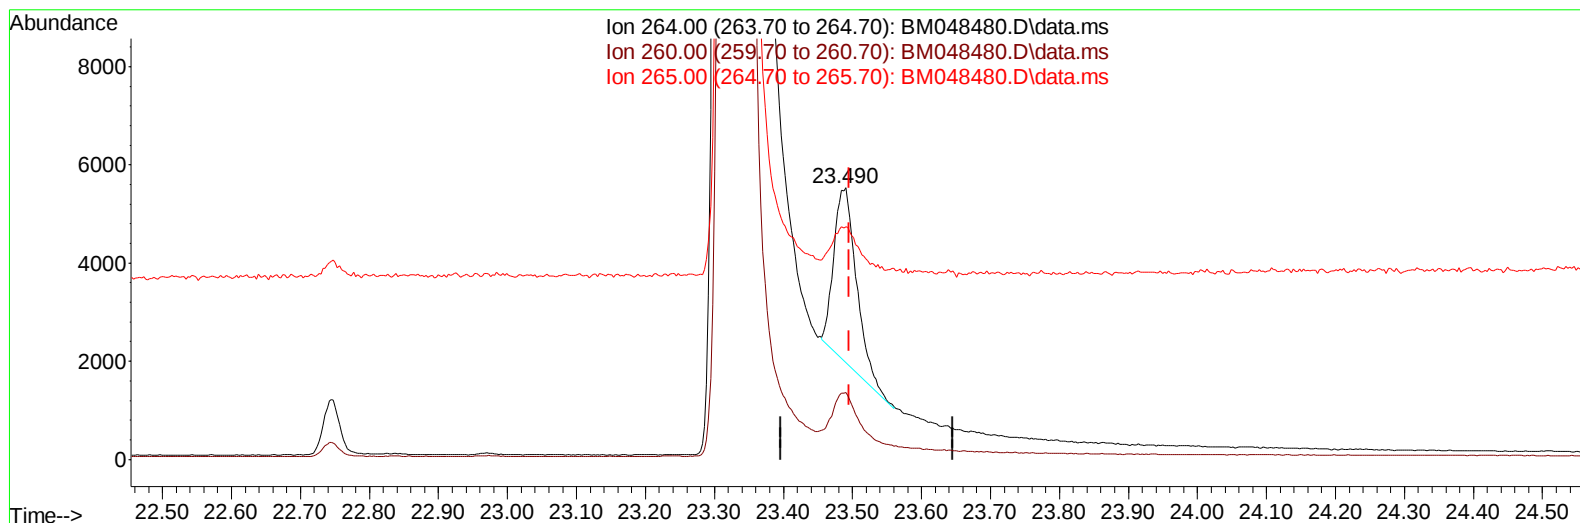

TIC: BM048480.D\data.ms

(23) Perylene-d12 (I)

23.490min (-0.006) 0.40 ng/ul m

response 7947

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.77
265.00	119.80	85.64#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110624\
 Data File : BM048480.D
 Acq On : 06 Nov 2024 16:55
 Operator : RC/JU
 Sample : P4634-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0PI6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/07/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 06 17:36:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 06 14:39:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.678	152	3631	0.400	ng/ul	0.00
4) Naphthalene-d8	10.462	136	11533	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.325	164	6233	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.068	188	12143m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.275	240	9762m	0.400	ng/ul	0.01
23) Perylene-d12	23.490	264	7947m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	22802	5.205	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.085	152	4977	0.334	ng/ul	0.01
18) Fluoranthene-d10	19.103	212	10362	0.378	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110624\
Data File : BM048480.D
Acq On : 06 Nov 2024 16:55
Operator : RC/JU
Sample : P4634-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0P16

Manual IntegrationsAPPROVED

Quant Time: Nov 06 17:36:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 14:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :mohammad ahmed 11/11/2024

