

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110716\
 Data File : BM007784.D
 Acq On : 07 Nov 2016 22:41
 Operator : UM/SJ
 Sample : H5554-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5N80

Manual Integrations
 APPROVED

umangi
 11/8/2016 3:15:28 PM

Quant Time: Nov 08 03:26:45 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM102016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 08 02:10:44 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	173802	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	658386	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.38	164	416534	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.13	188	816976	20.00	ng/ul	0.00
75) Chrysene-d12	21.31	240	1024143	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	1076793	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	5361	1.32	ng/uL	0.00
5) Phenol-d5	6.92	99	94155	7.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	278586	35.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	298502	29.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	180779	17.22	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	179839	37.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	196626	39.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	330112	33.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	6361m	0.56	ng/ul	0.02
43) Dimethylphthalate-d6	13.79	166	1074664	37.89	ng/ul	0.00
46) Acenaphthylene-d8	14.07	160	1307119	38.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	21236m	4.74	ng/ul	0.02
57) Fluorene-d10	15.37	176	944754	38.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.51	200	142874	29.44	ng/ul	0.00
70) Anthracene-d10	17.22	188	1439756	39.11	ng/ul	0.00
76) Pyrene-d10	19.52	212	1661974	39.50	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	1820857	38.73	ng/ul	0.00

Target Compounds						Ovalue
56) Diethylphthalate	15.20	149	329344	12.08	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM110716\
Data File : BM007784.D
Acq On : 07 Nov 2016 22:41
Operator : UM/SJ
Sample : H5554-08
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
E5N80

Manual Integrations
APPROVED

umangi
11/8/2016 3:15:28 PM

Quant Time: Nov 08 03:26:45 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 08 02:10:44 2016
Response via : Initial Calibration

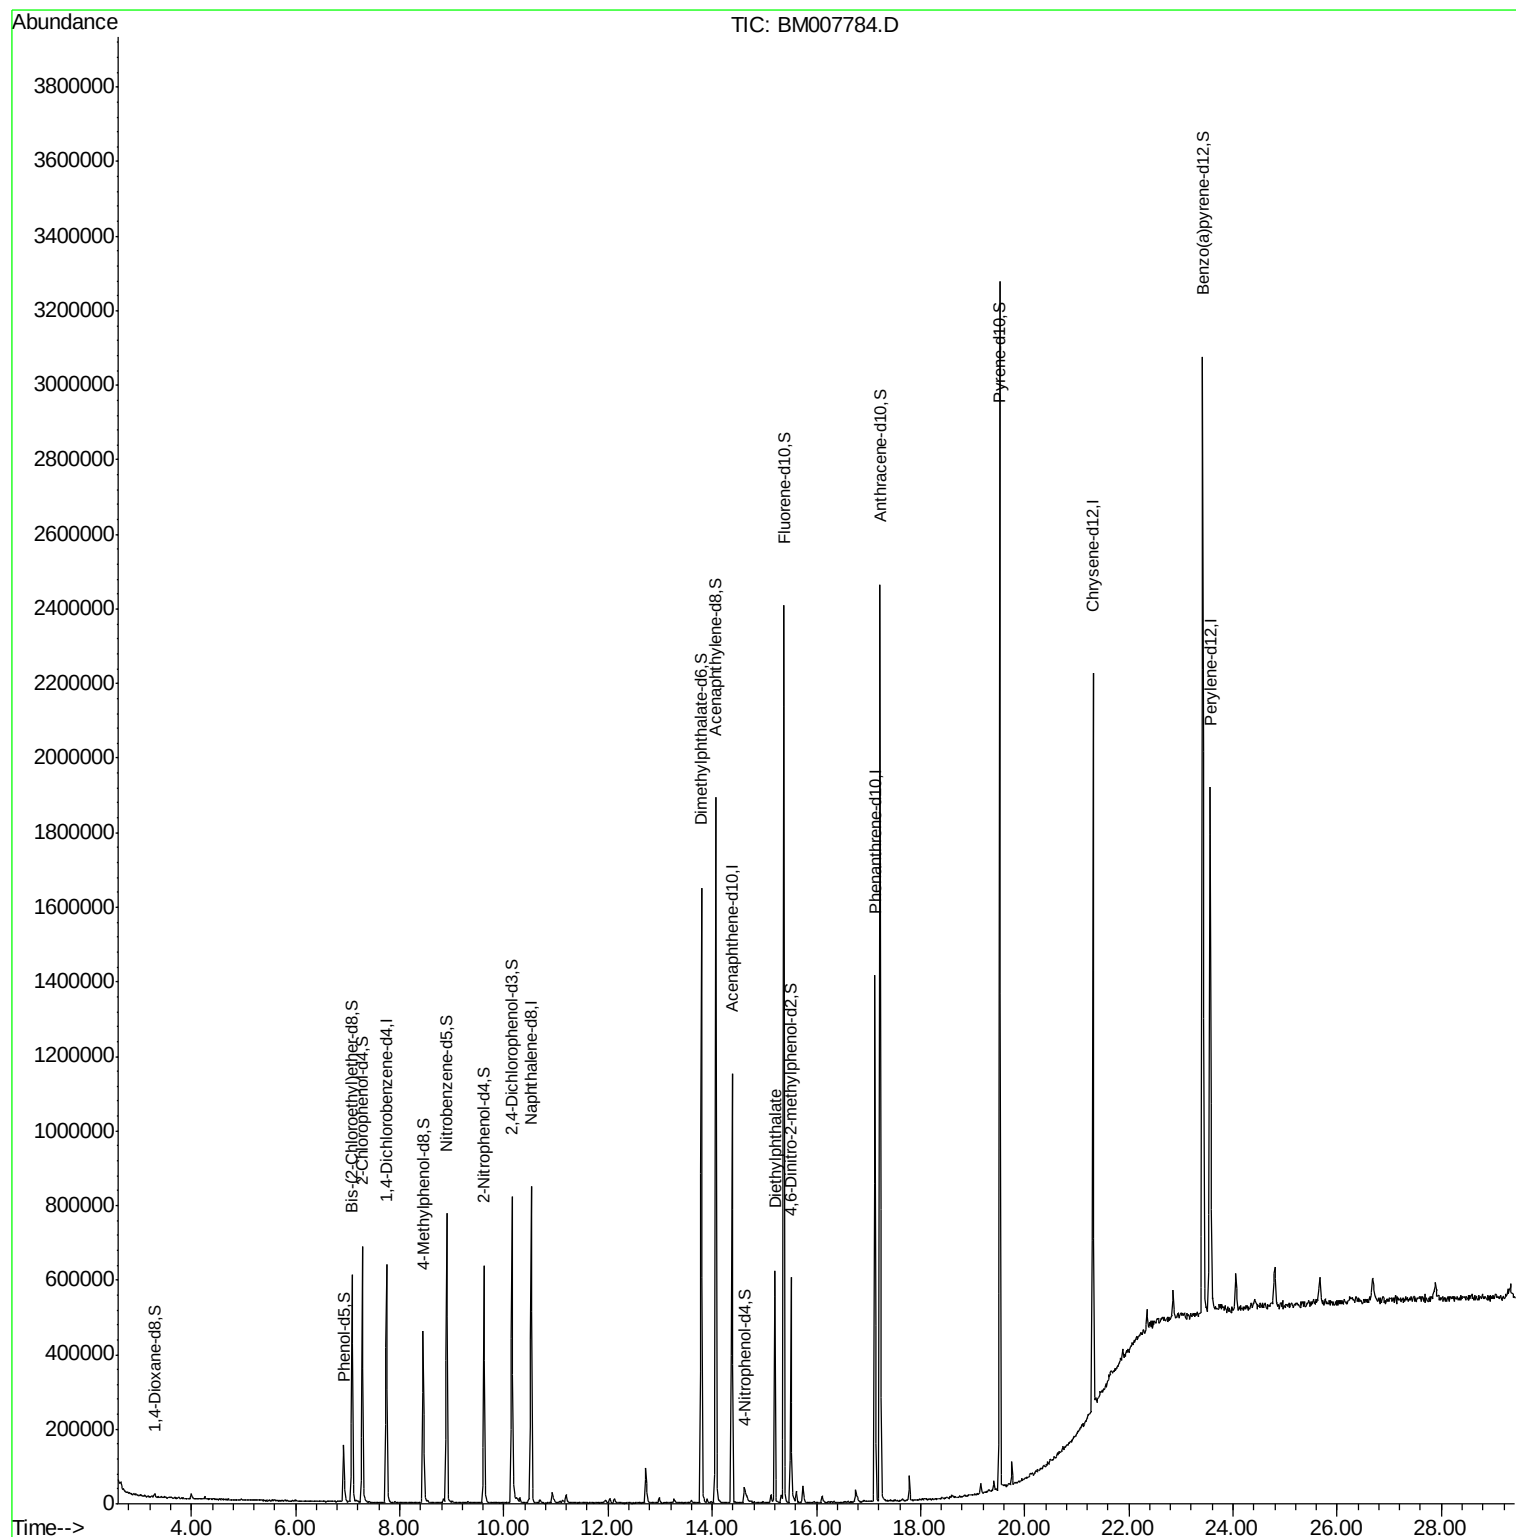

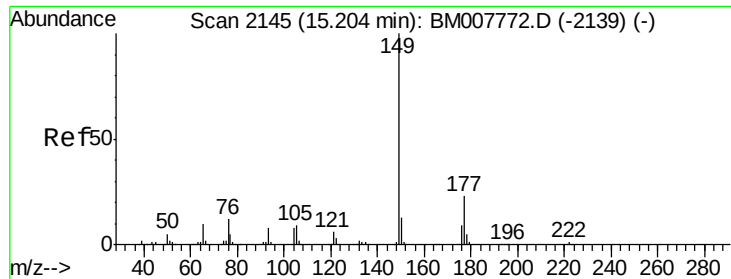

#56
 Diethylphthalate
 Concen: 12.08 ng/ul
 RT: 15.20 min Scan# 2145
 Delta R.T. -0.00 min
 Lab File: BM007784.D
 Acq: 07 Nov 2016 22:41

Instrument :
 BNA_M
 ClientSampleId :
 E5N80

Tot Ion	Ratio	Resp	Lower	Upper
149	100	329344		
177	22.9		18.6	28.0
150	12.7		10.0	15.0

Manual Integrations
 APPROVED

umangi
 11/8/2016 3:15:28 PM

