

Data Path : Z:\HPCHEM1\BNA M\Data\BM110717\
 Data File : BM012811.D
 Acq On : 08 Nov 2017 00:27
 Operator : SJ/JU
 Sample : I6164-04DL 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET0D0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM110417MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.804	118	122	128	rVB	25397	34362	1.13%	0.139%
2	6.975	655	661	673	rBB2	69360	126837	4.18%	0.512%
3	7.134	682	688	700	rBB	58287	91554	3.02%	0.370%
4	7.334	716	722	731	rVB	78398	124428	4.11%	0.502%
5	7.798	794	801	811	rBB	605792	949250	31.32%	3.833%
6	8.510	917	922	933	rBV	76622	128128	4.23%	0.517%
7	8.957	992	998	1007	rBB	71808	116736	3.85%	0.471%
8	9.681	1115	1121	1129	rBB	58024	96304	3.18%	0.389%
9	10.222	1207	1213	1223	rBV	85688	157400	5.19%	0.636%
10	10.586	1268	1275	1288	rBV	812779	1372402	45.28%	5.542%
11	10.733	1295	1300	1306	rBV	28597	55545	1.83%	0.224%
12	13.845	1824	1829	1833	rBV	196720	262505	8.66%	1.060%
13	13.892	1833	1837	1845	rVB	111206	145575	4.80%	0.588%
14	14.127	1871	1877	1886	rBV	213845	312890	10.32%	1.263%
15	14.439	1923	1930	1937	rBV2	1190297	1837423	60.63%	7.419%
16	14.498	1937	1940	1946	rVB	25813	36161	1.19%	0.146%
17	14.663	1964	1968	1981	rBV3	27309	52276	1.72%	0.211%
18	15.233	2061	2065	2072	rBV	52067	63986	2.11%	0.258%
19	15.427	2093	2098	2104	rBV	280227	406539	13.41%	1.642%
20	15.486	2104	2108	2114	rVB2	37386	52725	1.74%	0.213%
21	15.568	2118	2122	2126	rBV	23375	31326	1.03%	0.126%
22	15.792	2154	2160	2166	rBV2	23616	39531	1.30%	0.160%
23	17.180	2385	2396	2400	rBV2	1407314	2016604	66.54%	8.143%
24	17.221	2400	2403	2409	rVV	576434	811330	26.77%	3.276%
25	17.280	2409	2413	2416	rVV	305313	410492	13.54%	1.658%
26	17.315	2416	2419	2425	rVB	133887	181622	5.99%	0.733%
27	17.586	2457	2465	2470	rBV	29826	46660	1.54%	0.188%
28	18.062	2540	2546	2550	rBV2	45996	94519	3.12%	0.382%
29	18.104	2550	2553	2560	rVB	64400	87830	2.90%	0.355%
30	18.256	2572	2579	2583	rBV3	100703	174061	5.74%	0.703%
31	18.556	2625	2630	2634	rBV	49746	64308	2.12%	0.260%
32	18.604	2634	2638	2645	rVB	43135	59946	1.98%	0.242%
33	19.121	2721	2726	2732	rBV2	22808	38381	1.27%	0.155%
34	19.239	2740	2746	2754	rBV	1436849	1855674	61.23%	7.493%

Data Path : Z:\HPCHEM1\BNA M\Data\BM110717\
Data File : BM012811.D
Acq On : 08 Nov 2017 00:27
Operator : SJ/JU
Sample : I6164-04DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETOD0DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM110417MA.M
Title : SVOA CALIBRATION

35	19.486	2784	2788	2791	rVB	27516	36393	1.20%	0.147%
36	19.574	2797	2803	2805	rBV3	536032	771830	25.47%	3.117%
37	19.603	2805	2808	2815	rVV	1033132	1361533	44.92%	5.498%
38	19.674	2816	2820	2826	rVV2	40099	61572	2.03%	0.249%
39	19.780	2835	2838	2844	rBV	52395	69021	2.28%	0.279%
40	19.845	2846	2849	2853	rVV2	31137	49497	1.63%	0.200%
41	19.927	2857	2863	2869	rVV4	51565	132832	4.38%	0.536%
42	20.062	2881	2886	2888	rBV4	38621	63013	2.08%	0.254%
43	20.098	2888	2892	2897	rVB	164726	223020	7.36%	0.901%
44	20.198	2905	2909	2913	rBV	138202	173147	5.71%	0.699%
45	20.256	2913	2919	2922	rBV2	63578	114094	3.76%	0.461%
46	20.292	2922	2925	2929	rVB2	40355	51803	1.71%	0.209%
47	20.339	2930	2933	2938	rBV7	20756	41218	1.36%	0.166%
48	20.403	2940	2944	2947	rBV3	34483	62126	2.05%	0.251%
49	20.850	3017	3020	3025	rVB2	49717	65351	2.16%	0.264%
50	21.009	3043	3047	3050	rBV	110745	159222	5.25%	0.643%
51	21.045	3051	3053	3056	rVV	72513	86776	2.86%	0.350%
52	21.086	3057	3060	3065	rVB2	80229	142629	4.71%	0.576%
53	21.362	3100	3107	3111	rBV2	1823835	3030785	100.00%	12.238%
54	21.397	3111	3113	3118	rVB	611694	694213	22.91%	2.803%
55	21.515	3130	3133	3139	rBV	142524	196156	6.47%	0.792%
56	22.956	3373	3378	3383	rBV	574569	1259880	41.57%	5.087%
57	23.444	3457	3461	3466	rBV	299215	493001	16.27%	1.991%
58	23.497	3466	3470	3473	rVV2	178094	274340	9.05%	1.108%
59	23.544	3474	3478	3485	rVB	481684	859596	28.36%	3.471%
60	23.644	3489	3495	3501	rBV	1035357	1956510	64.55%	7.900%


Sum of corrected areas: 24764868

Data Path : Z:\HPCHEM1\BNA M\Data\BM110717\
Data File : BM012811.D
Acq On : 08 Nov 2017 00:27
Operator : SJ/JU
Sample : I6164-04DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETOD0DL

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

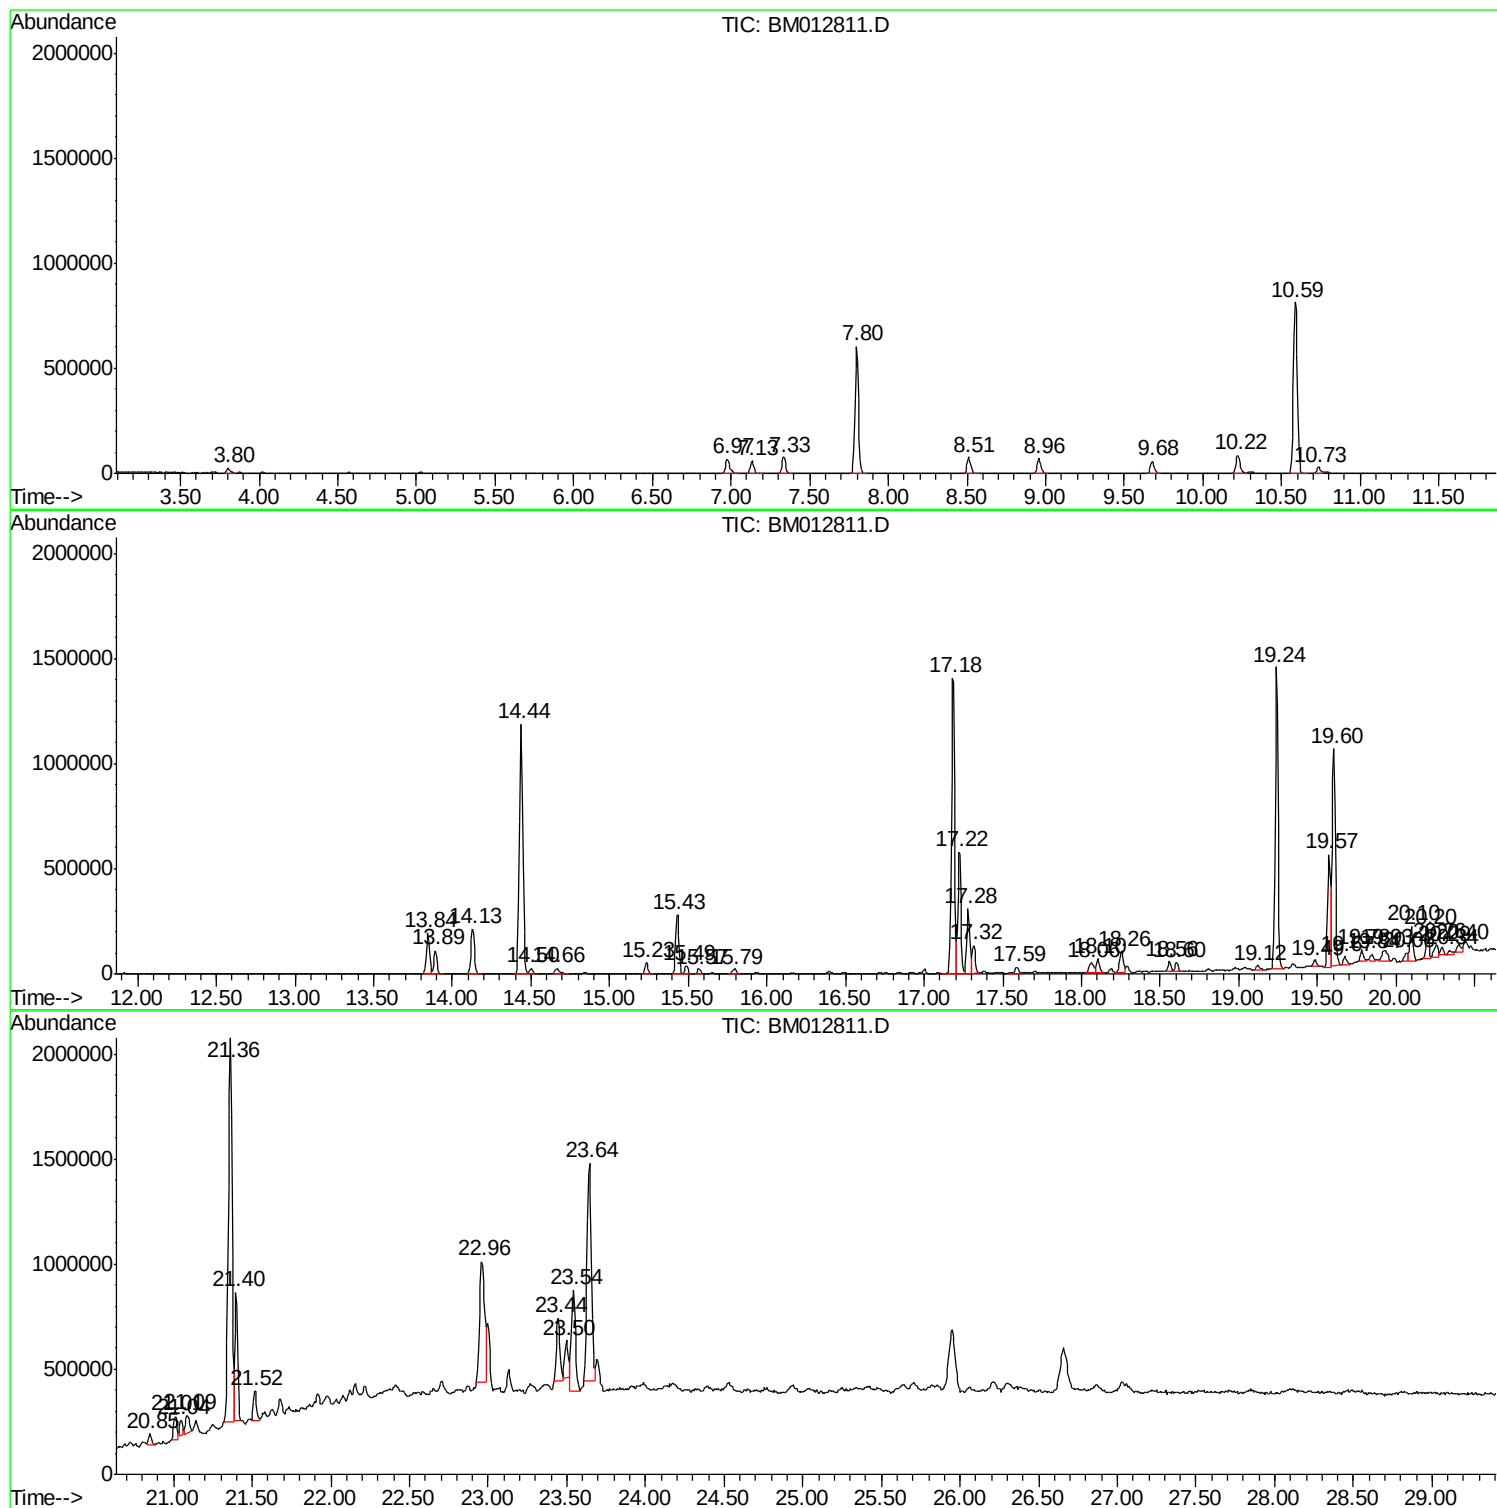

Data Path : Z:\HPCHEM1\BNA_M\Data\BM110717\
Data File : BM012811.D
Acq On : 08 Nov 2017 00:27
Operator : SJ/JU
Sample : I6164-04DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET0D0DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM110417MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM110717\
Data File : BM012811.D
Acq On : 08 Nov 2017 00:27
Operator : SJ/JU
Sample : I6164-04DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET0D0DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM110417MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc