

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
 Data File : BM037384.D
 Acq On : 07 Nov 2022 10:15
 Operator : CG/JU
 Sample : PB148709BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK709

Quant Time: Nov 07 23:06:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 00:30:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.842	152	6481	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	21814	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	13015	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	25752	0.400	ng/ul	0.00
17) Chrysene-d12	21.391	240	17647	0.400	ng/ul	0.00
23) Perylene-d12	23.720	264	17838	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	38829	4.719	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.239	152	7610	0.232	ng/ul	0.01
18) Fluoranthene-d10	19.239	212	15164	0.275	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.464	166	3308	0.059	ng/ul#	14
20) Pyrene	19.601	202	3176	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.568	252	6644	0.078	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
Data File : BM037384.D
Acq On : 07 Nov 2022 10:15
Operator : CG/JU
Sample : PB148709BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK709

Quant Time: Nov 07 23:06:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:30:18 2022
Response via : Initial Calibration




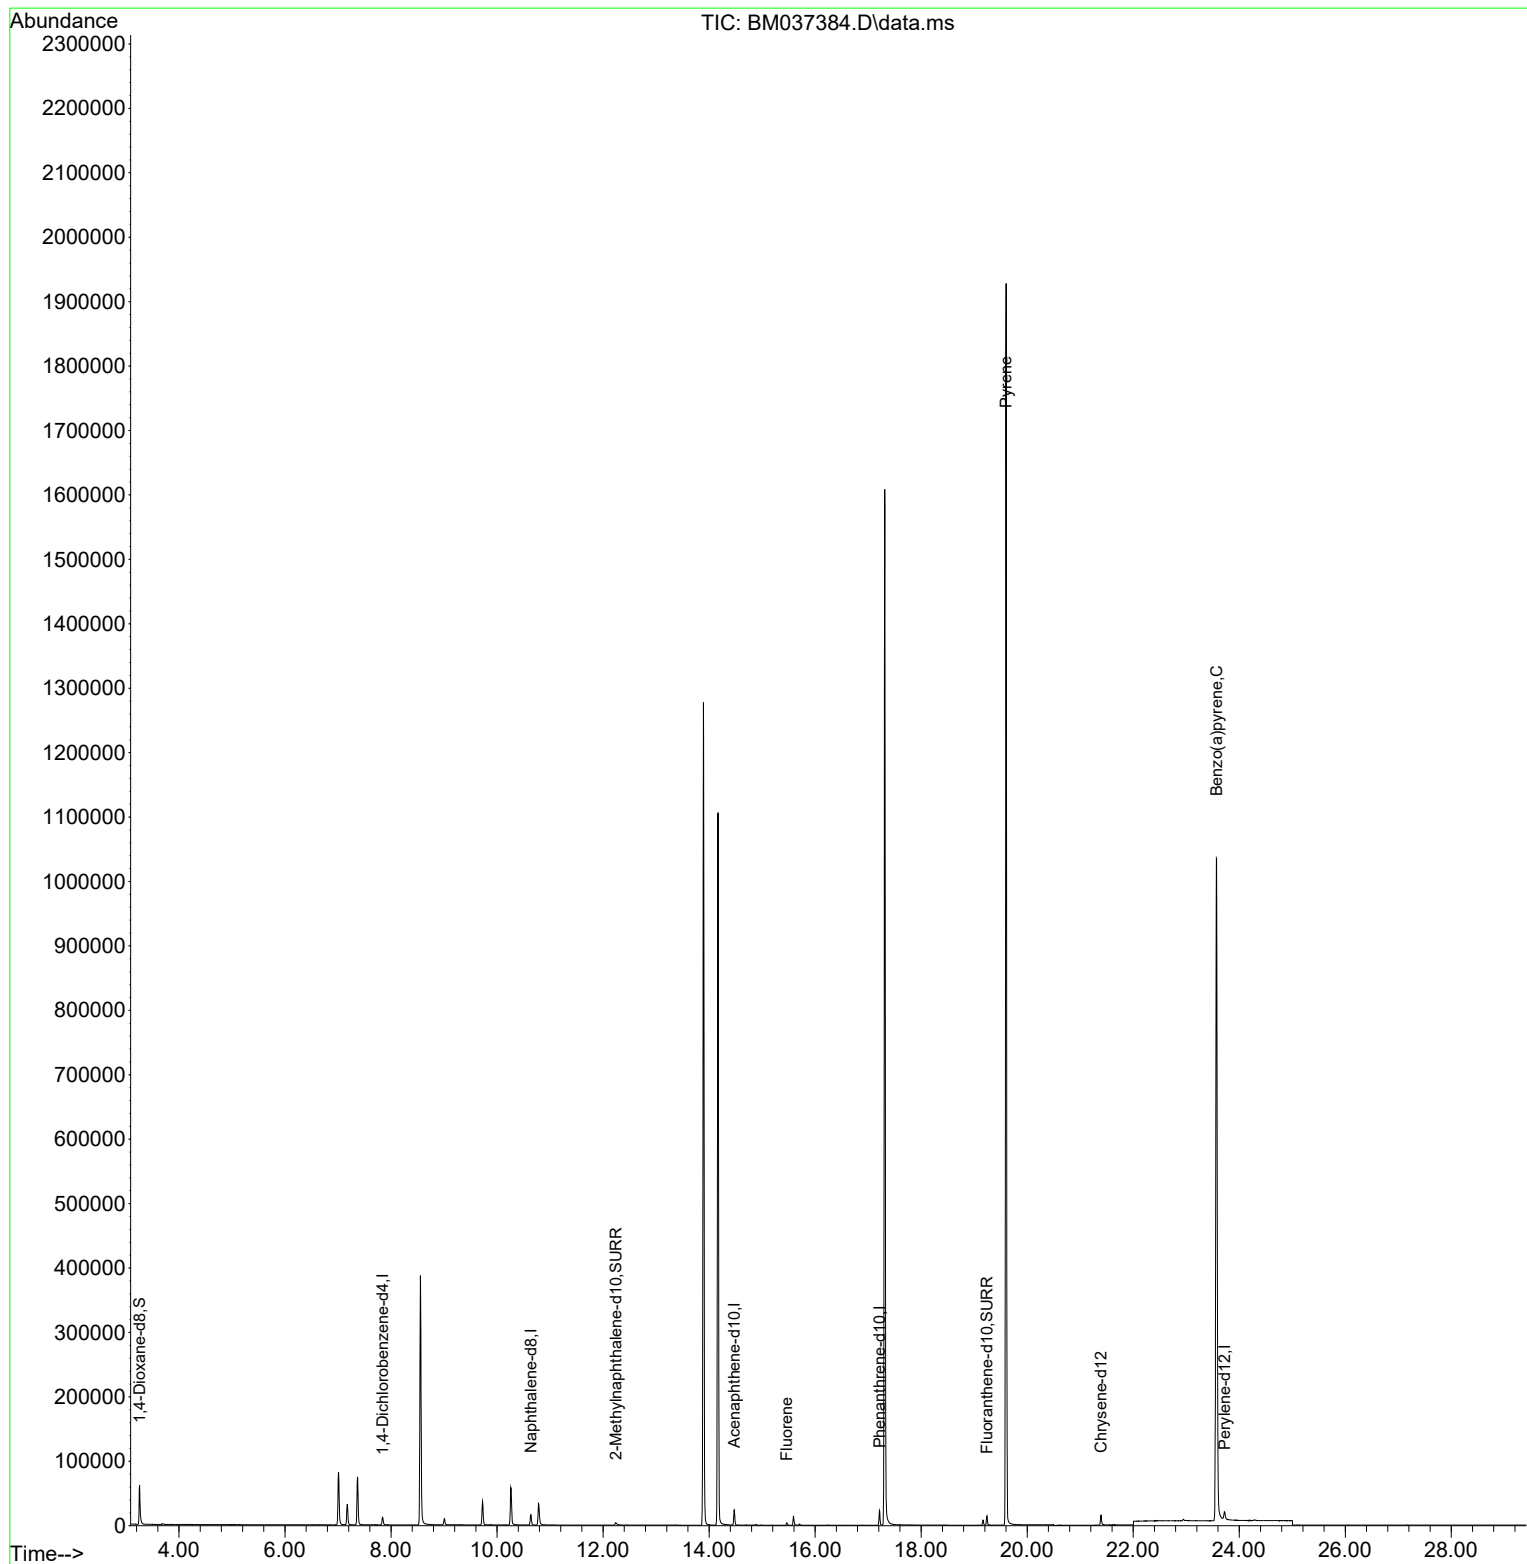


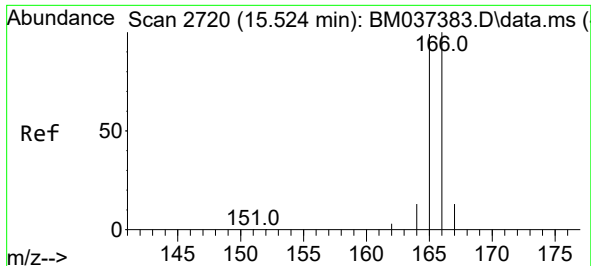

#12
Fluorene
Concen: 0.059 ng/ul
RT: 15.464 min Scan# 21
Delta R.T. -0.059 min
Lab File: BM037384.D
Acq: 07 Nov 2022 10:15




Instrument :
BNA_M
ClientSampleId :
SBLK709


Tgt Ion:166 Resp: 3308
Ion Ratio Lower Upper
166 100
165 7.3 79.0 118.4#
167 31.4 11.1 16.7#

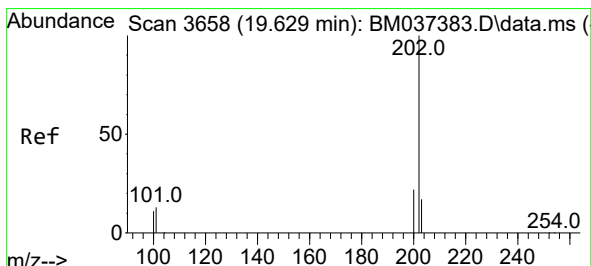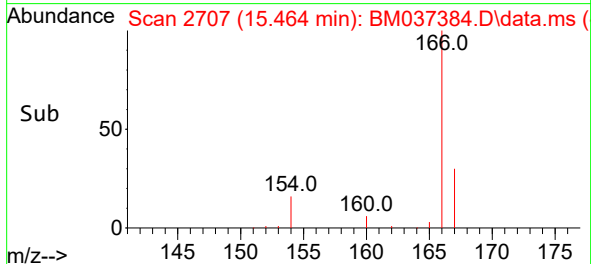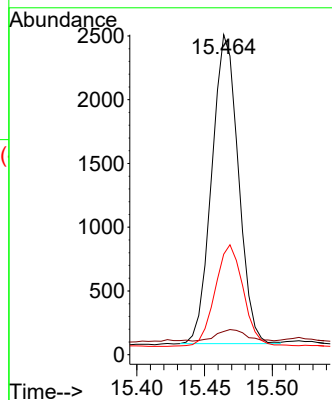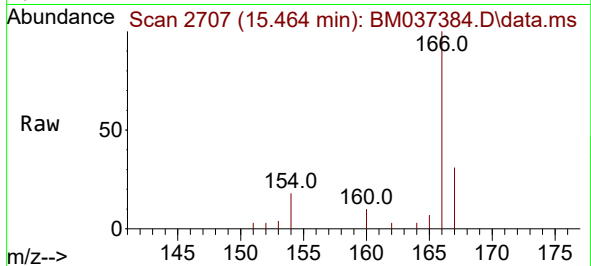

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.601 min Scan# 3652
Delta R.T. -0.027 min
Lab File: BM037384.D
Acq: 07 Nov 2022 10:15


Tgt Ion:202 Resp: 3176
Ion Ratio Lower Upper
202 100
101 147.5 11.1 16.7#
100 1094.5 9.0 13.4#

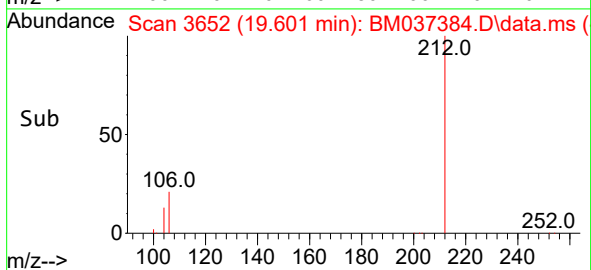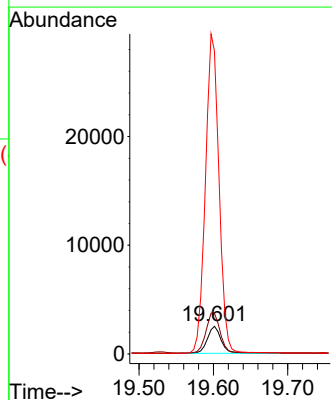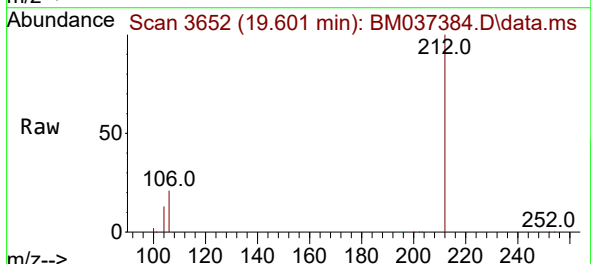

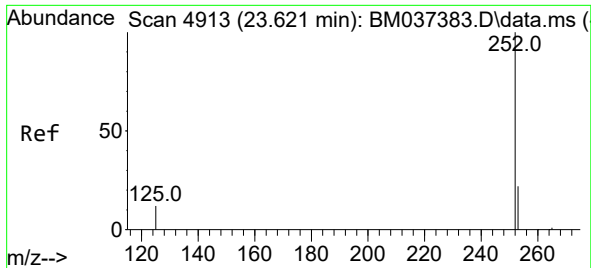

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.568 min Scan# 41
Delta R.T. -0.051 min
Lab File: BM037384.D
Acq: 07 Nov 2022 10:15

Instrument :
BNA_M
ClientSampleId :
SBLK709

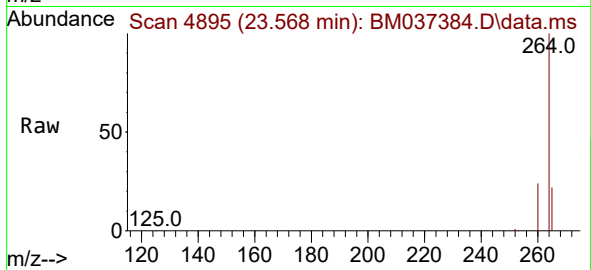

Tgt Ion:252 Resp: 6644
Ion Ratio Lower Upper
252 100
253 49.2 23.8 35.6#
125 46.2 17.2 25.8#

