

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
 Data File : BM037396.D
 Acq On : 07 Nov 2022 17:49
 Operator : CG/JU
 Sample : PB148649BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK649

Quant Time: Nov 07 23:08:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 00:30:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.837	152	5381	0.400	ng/ul	0.00
4) Naphthalene-d8	10.633	136	17564	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.473	164	10562	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.212	188	20344	0.400	ng/ul	0.00
17) Chrysene-d12	21.389	240	13754	0.400	ng/ul	0.00
23) Perylene-d12	23.724	264	14124	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	41117	6.018	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	8495	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.238	212	16187	0.376	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.463	166	3602	0.079	ng/ul#	13
20) Pyrene	19.601	202	3449	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.572	252	7142	0.105	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
Data File : BM037396.D
Acq On : 07 Nov 2022 17:49
Operator : CG/JU
Sample : PB148649BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK649

Quant Time: Nov 07 23:08:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:30:18 2022
Response via : Initial Calibration




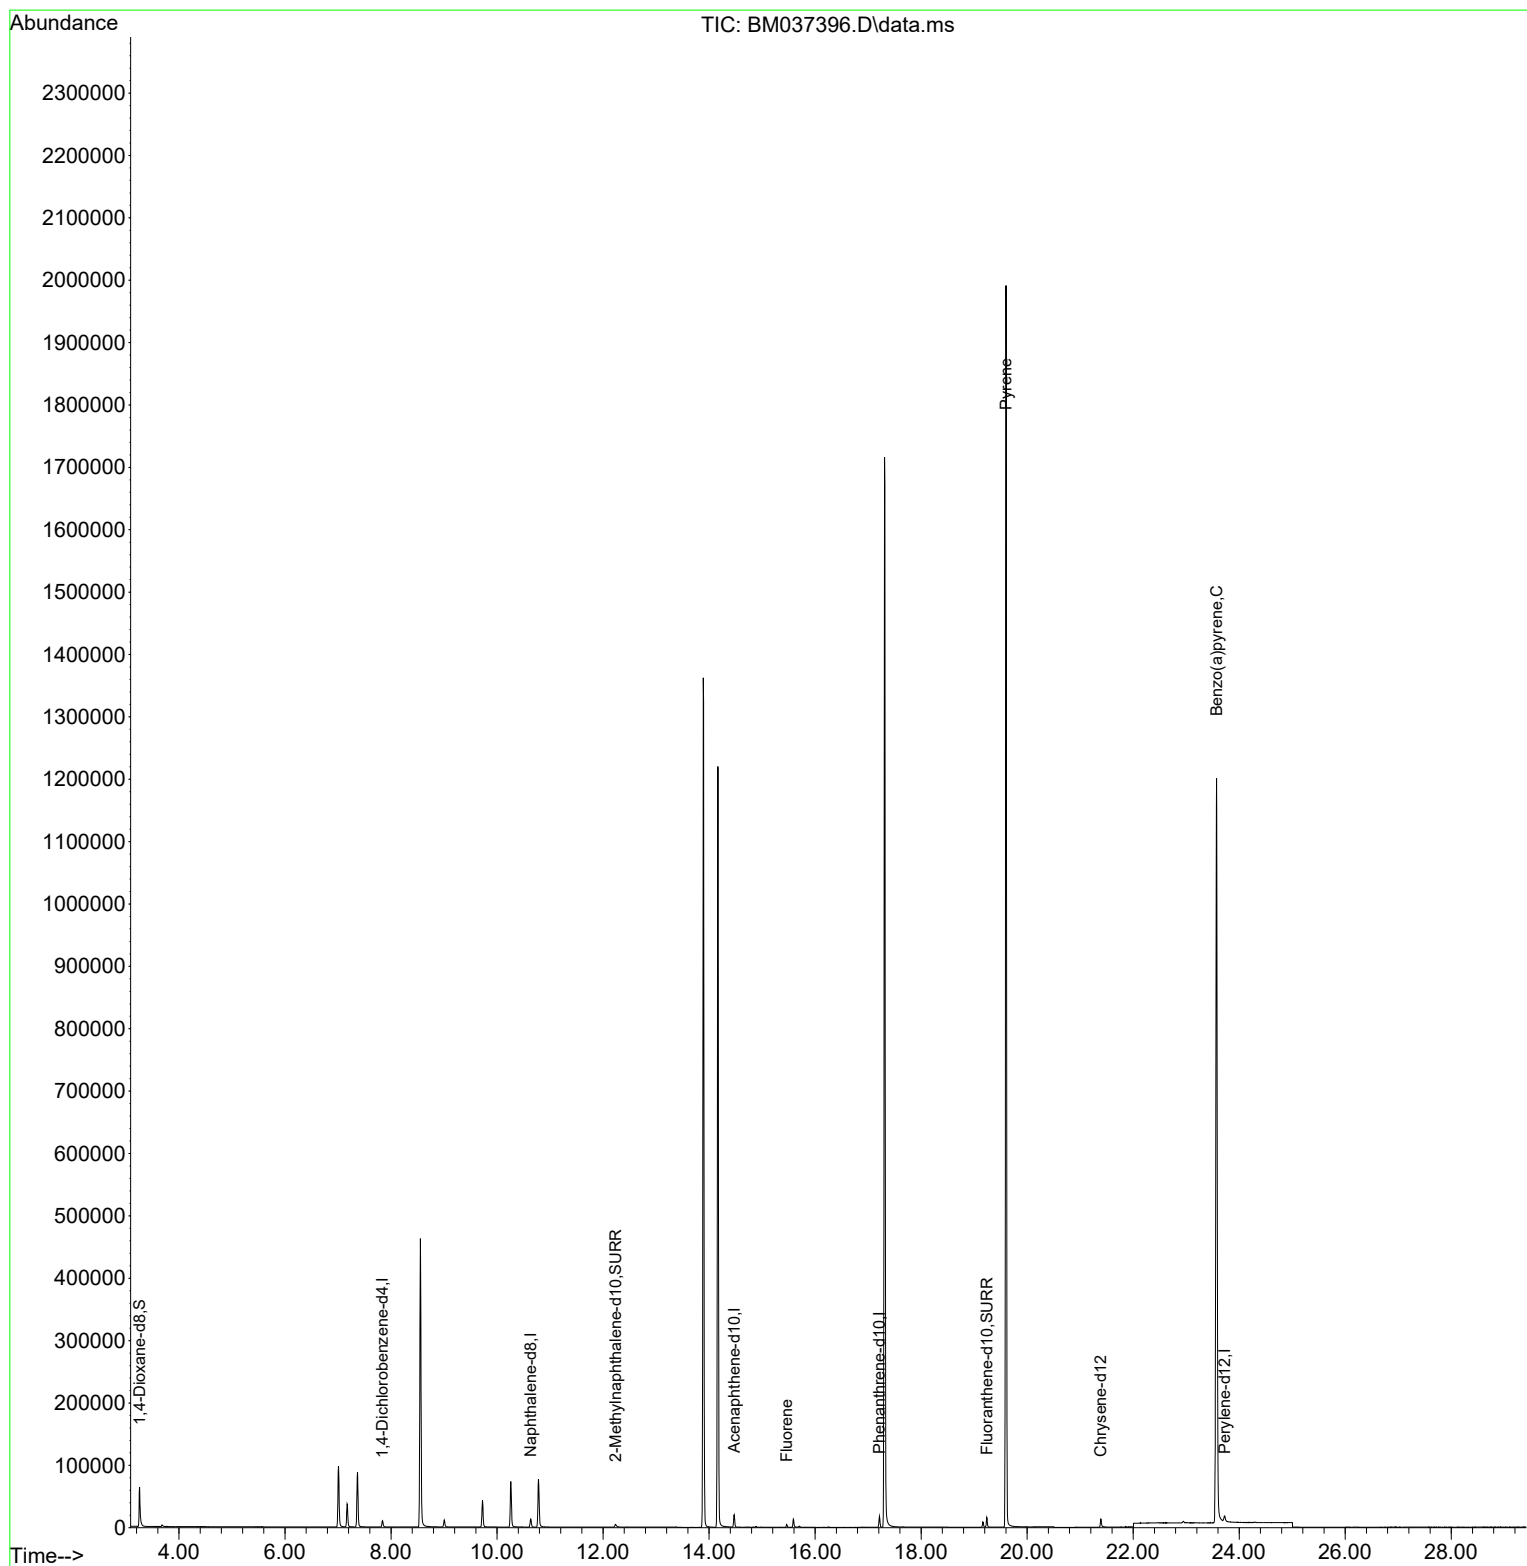


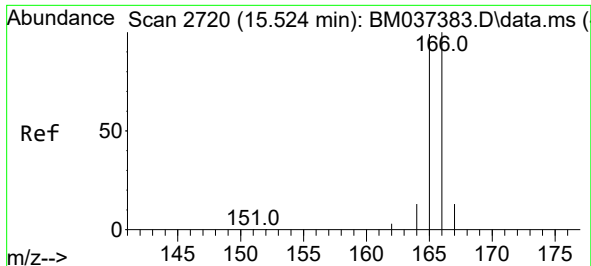

#12
Fluorene
Concen: 0.079 ng/ul
RT: 15.463 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM037396.D
Acq: 07 Nov 2022 17:49




Instrument :
BNA_M
ClientSampleId :
SBLK649


Tgt Ion:166 Resp: 3602
Ion Ratio Lower Upper
166 100
165 6.9 79.0 118.4#
167 33.5 11.1 16.7#

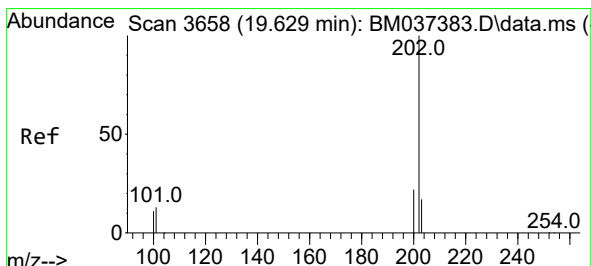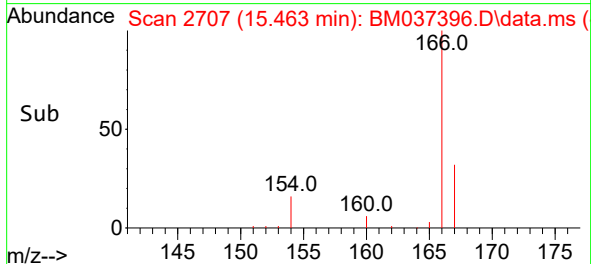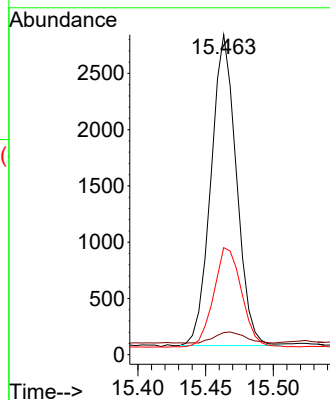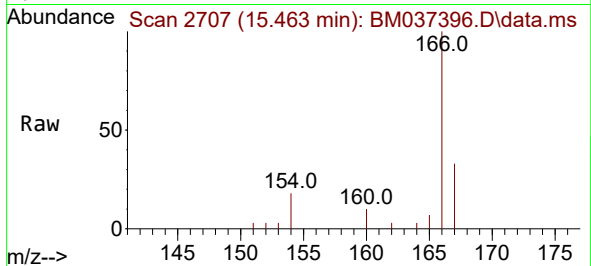

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.601 min Scan# 3652
Delta R.T. -0.028 min
Lab File: BM037396.D
Acq: 07 Nov 2022 17:49


Tgt Ion:202 Resp: 3449
Ion Ratio Lower Upper
202 100
101 158.1 11.1 16.7#
100 1194.5 9.0 13.4#

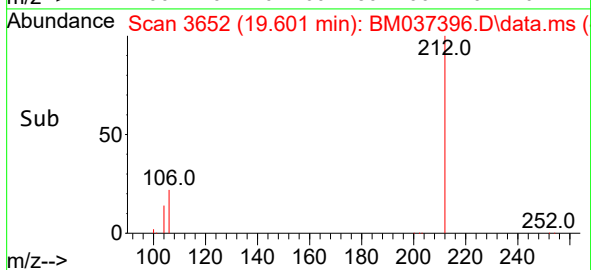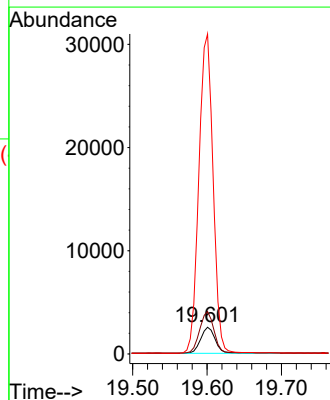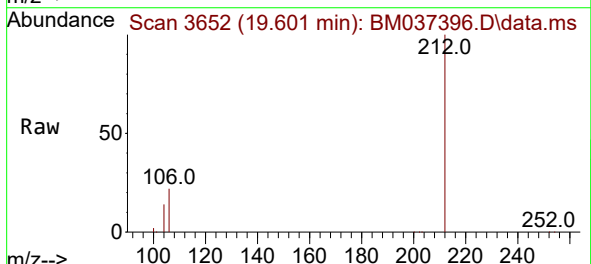

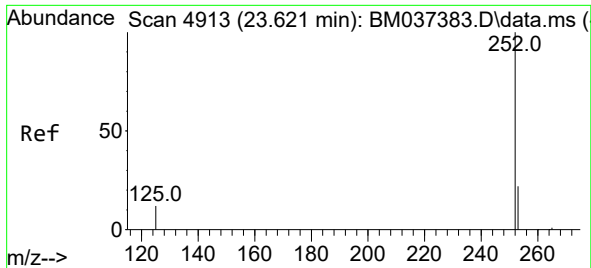

#26
Benzo(a)pyrene
Concen: 0.105 ng/ul
RT: 23.572 min Scan# 41
Delta R.T. -0.047 min
Lab File: BM037396.D
Acq: 07 Nov 2022 17:49

Instrument :
BNA_M
ClientSampleId :
SBLK649

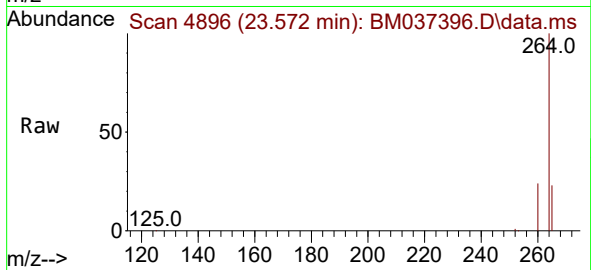

Tgt Ion:252 Resp: 7142
Ion Ratio Lower Upper
252 100
253 49.1 23.8 35.6#
125 44.7 17.2 25.8#

