

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
 Data File : BM037387.D
 Acq On : 07 Nov 2022 12:09
 Operator : CG/JU
 Sample : N5277-19
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Y0

Quant Time: Nov 07 23:27:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 00:30:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.837	152	6130	0.400	ng/u1	0.00
4) Naphthalene-d8	10.633	136	20396	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.474	164	12299	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.213	188	24598	0.400	ng/u1	0.00
17) Chrysene-d12	21.385	240	17478	0.400	ng/u1	0.00
23) Perylene-d12	23.720	264	17399	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	31673	4.070	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.228	152	11002	0.359	ng/u1	0.00
18) Fluoranthene-d10	19.239	212	23366	0.427	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.293	88	1525	0.198	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
Data File : BM037387.D
Acq On : 07 Nov 2022 12:09
Operator : CG/JU
Sample : N5277-19
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Y0

Quant Time: Nov 07 23:27:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:30:18 2022
Response via : Initial Calibration

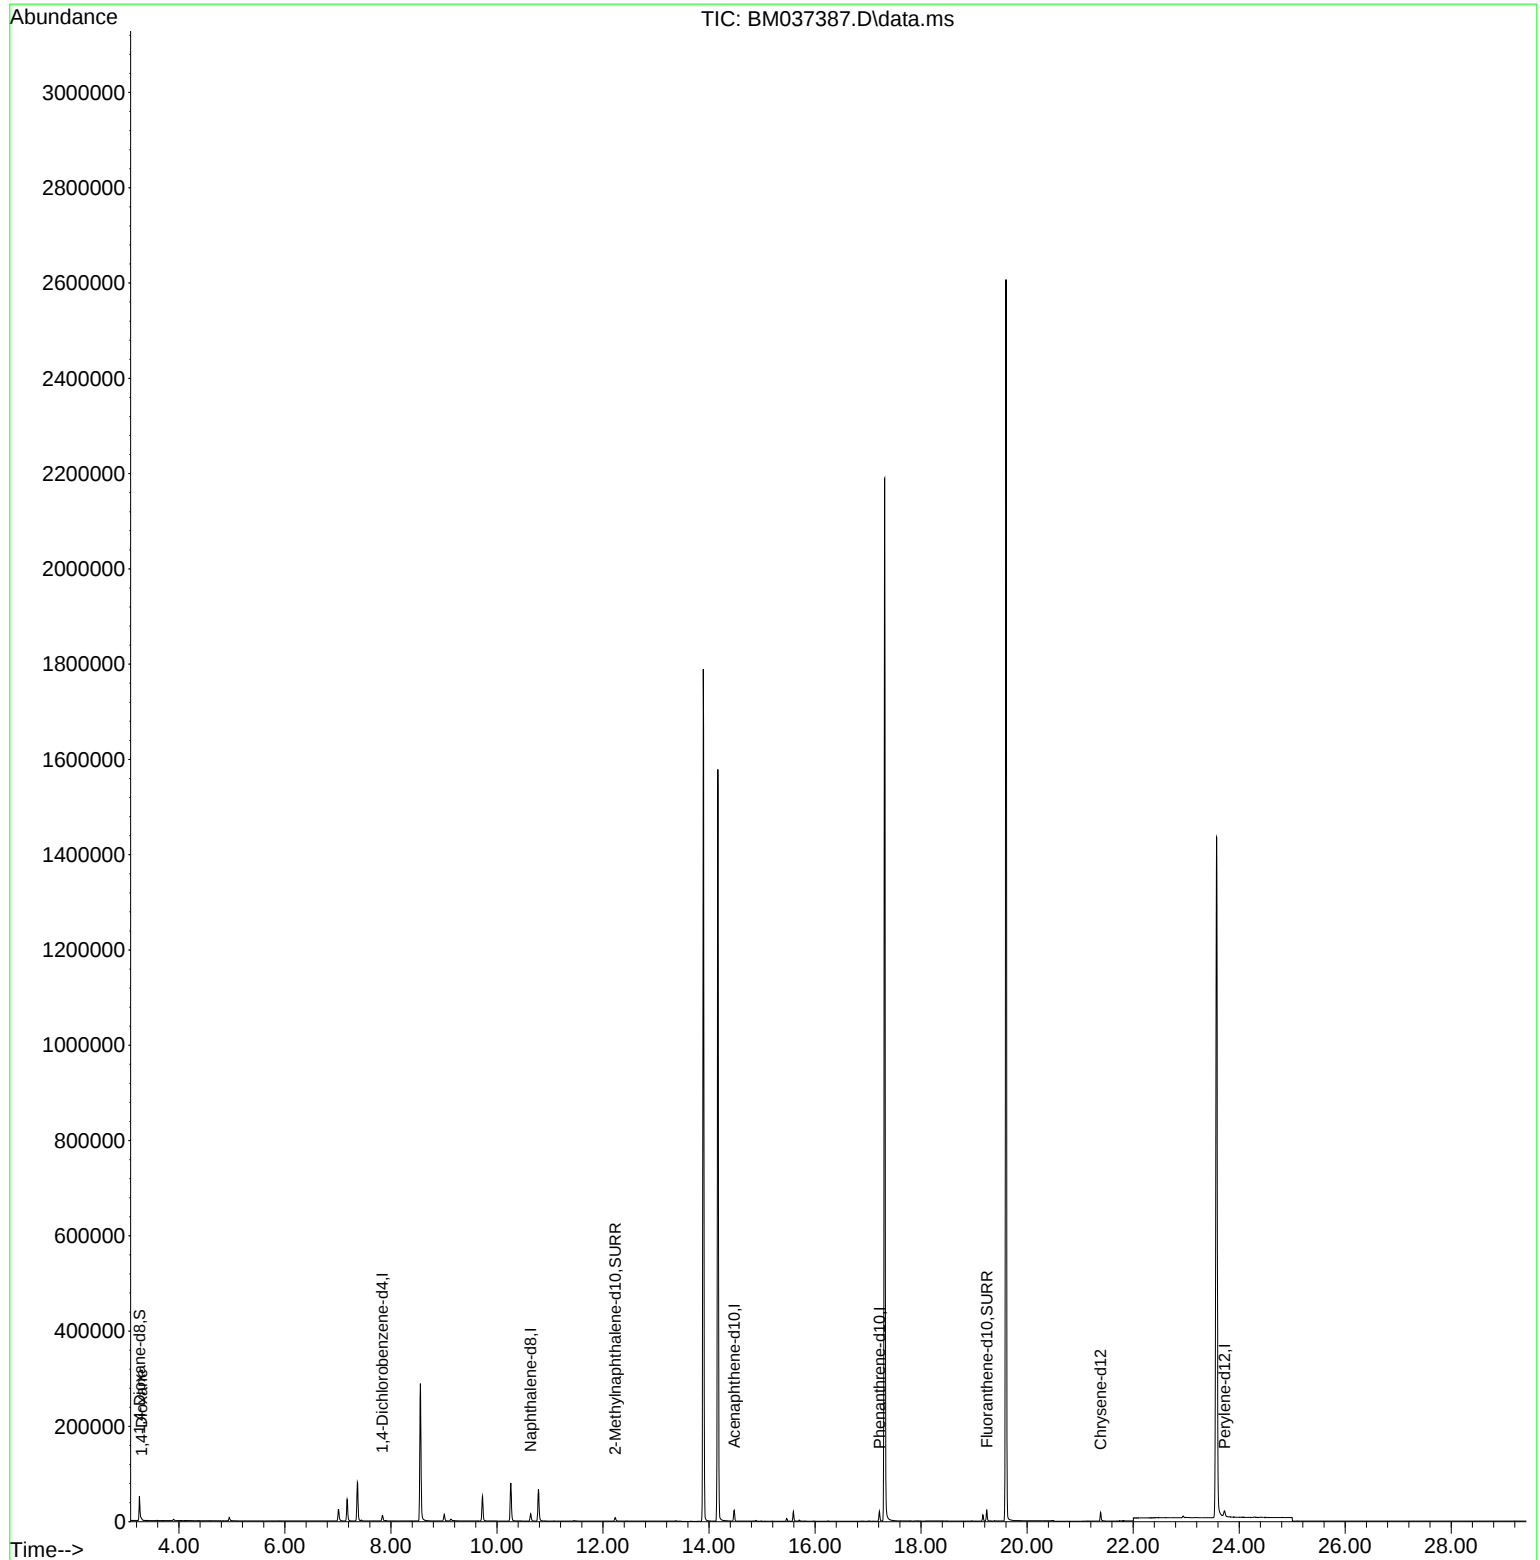

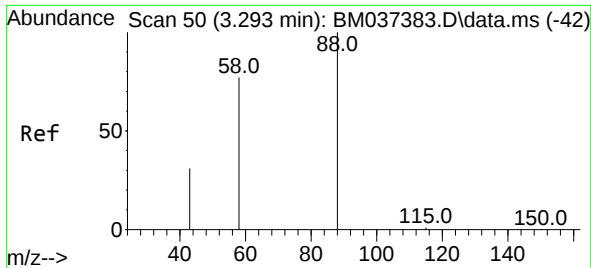

#2
 1,4-Dioxane
 Concen: 0.198 ng/ul
 RT: 3.293 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: BM037387.D
 Acq: 07 Nov 2022 12:09

Instrument :
 BNA_M
 ClientSampleId :
 EW4Y0

Tgt Ion: 88	Resp: 1525
Ion Ratio	Lower Upper
88	100
43	57.1 39.9 59.9
58	57.8 50.2 75.2

