

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
 Data File : BM037391.D
 Acq On : 07 Nov 2022 14:42
 Operator : CG/JU
 Sample : N5277-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4W5

Quant Time: Nov 07 23:07:22 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 00:30:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.837	152	5773	0.400	ng/u1	0.00
4) Naphthalene-d8	10.638	136	19630	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.473	164	11988	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.216	188	24431	0.400	ng/u1	0.00
17) Chrysene-d12	21.386	240	18669	0.400	ng/u1	0.00
23) Perylene-d12	23.724	264	17955	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	25212	3.440	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.228	152	8491	0.288	ng/u1	0.00
18) Fluoranthene-d10	19.238	212	21262	0.364	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.293	88	1310	0.181	ng/u1	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
Data File : BM037391.D
Acq On : 07 Nov 2022 14:42
Operator : CG/JU
Sample : N5277-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4W5

Quant Time: Nov 07 23:07:22 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:30:18 2022
Response via : Initial Calibration

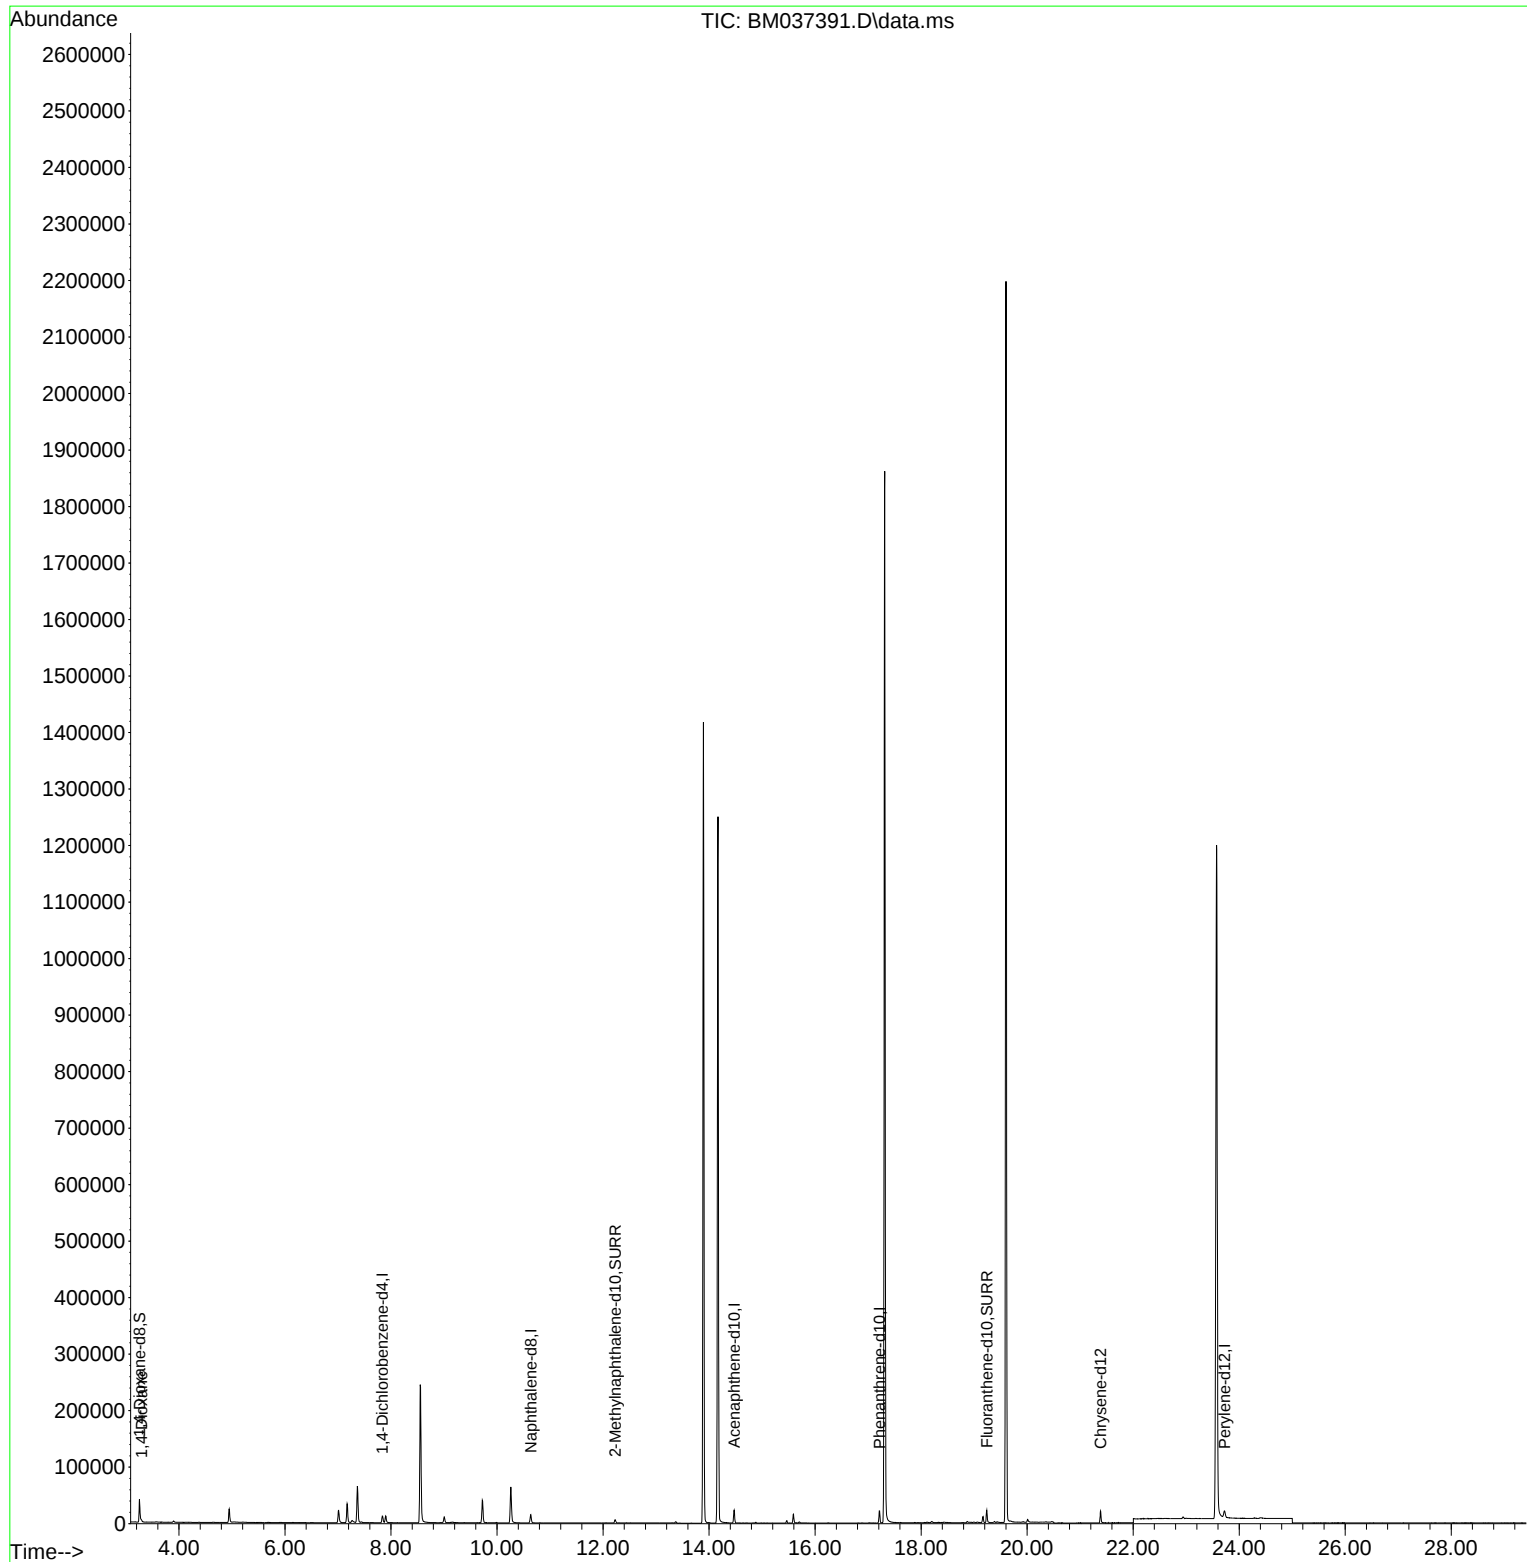

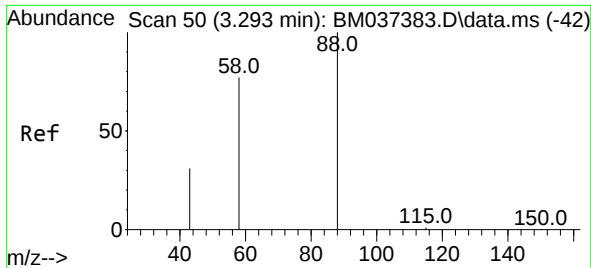

#2
 1,4-Dioxane
 Concen: 0.181 ng/ul
 RT: 3.293 min Scan# 50
 Delta R.T. -0.000 min
 Lab File: BM037391.D
 Acq: 07 Nov 2022 14:42

Instrument :
 BNA_M
 ClientSampleId :
 EW4W5

Tgt Ion: 88	Resp: 1310
Ion Ratio	Lower Upper
88 100	
43 58.6	39.9 59.9
58 53.6	50.2 75.2

