

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
 Data File : BM037404.D
 Acq On : 07 Nov 2022 23:16
 Operator : CG/JU
 Sample : N5407-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Z2

Quant Time: Nov 08 00:19:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 00:30:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.837	152	5778	0.400	ng/ul	0.00
4) Naphthalene-d8	10.633	136	18977	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.470	164	11313	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.209	188	22246	0.400	ng/ul	0.00
17) Chrysene-d12	21.385	240	15088	0.400	ng/ul	0.00
23) Perylene-d12	23.718	264	15311	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	31842	4.341	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.222	152	9622	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.234	212	21181	0.449	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.267	202	1563	0.022	ng/ul#	59
24) Benzo(b)fluoranthene	23.007	252	1790	0.020	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
Data File : BM037404.D
Acq On : 07 Nov 2022 23:16
Operator : CG/JU
Sample : N5407-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Z2

Quant Time: Nov 08 00:19:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:30:18 2022
Response via : Initial Calibration




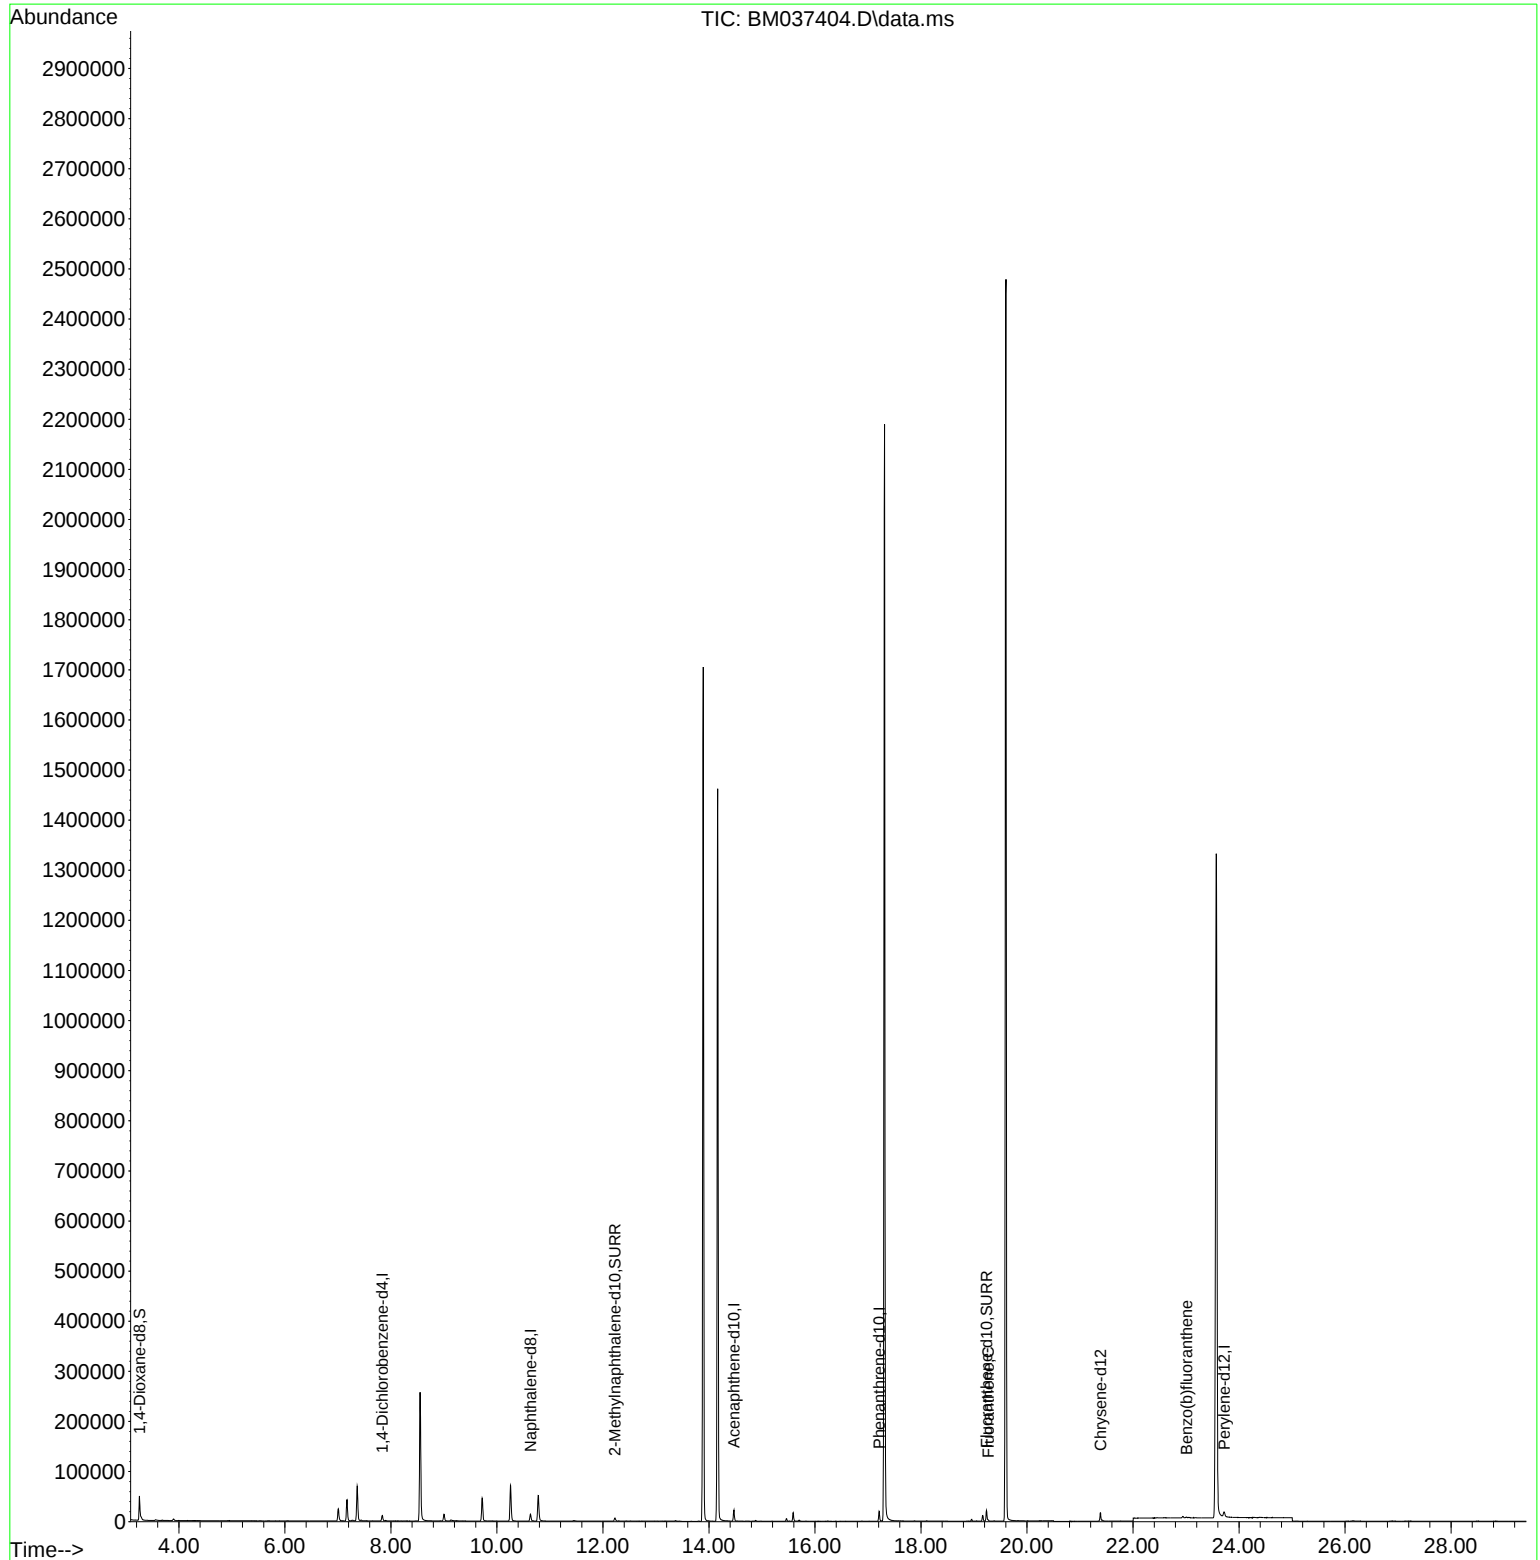


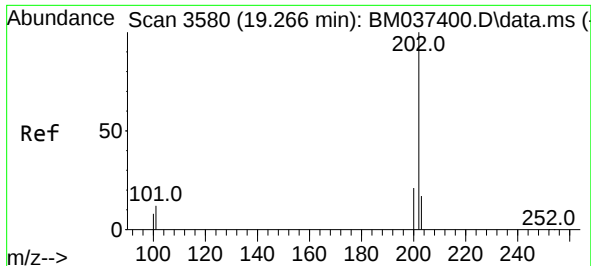

#19
Fluoranthene
Concen: 0.022 ng/ul
RT: 19.267 min Scan# 3580
Delta R.T. -0.004 min
Lab File: BM037404.D
Acq: 07 Nov 2022 23:16

Instrument :
BNA_M
ClientSampleId :
EW4Z2

Tgt Ion:202 Resp: 1563
Ion Ratio Lower Upper
202 100
101 27.6 8.7 13.1#
100 21.3 6.6 10.0#

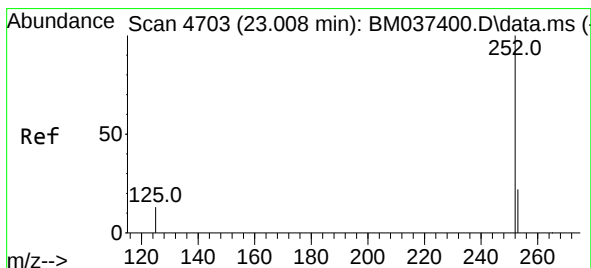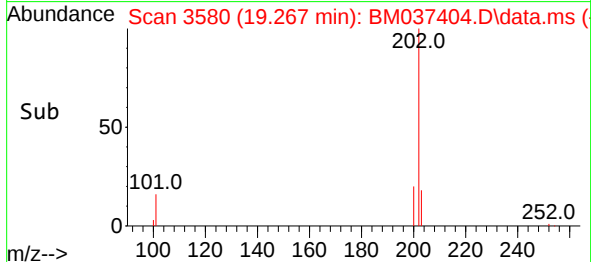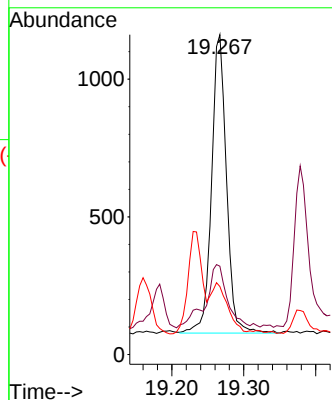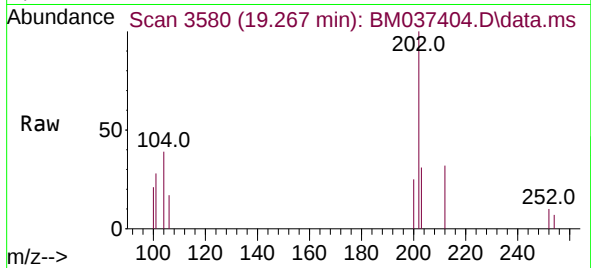

#24
Benzo(b)fluoranthene
Concen: 0.020 ng/ul
RT: 23.007 min Scan# 4703
Delta R.T. -0.004 min
Lab File: BM037404.D
Acq: 07 Nov 2022 23:16

Tgt Ion:252 Resp: 1790
Ion Ratio Lower Upper
252 100
253 73.4 0.0 52.6#
125 76.7 0.0 34.0#

