

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
 Data File : BM037405.D
 Acq On : 07 Nov 2022 23:52
 Operator : CG/JU
 Sample : N5408-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Z2

Quant Time: Nov 08 00:43:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 00:30:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.837	152	5365	0.400	ng/u1	0.00
4) Naphthalene-d8	10.633	136	17761	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.469	164	10670	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.208	188	21289	0.400	ng/u1	0.00
17) Chrysene-d12	21.383	240	14534	0.400	ng/u1	0.00
23) Perylene-d12	23.715	264	14994	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.251	96	25666	3.768	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.222	152	8620	0.323	ng/u1	0.00
18) Fluoranthene-d10	19.233	212	19266	0.424	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.289	88	1264	0.188	ng/u1	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
Data File : BM037405.D
Acq On : 07 Nov 2022 23:52
Operator : CG/JU
Sample : N5408-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Z2


Quant Time: Nov 08 00:43:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:30:18 2022
Response via : Initial Calibration

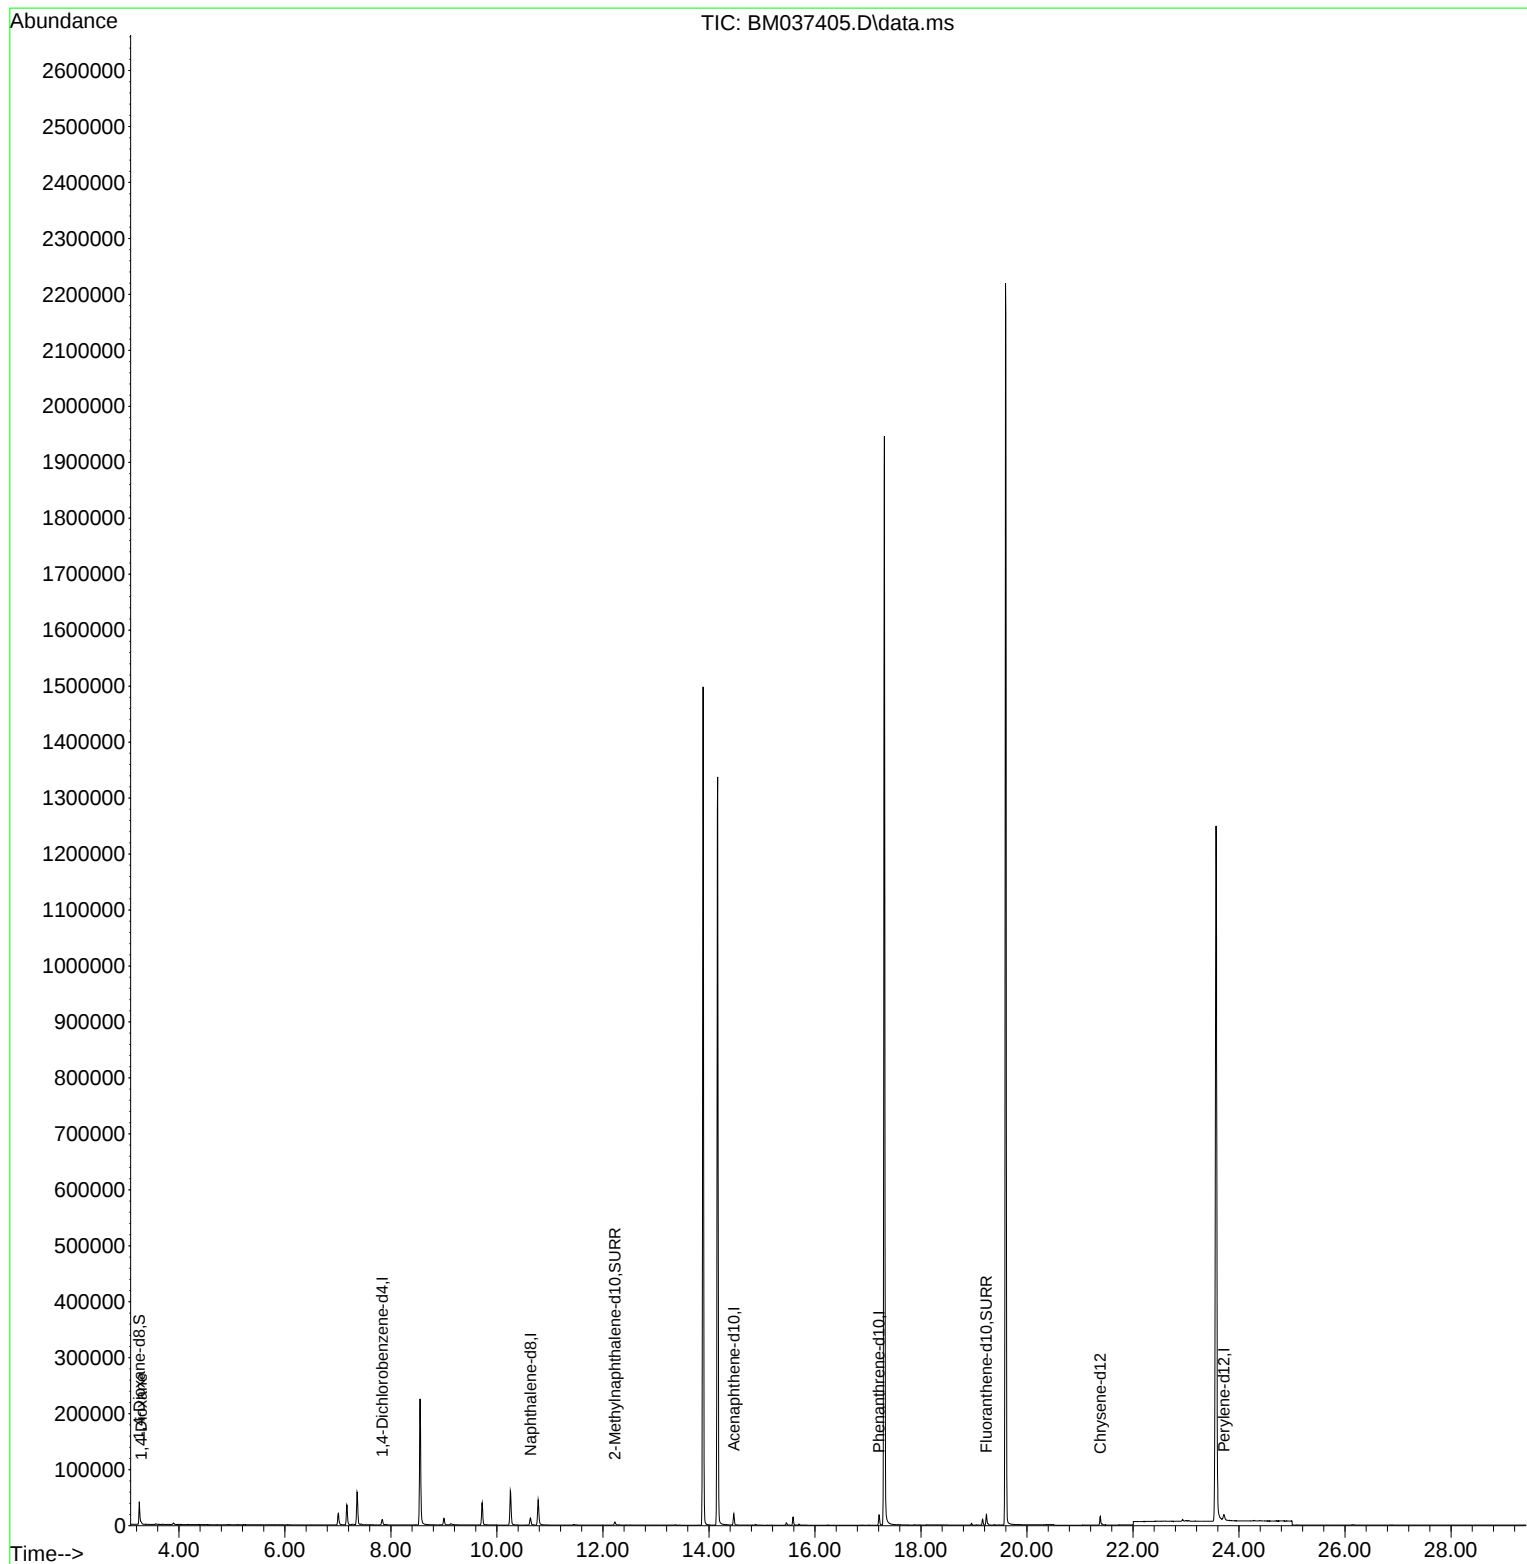

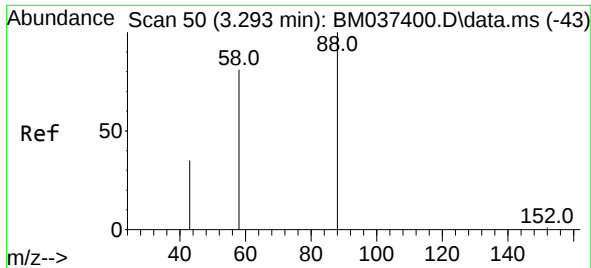

#2
 1,4-Dioxane
 Concen: 0.188 ng/ul
 RT: 3.289 min Scan# 49
 Delta R.T. -0.004 min
 Lab File: BM037405.D
 Acq: 07 Nov 2022 23:52

Instrument :
 BNA_M
 ClientSampleId :
 EW4Z2

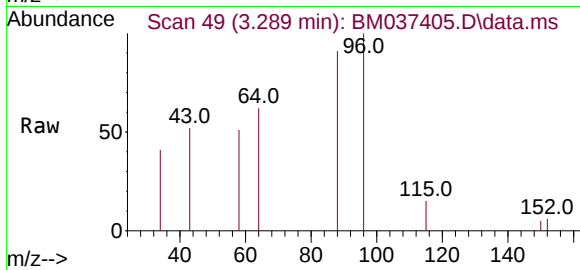

Tgt Ion: 88 Resp: 1264

Ion	Ratio	Lower	Upper
88	100		
43	57.4	39.9	59.9
58	56.4	50.2	75.2

