

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
 Data File : BM037410.D
 Acq On : 08 Nov 2022 02:49
 Operator : CG/JU
 Sample : N5455-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFZ11

Quant Time: Nov 08 03:23:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 00:30:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.833	152	5048	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.627	136	16574	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.469	164	9969	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.208	188	19630	0.400	ng/ul	0.00
17) Chrysene-d12	21.383	240	13315	0.400	ng/ul	0.00
23) Perylene-d12	23.712	264	13788	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.251	96	25721	4.013	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	7503	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.233	212	17709	0.425	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.261	202	1545	0.024	ng/ul#	Qvalue 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
Data File : BM037410.D
Acq On : 08 Nov 2022 02:49
Operator : CG/JU
Sample : N5455-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFZ11

Quant Time: Nov 08 03:23:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:30:18 2022
Response via : Initial Calibration

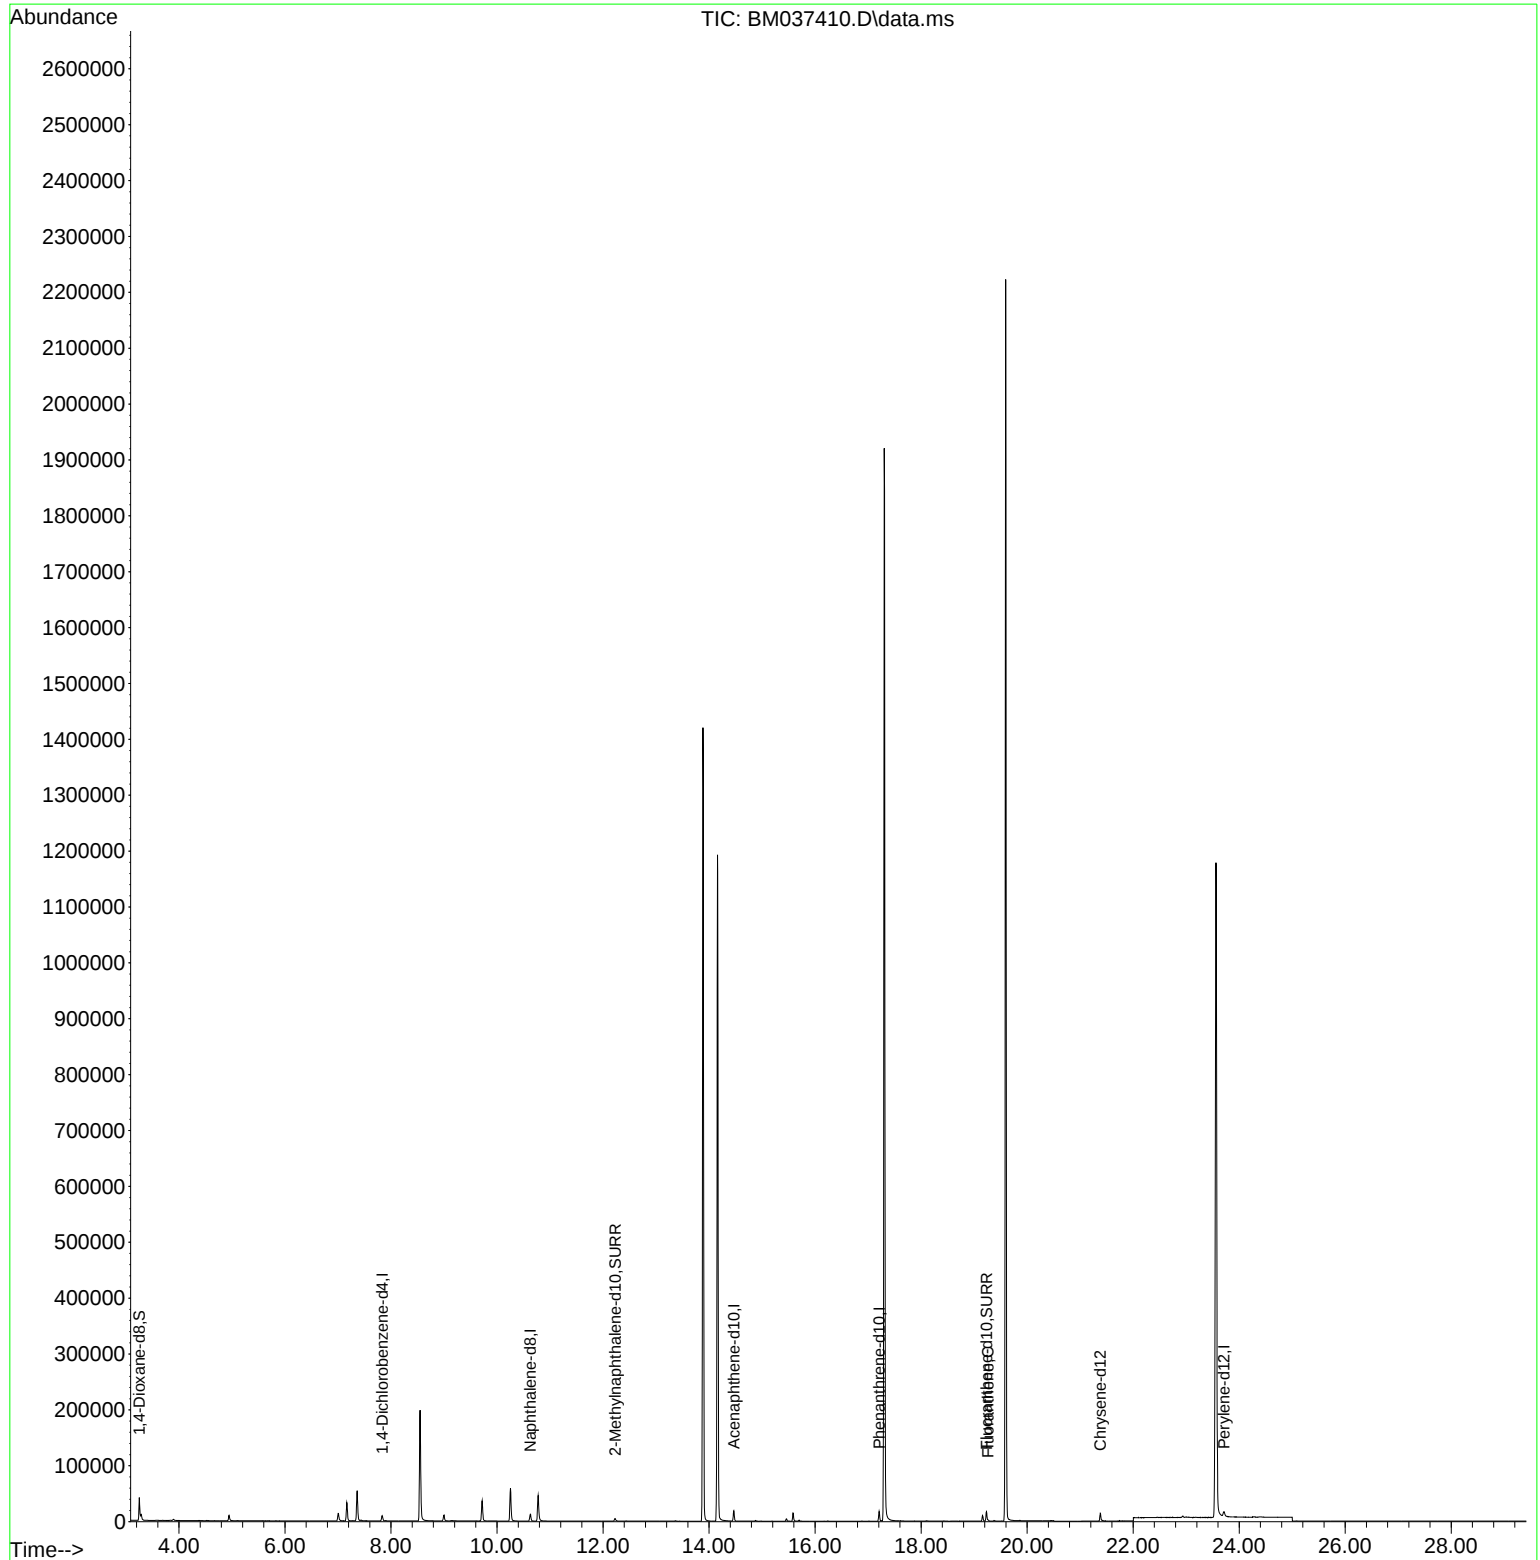

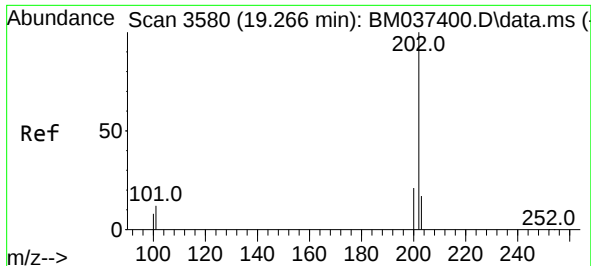

#19

Fluoranthene

Concen: 0.024 ng/ul

RT: 19.261 min Scan# 31

Delta R.T. -0.009 min

Lab File: BM037410.D


Acq: 08 Nov 2022 02:49

Instrument :

BNA_M

ClientSampleId :

BFZ11

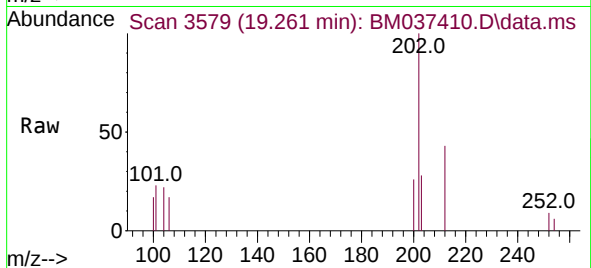

Tgt Ion:202 Resp: 1545

Ion Ratio Lower Upper

202 100

101 23.5 8.7 13.1#

100 17.5 6.6 10.0#

