

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
 Data File : BM037411.D
 Acq On : 08 Nov 2022 03:25
 Operator : CG/JU
 Sample : N5456-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFZ11

Quant Time: Nov 08 04:04:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 07 00:30:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.833	152	5782	0.400	ng/u1	-0.01
4) Naphthalene-d8	10.628	136	18809	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.469	164	11306	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.208	188	21889	0.400	ng/u1	0.00
17) Chrysene-d12	21.380	240	14501	0.400	ng/u1	# 0.00
23) Perylene-d12	23.712	264	14312	0.400	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.251	96	27069	3.687	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.228	152	8187	0.290	ng/u1	0.00
18) Fluoranthene-d10	19.233	212	18722	0.413	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.289	88	5893	0.812	ng/u1	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110722\
Data File : BM037411.D
Acq On : 08 Nov 2022 03:25
Operator : CG/JU
Sample : N5456-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFZ11


Quant Time: Nov 08 04:04:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:30:18 2022
Response via : Initial Calibration

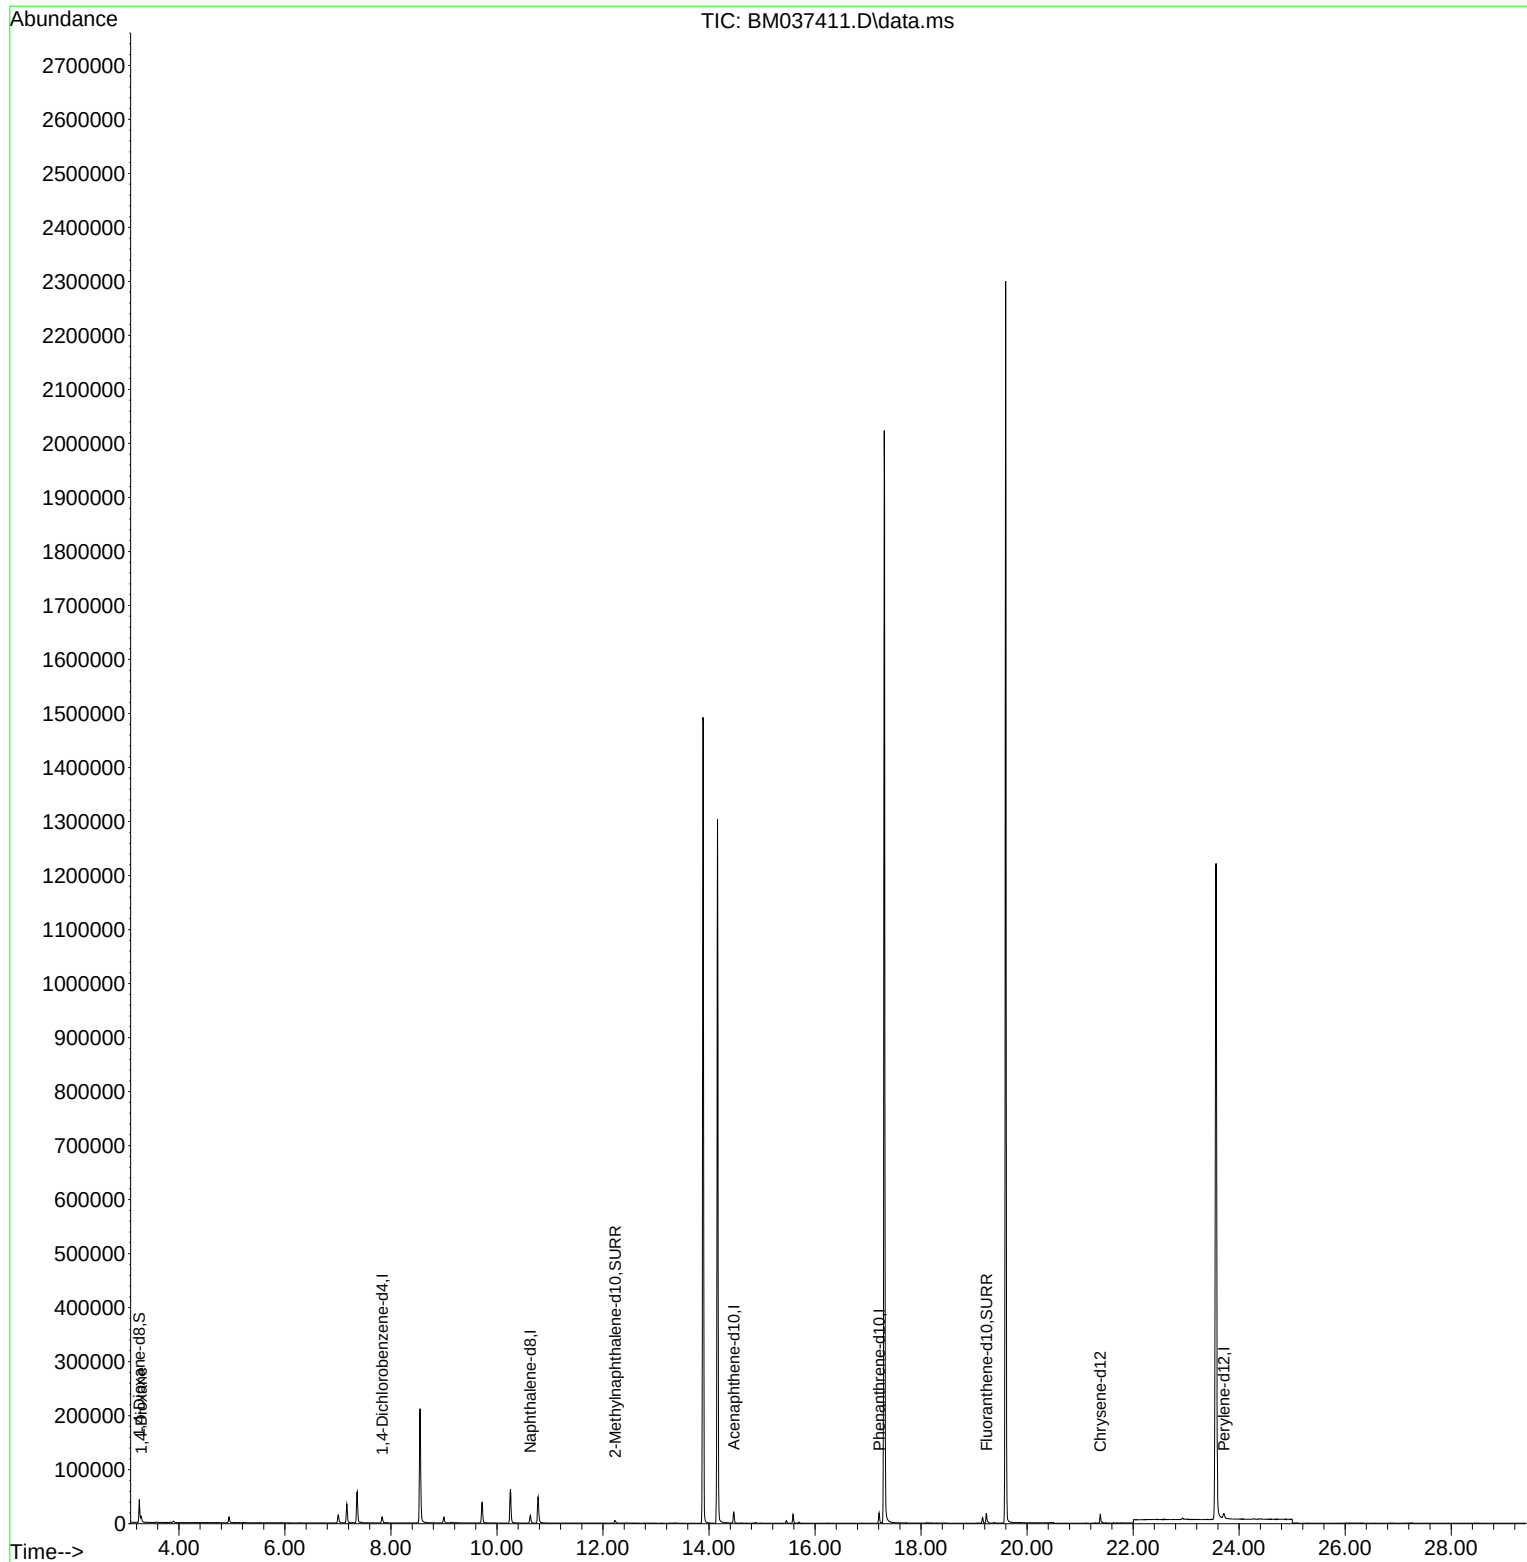

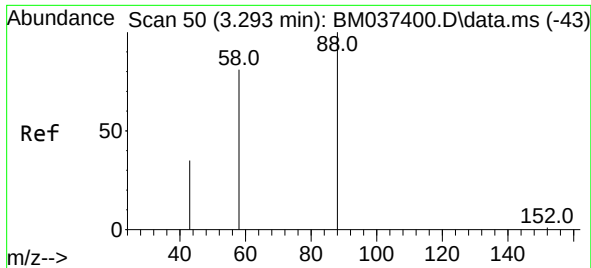

#2
 1,4-Dioxane
 Concen: 0.812 ng/ul
 RT: 3.289 min Scan# 49
 Delta R.T. -0.004 min
 Lab File: BM037411.D
 Acq: 08 Nov 2022 03:25

Instrument :
 BNA_M
 ClientSampleId :
 BFZ11

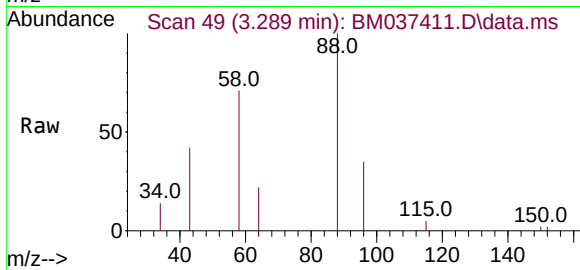

Tgt Ion: 88 Resp: 5893

Ion	Ratio	Lower	Upper
88	100		
43	42.3	39.9	59.9
58	70.9	50.2	75.2

