

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110817\
 Data File : BM012824.D
 Acq On : 08 Nov 2017 16:57
 Operator : SJ/JU
 Sample : I5876-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B-20(3.5-4)-101817

Quant Time: Nov 09 01:34:12 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 09 01:31:40 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	119457	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	489221	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	283458	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	575034	20.00	ng/ul	0.00
77) Chrysene-d12	21.36	240	575806	20.00	ng/ul	0.00
85) Perylene-d12	23.64	264	651016	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.29	96	11755	5.32	ng/uL	0.00
5) Phenol-d5	6.97	99	269740	30.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	154193	32.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	230587	31.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	210846	27.48	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	117521	32.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	134299	32.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	242834	28.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	312386	38.18	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	775650	33.07	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	942247	32.48	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	56323	14.99	ng/ul	0.00
57) Fluorene-d10	15.43	176	642964	32.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	38694	10.19	ng/ul	0.00
70) Anthracene-d10	17.28	188	914740	32.92	ng/ul	0.00
78) Pyrene-d10	19.57	212	948972	35.52	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.50	264	1089223	35.39	ng/ul	0.00


Target Compounds						Ovalue
6) Phenol	7.00	94	20180	2.21	ng/ul	93
44) Dimethylphthalate	13.89	163	100122	4.30	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110817\
Data File : BM012824.D
Acq On : 08 Nov 2017 16:57
Operator : SJ/JU
Sample : I5876-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-20(3.5-4)-101817

Quant Time: Nov 09 01:34:12 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 09 01:31:40 2017
Response via : Initial Calibration

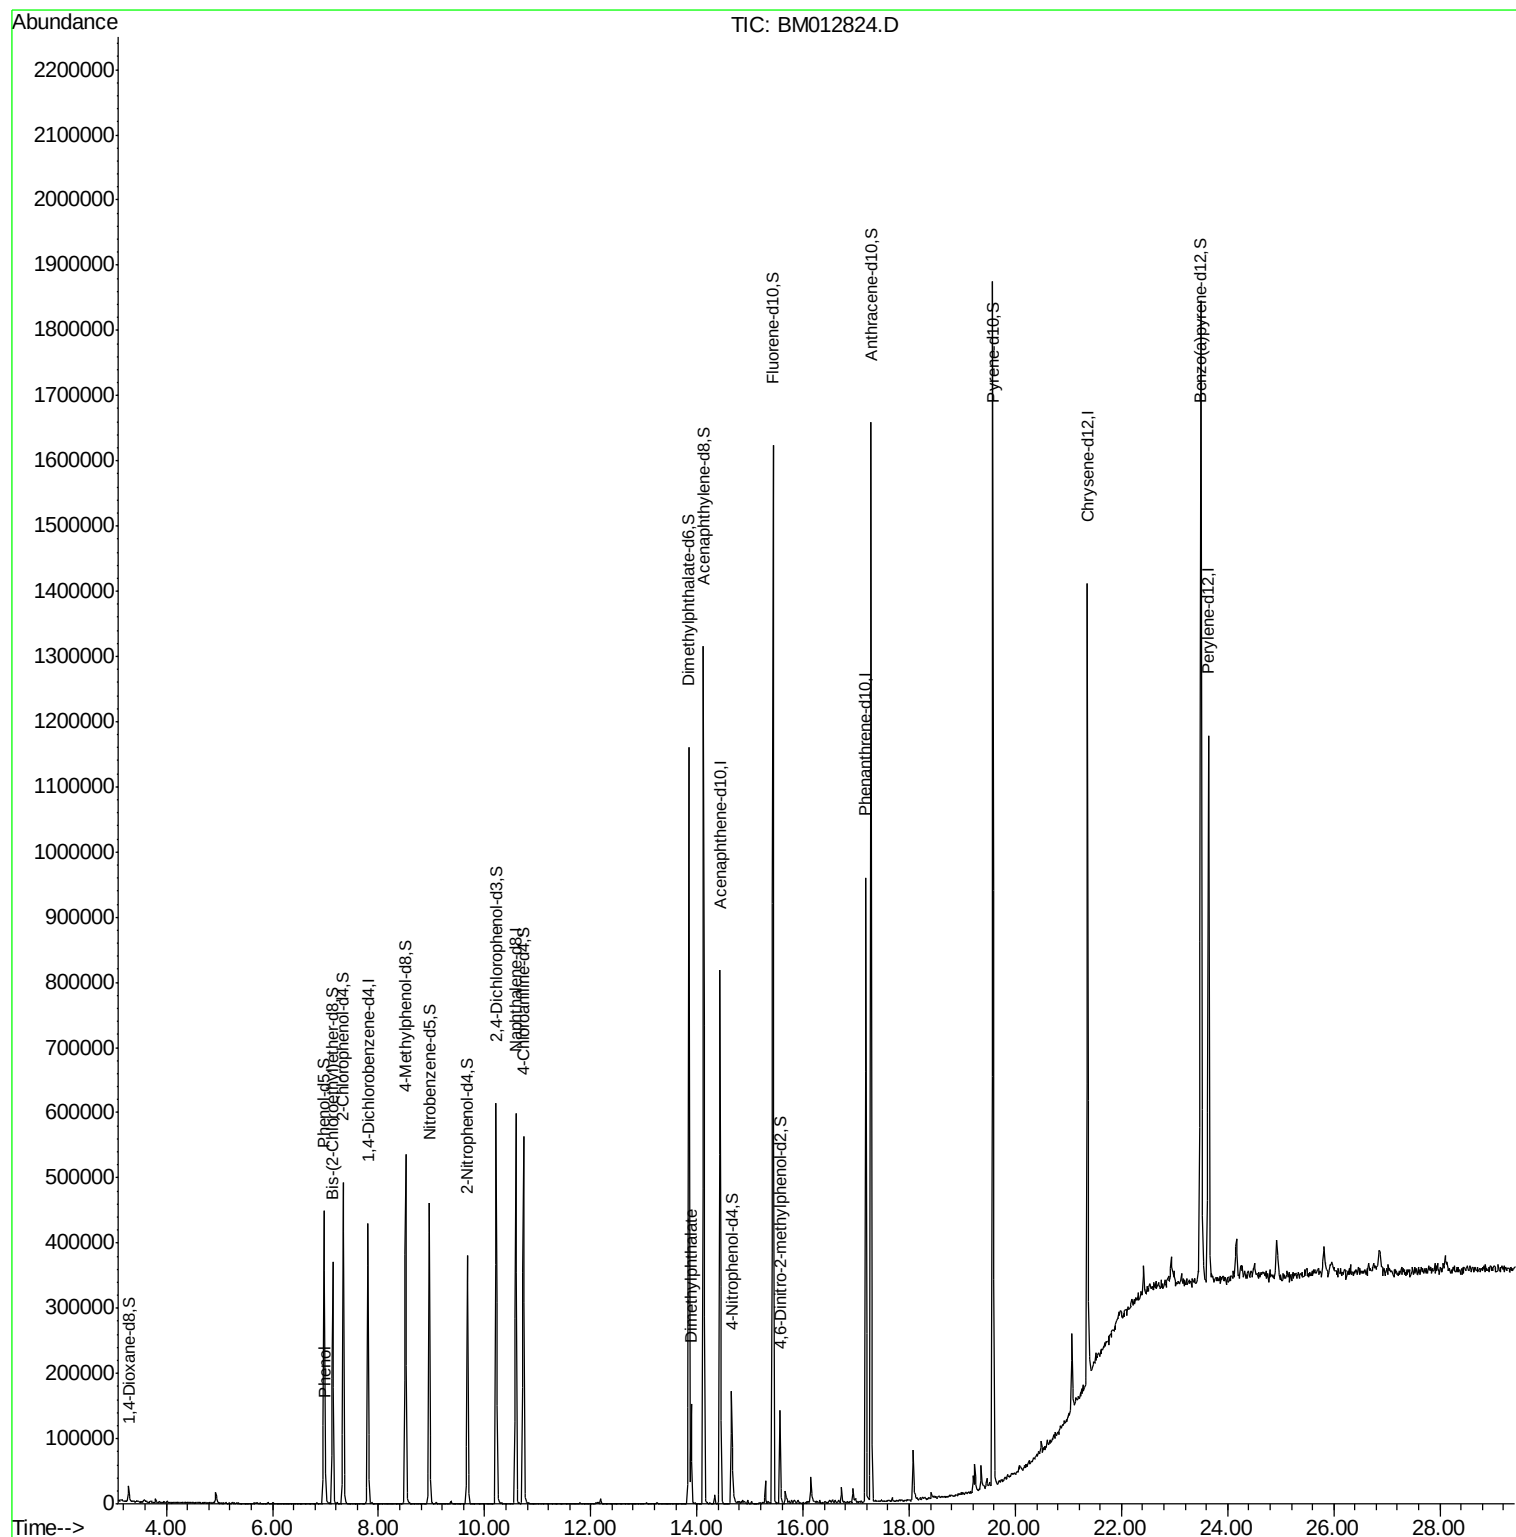

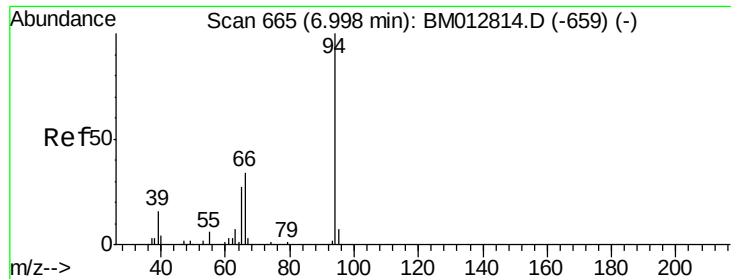

#6

Phenol

Concen: 2.21 ng/ul

RT: 7.00 min Scan# 666

Delta R.T. 0.01 min

Lab File: BM012824.D

Acq: 08 Nov 2017 16:57

Instrument :


BNA_M

ClientSampleId :

B-20(3.5-4)-101817

Tot Ion: 94 Resp: 20180


Ion	Ratio	Lower	Upper
94	100		
65	27.8	21.0	31.6
66	42.4	29.3	43.9

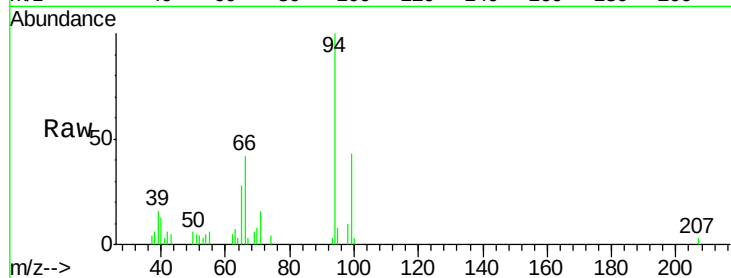


Abundance Ion 94.00 (93.70 to 94.70): BM012814.D (-659) (-)

Ion 65.00 (64.70 to 65.70): BM012814.D (-659) (-)

Ion 66.00 (65.70 to 66.70): BM012814.D (-659) (-)

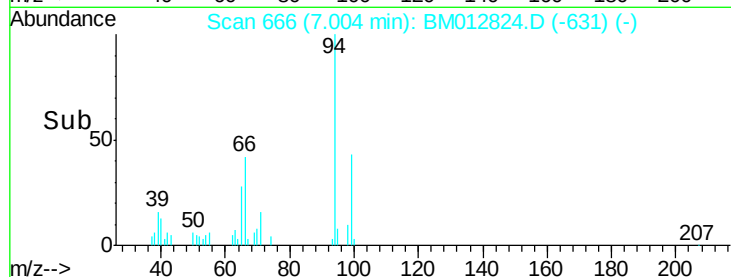

Time-->

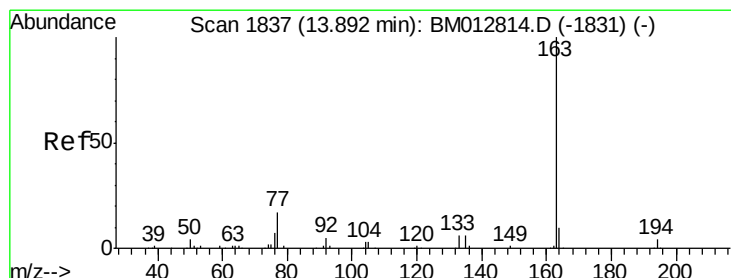

#44

Dimethylphthalate

Concen: 4.30 ng/ul

RT: 13.89 min Scan# 1837


Delta R.T. -0.00 min

Lab File: BM012824.D

Acq: 08 Nov 2017 16:57

Tgt Ion:163 Resp: 100122


Ion	Ratio	Lower	Upper
163	100		
194	4.8	3.2	4.8
164	10.0	7.8	11.8

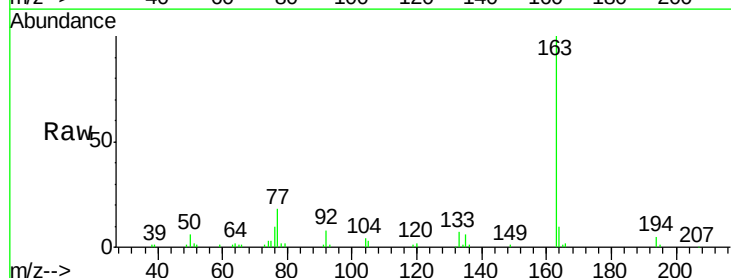

Abundance Ion 163.00 (162.70 to 163.70): BM012814.D (-1831) (-)

Ion 194.00 (193.70 to 194.70): BM012814.D (-1831) (-)

Ion 164.00 (163.70 to 164.70): BM012814.D (-1831) (-)

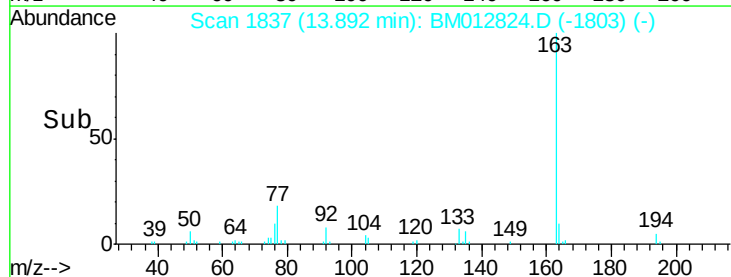

Time-->