

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110817\
 Data File : BM012825.D
 Acq On : 08 Nov 2017 17:33
 Operator : SJ/JU
 Sample : I5876-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B-20(5-6)-101817

Quant Time: Nov 09 01:34:22 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 09 01:31:40 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	109238	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	435979	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	247795	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	813537	20.00	ng/ul	0.10
77) Chrysene-d12	21.36	240	525694	20.00	ng/ul	0.00
85) Perylene-d12	23.64	264	583900	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	11172	5.53	ng/uL	0.00
5) Phenol-d5	6.97	99	250623	30.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	143888	32.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	212843	31.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	216373	30.84	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	106696	33.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	120505	32.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	223110	29.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	289848	39.75	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	683811	33.35	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	843631	33.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	30352	9.24	ng/ul	0.00
57) Fluorene-d10	15.43	176	568468	32.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	19402	3.61	ng/ul	0.00
70) Anthracene-d10	17.28	188	813537	20.70	ng/ul	0.00
78) Pyrene-d10	19.57	212	880429	36.09	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.50	264	1025181	37.13	ng/ul	0.00

Target Compounds


						Ovalue
6) Phenol	7.00	94	22031	2.64	ng/ul	93
44) Dimethylphthalate	13.89	163	130597	6.42	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110817\
Data File : BM012825.D
Acq On : 08 Nov 2017 17:33
Operator : SJ/JU
Sample : I5876-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-20(5-6)-101817

Quant Time: Nov 09 01:34:22 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM110417MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 09 01:31:40 2017
Response via : Initial Calibration

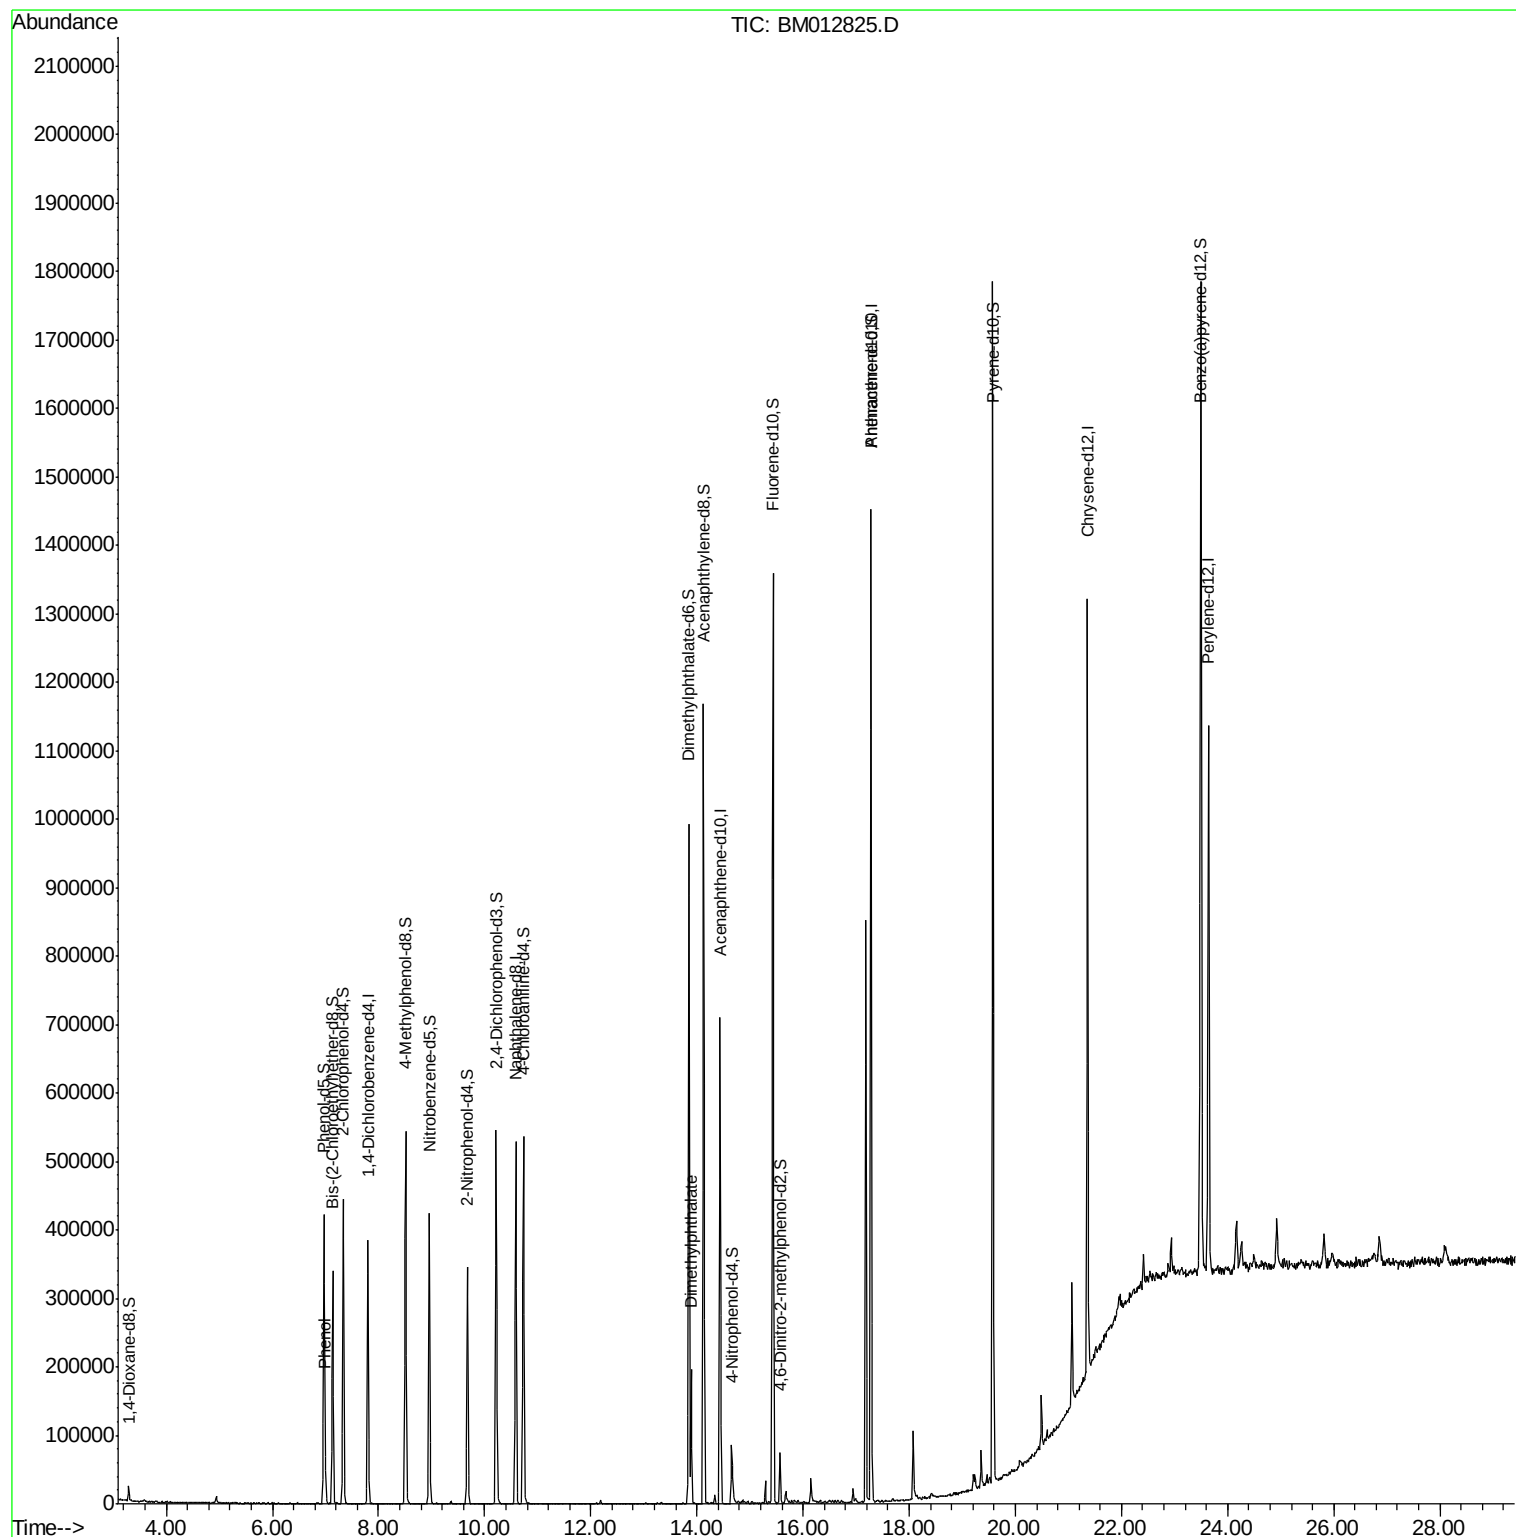

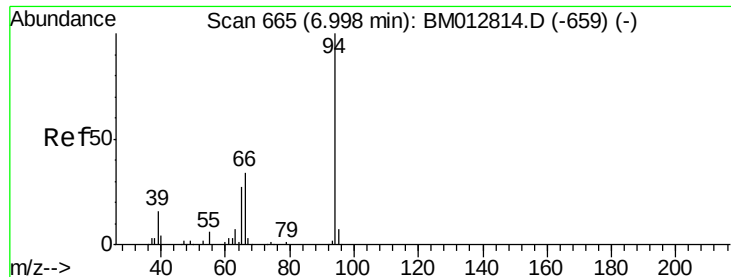

#6

Phenol

Concen: 2.64 ng/ul

RT: 7.00 min Scan# 665

Delta R.T. 0.00 min

Lab File: BM012825.D

Acq: 08 Nov 2017 17:33

Instrument :

BNA_M

ClientSampleId :

B-20(5-6)-101817


Tot Ion: 94 Resp: 22031

Ion Ratio Lower Upper

94 100

65 27.5 21.0 31.6




66 42.8 29.3 43.9

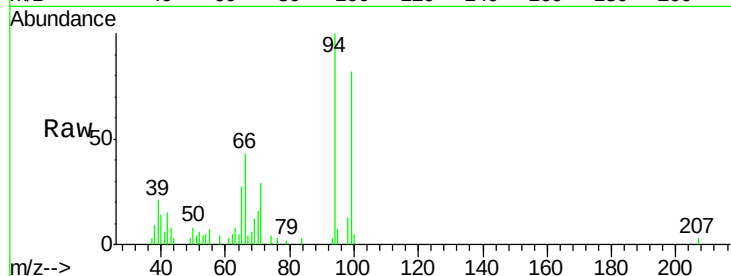

Abundance Ion 94.00 (93.70 to 94.70): BM012814.D (-659) (-)

Ion 65.00 (64.70 to 65.70): BM012814.D (-659) (-)

Ion 66.00 (65.70 to 66.70): BM012814.D (-659) (-)

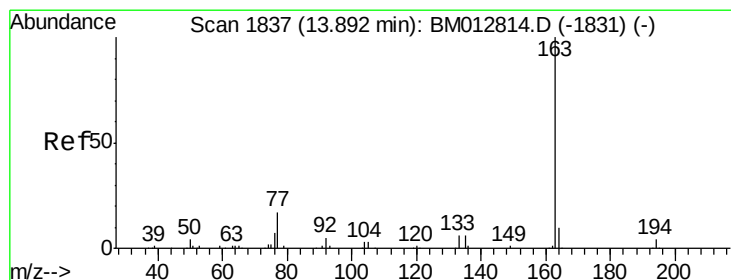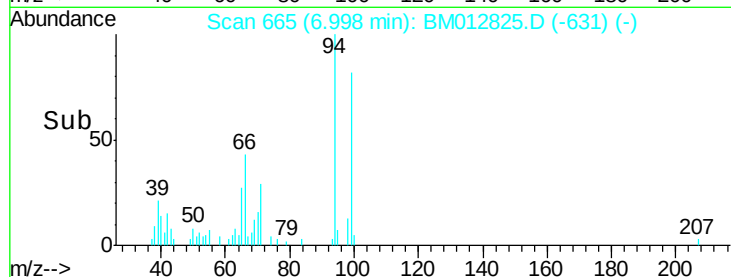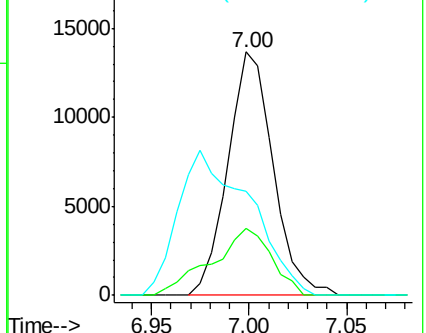

#44

Dimethylphthalate

Concen: 6.42 ng/ul

RT: 13.89 min Scan# 1837

Delta R.T. 0.00 min

Lab File: BM012825.D

Acq: 08 Nov 2017 17:33


Tgt Ion: 163 Resp: 130597

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.3 7.8 11.8

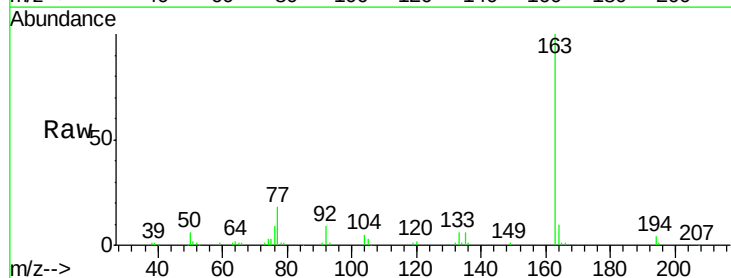

Abundance Ion 163.00 (162.70 to 163.70): BM012814.D (-1831) (-)

Ion 194.00 (193.70 to 194.70): BM012814.D (-1831) (-)

Ion 164.00 (163.70 to 164.70): BM012814.D (-1831) (-)

