


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110822\
 Data File : BM037420.D
 Acq On : 08 Nov 2022 09:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 09 02:08:14 2022

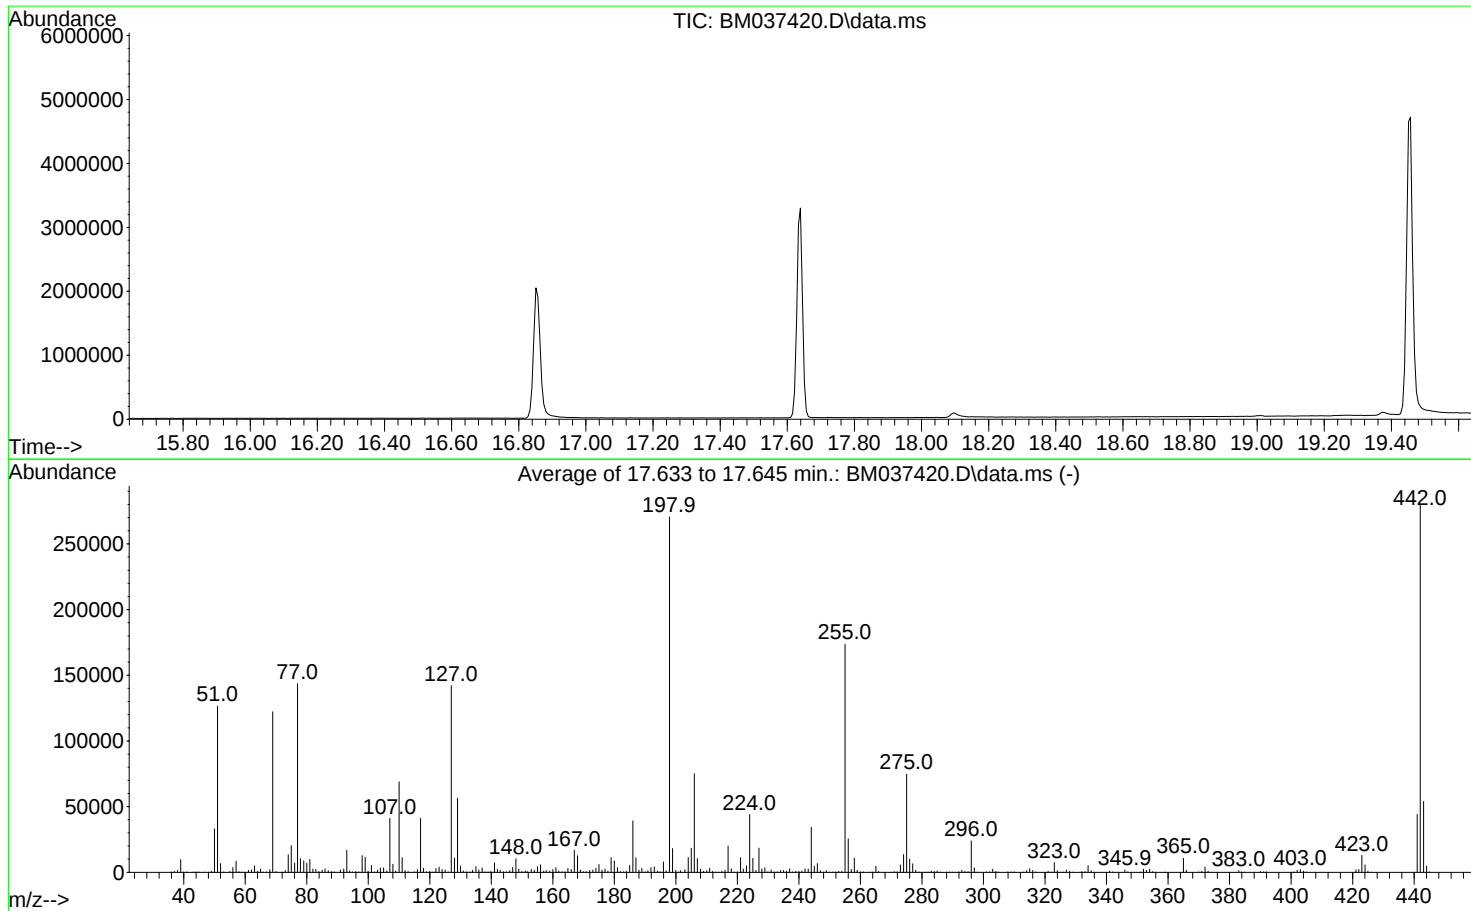




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	126447	PASS
68	69	0.00	2	1.5	1843	PASS
69	198	0.00	100	45.2	122226	PASS
70	69	0.00	2	0.6	703	PASS
127	198	10	80	52.6	142157	PASS
197	198	0.00	2	0.4	1138	PASS
198	198	100	100	100.0	270464	PASS
199	198	5	9	6.7	18099	PASS
275	198	10	60	27.6	74643	PASS
365	198	1	100	4.0	10708	PASS
441	198	0.01	100	16.3	44021	PASS
442	442	50	100	100.0	280085	PASS
443	442	15	24	19.2	53875	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110822\
Data File : BM037420.D
Acq On : 08 Nov 2022 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 09 06:49:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 02:08:14 2022
Response via : Initial Calibration

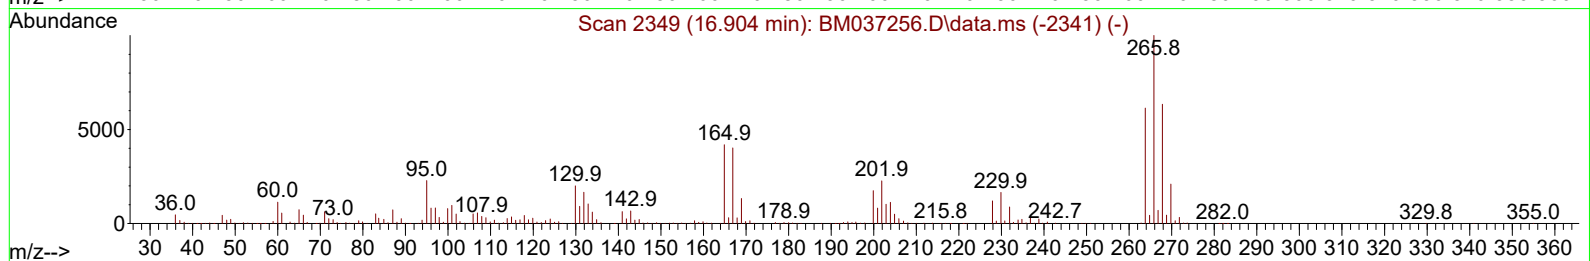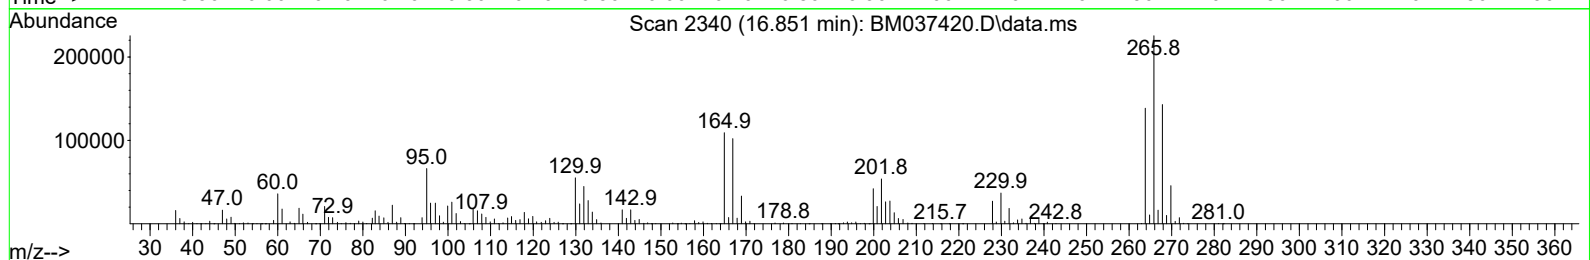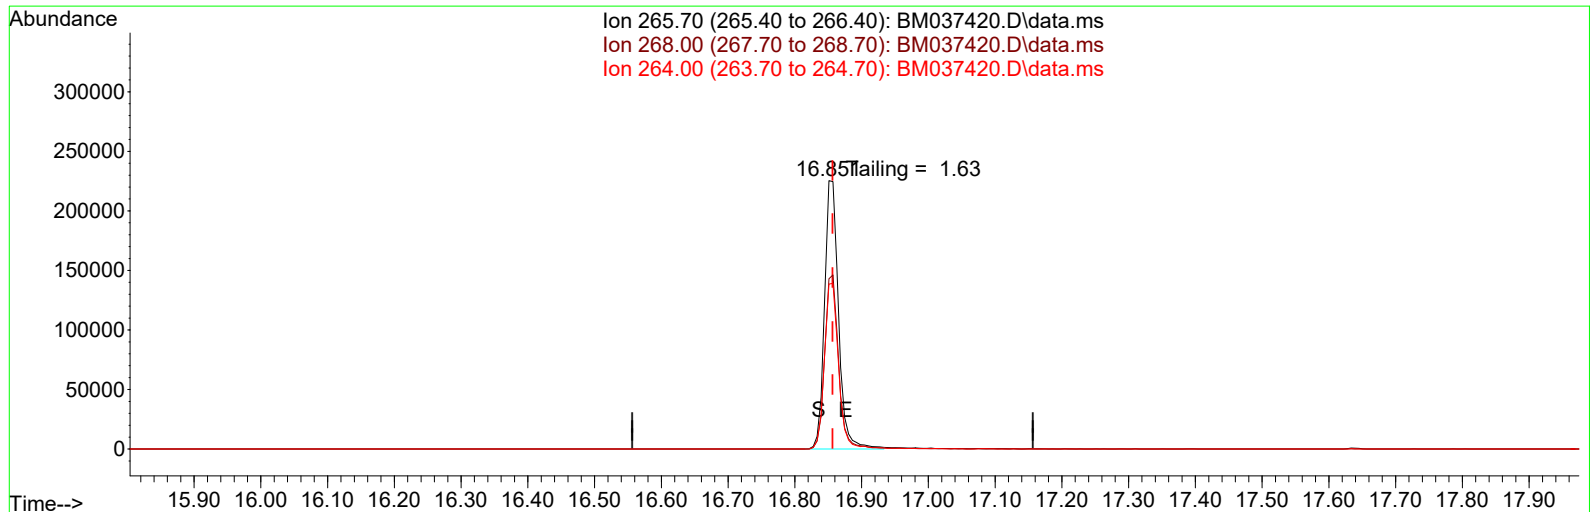

TIC: BM037420.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.006) 0.00 ng




response 331277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.43
264.00	61.40	61.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110822\
Data File : BM037420.D
Acq On : 08 Nov 2022 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 09 06:49:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 02:08:14 2022
Response via : Initial Calibration

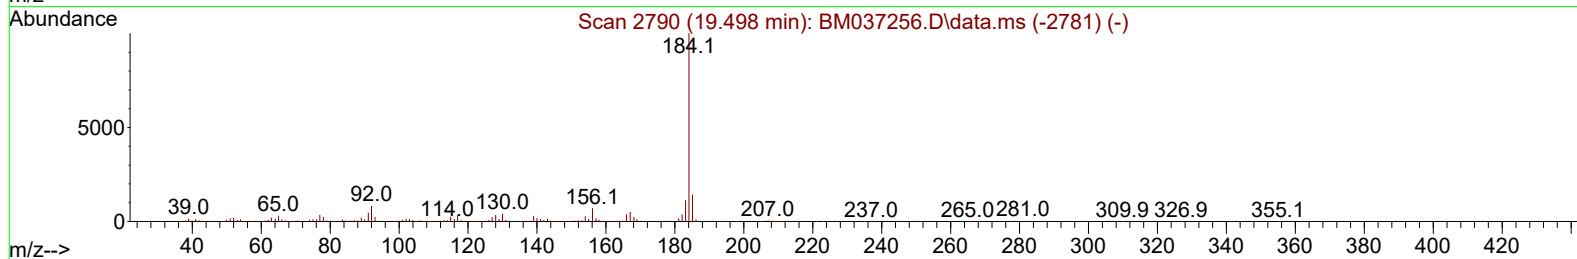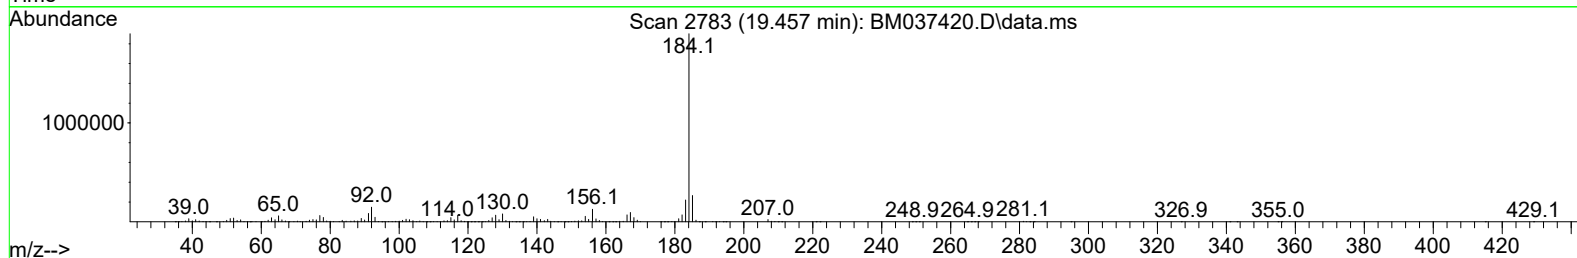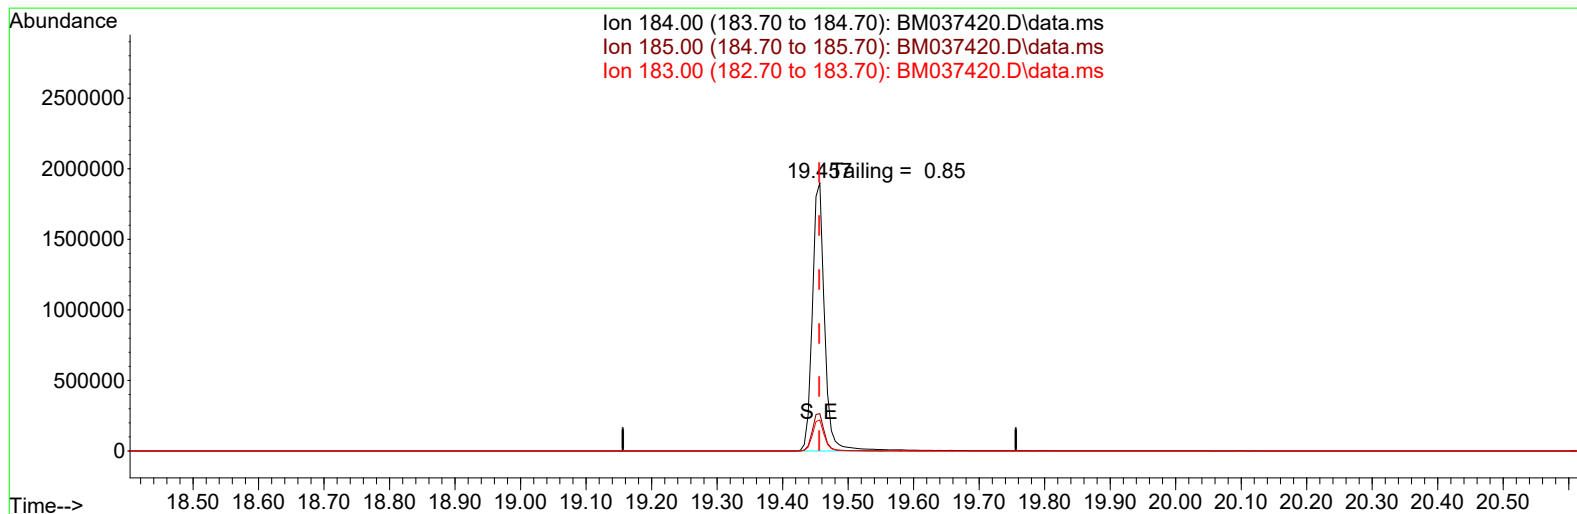

TIC: BM037420.D\data.ms

(77) Benzidine

19.457min (+ 0.000) 447232.15 ng

response 2460806

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.96
183.00	11.20	11.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/8/2022	BNA_M	<u>BM037420.D</u>
Compound Name	Response	Retention Time
DDT	1177412	20.674
DDD	17943	20.239
DDE	1082	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19025	1196437	1.59

Instrument :
BNA_M
ClientSampleId :
DFTPP