




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048547.D
Acq On : 09 Nov 2024 02:49
Operator : RC/JU
Sample : PB164769TB
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB620

Manual IntegrationsAPPROVED

Quant Time: Nov 09 03:31:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 07 22:50:20 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/11/2024

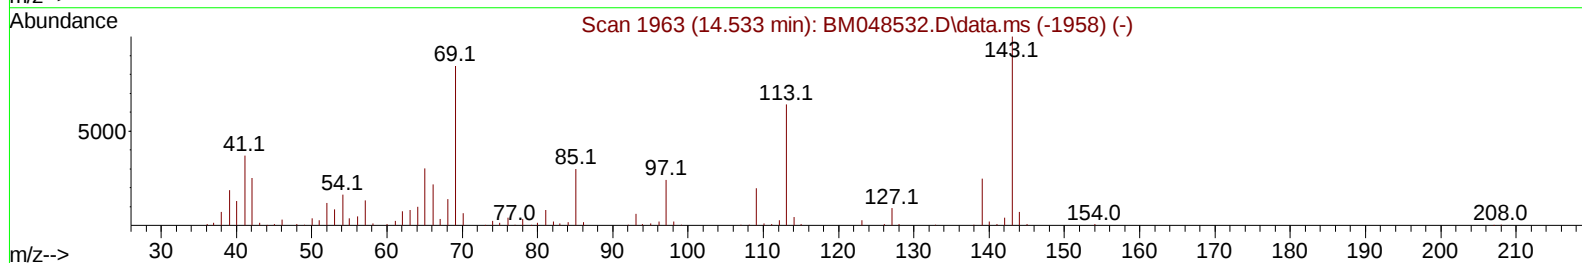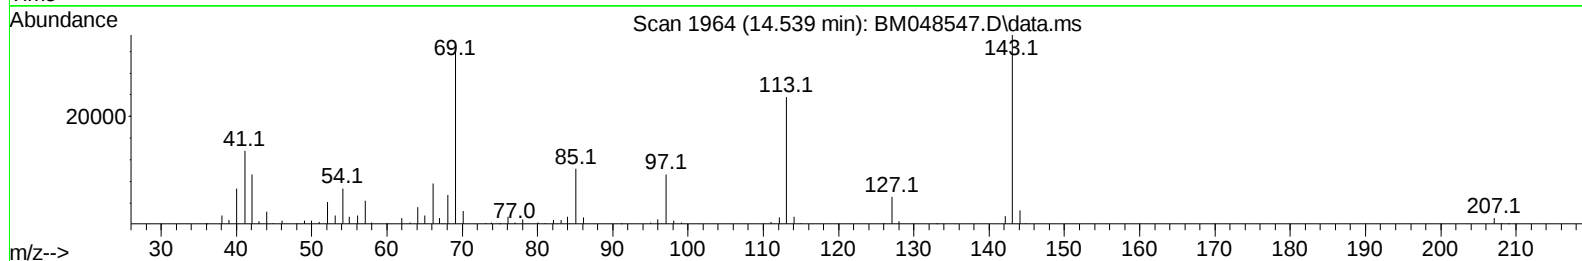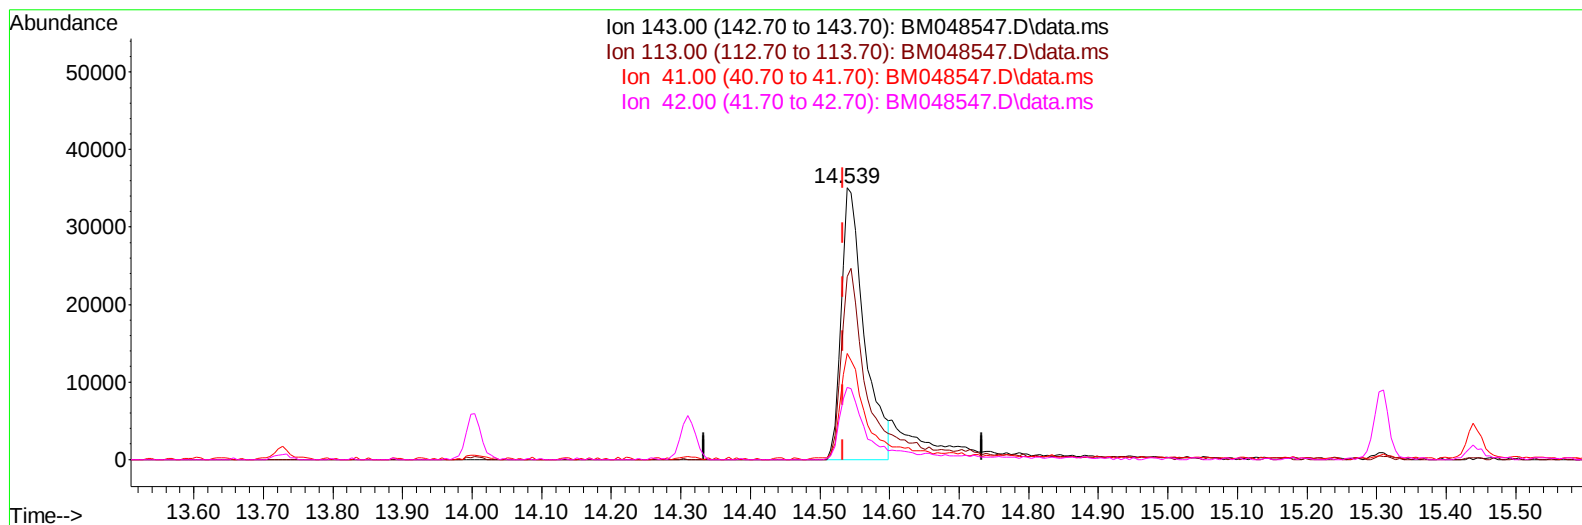

TIC: BM048547.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.539min (+ 0.006) 20.14 ng/u1

response 80444

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.50	67.27
41.00	36.20	39.02
42.00	24.50	26.61




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048547.D
Acq On : 09 Nov 2024 02:49
Operator : RC/JU
Sample : PB164769TB
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB620

Manual IntegrationsAPPROVED

Quant Time: Nov 09 03:31:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 07 22:50:20 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/11/2024

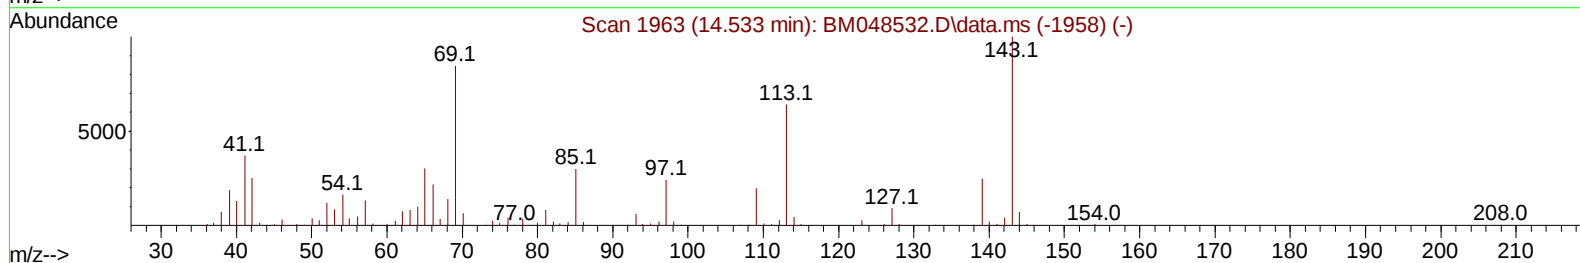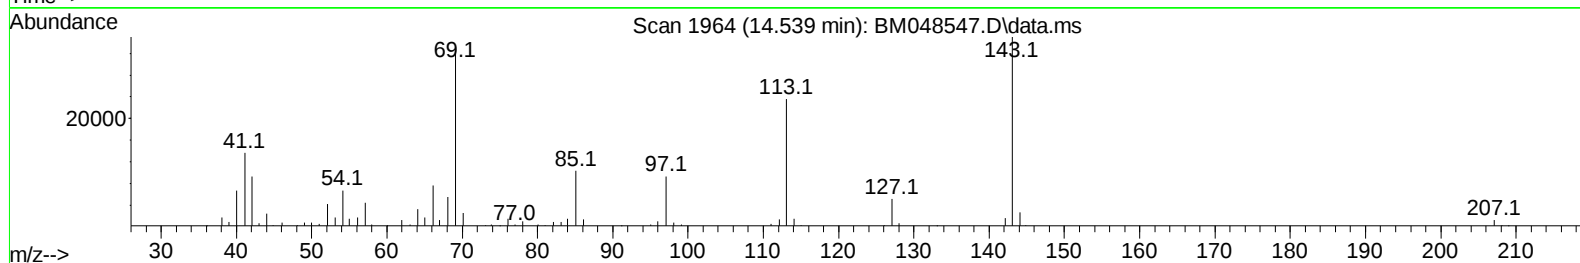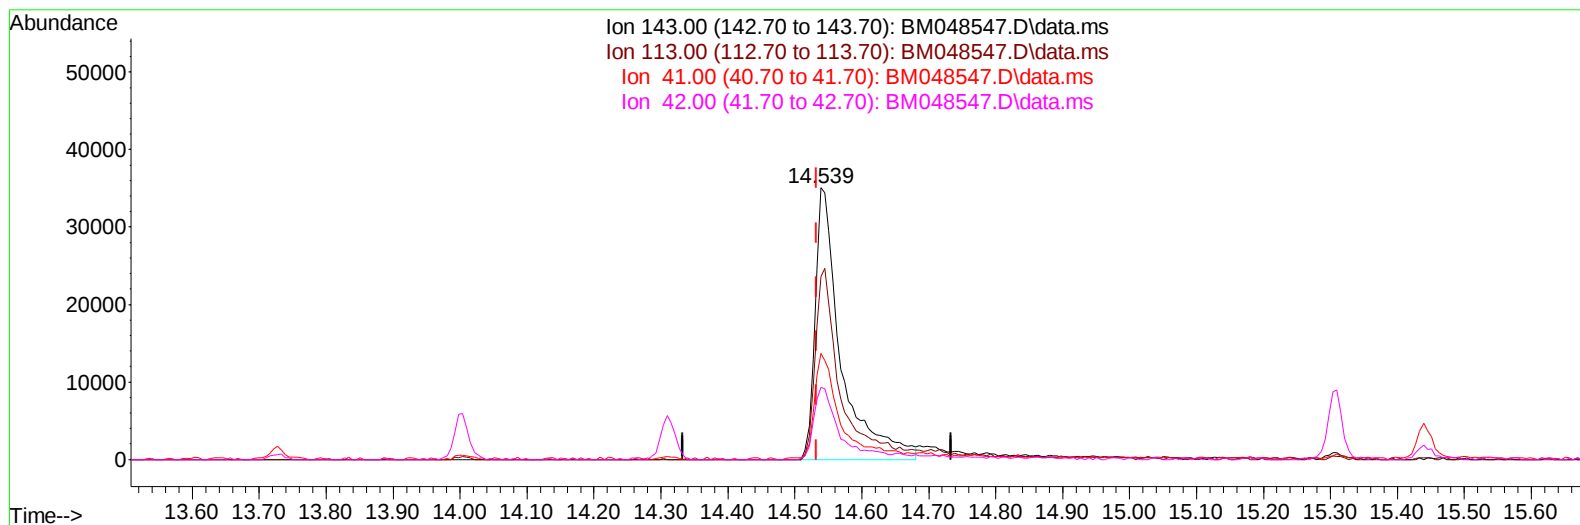

TIC: BM048547.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.539min (+ 0.006) 23.54 ng/ul m

response 94035

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.50	67.27
41.00	36.20	39.02
42.00	24.50	26.61

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048547.D
 Acq On : 09 Nov 2024 02:49
 Operator : RC/JU
 Sample : PB164769TB
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLEB620

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 09 03:33:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 07 22:50:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	148240	20.000	ng/ul	0.00
20) Naphthalene-d8	10.451	136	572544	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.310	164	336934	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	683926	20.000	ng/ul	0.00
79) Chrysene-d12	21.280	240	675860	20.000	ng/ul	0.00
88) Perylene-d12	24.191	264	798778	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	22028	5.924	ng/uL	0.00
4) Pyridine-d5	3.546	84	306665	29.925	ng/ul	0.00
7) Phenol-d5	6.845	99	345494	30.616	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.998	67	208061	30.696	ng/ul	0.00
11) 2-Chlorophenol-d4	7.198	132	296889	31.761	ng/ul	0.00
15) 4-Methylphenol-d8	8.381	113	261946	29.521	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	130572	31.465	ng/ul	0.00
24) 2-Nitrophenol-d4	9.539	143	139919	31.700	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.080	165	235135	28.676	ng/ul	0.00
31) 4-Chloroaniline-d4	10.598	131	345496	29.664	ng/ul	0.00
46) Dimethylphthalate-d6	13.727	166	707597	32.899	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	829789	32.723	ng/ul	0.00
54) 4-Nitrophenol-d4	14.539	143	94035m	23.539	ng/ul	0.00
60) Fluorene-d10	15.310	176	623545	33.212	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.439	200	85373	24.814	ng/ul	0.00
73) Anthracene-d10	17.157	188	965528	33.361	ng/ul	0.00
81) Pyrene-d10	19.450	212	1178136	34.734	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.991	264	1276386	34.200	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048547.D
Acq On : 09 Nov 2024 02:49
Operator : RC/JU
Sample : PB164769TB
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLEB620

Manual IntegrationsAPPROVED

Quant Time: Nov 09 03:33:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 07 22:50:20 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/11/2024

