

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048550.D
 Acq On : 09 Nov 2024 04:48
 Operator : RC/JU
 Sample : P4636-17
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CC0R1

Quant Time: Nov 09 05:24:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 07 22:50:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	181868	20.000	ng/ul	0.00
20) Naphthalene-d8	10.445	136	721114	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.310	164	427544	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	872842	20.000	ng/ul	0.00
79) Chrysene-d12	21.280	240	848959	20.000	ng/ul	0.00
88) Perylene-d12	24.191	264	991543	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	14117	3.094	ng/uL	0.00
4) Pyridine-d5	3.546	84	145447	11.569	ng/ul	0.00
7) Phenol-d5	6.846	99	249162	17.997	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.998	67	153026	18.402	ng/ul	0.00
11) 2-Chlorophenol-d4	7.198	132	215145	18.760	ng/ul	0.00
15) 4-Methylphenol-d8	8.381	113	200766	18.443	ng/ul	0.00
21) Nitrobenzene-d5	8.816	128	100738	19.274	ng/ul	0.00
24) 2-Nitrophenol-d4	9.539	143	108435	19.505	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.081	165	196789	19.055	ng/ul	0.00
31) 4-Chloroaniline-d4	10.598	131	238562	16.263	ng/ul	0.00
46) Dimethylphthalate-d6	13.727	166	569152	20.854	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	678969	21.101	ng/ul	0.00
54) 4-Nitrophenol-d4	14.545	143	59312	11.701	ng/ul	0.01
60) Fluorene-d10	15.304	176	506774	21.272	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.439	200	61505	14.007	ng/ul	0.00
73) Anthracene-d10	17.157	188	752300	20.367	ng/ul	0.00
81) Pyrene-d10	19.451	212	924247	21.693	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.991	264	982657	21.211	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.192	149	35118	1.169	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048550.D
Acq On : 09 Nov 2024 04:48
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CC0R1

Quant Time: Nov 09 05:24:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 07 22:50:20 2024
Response via : Initial Calibration

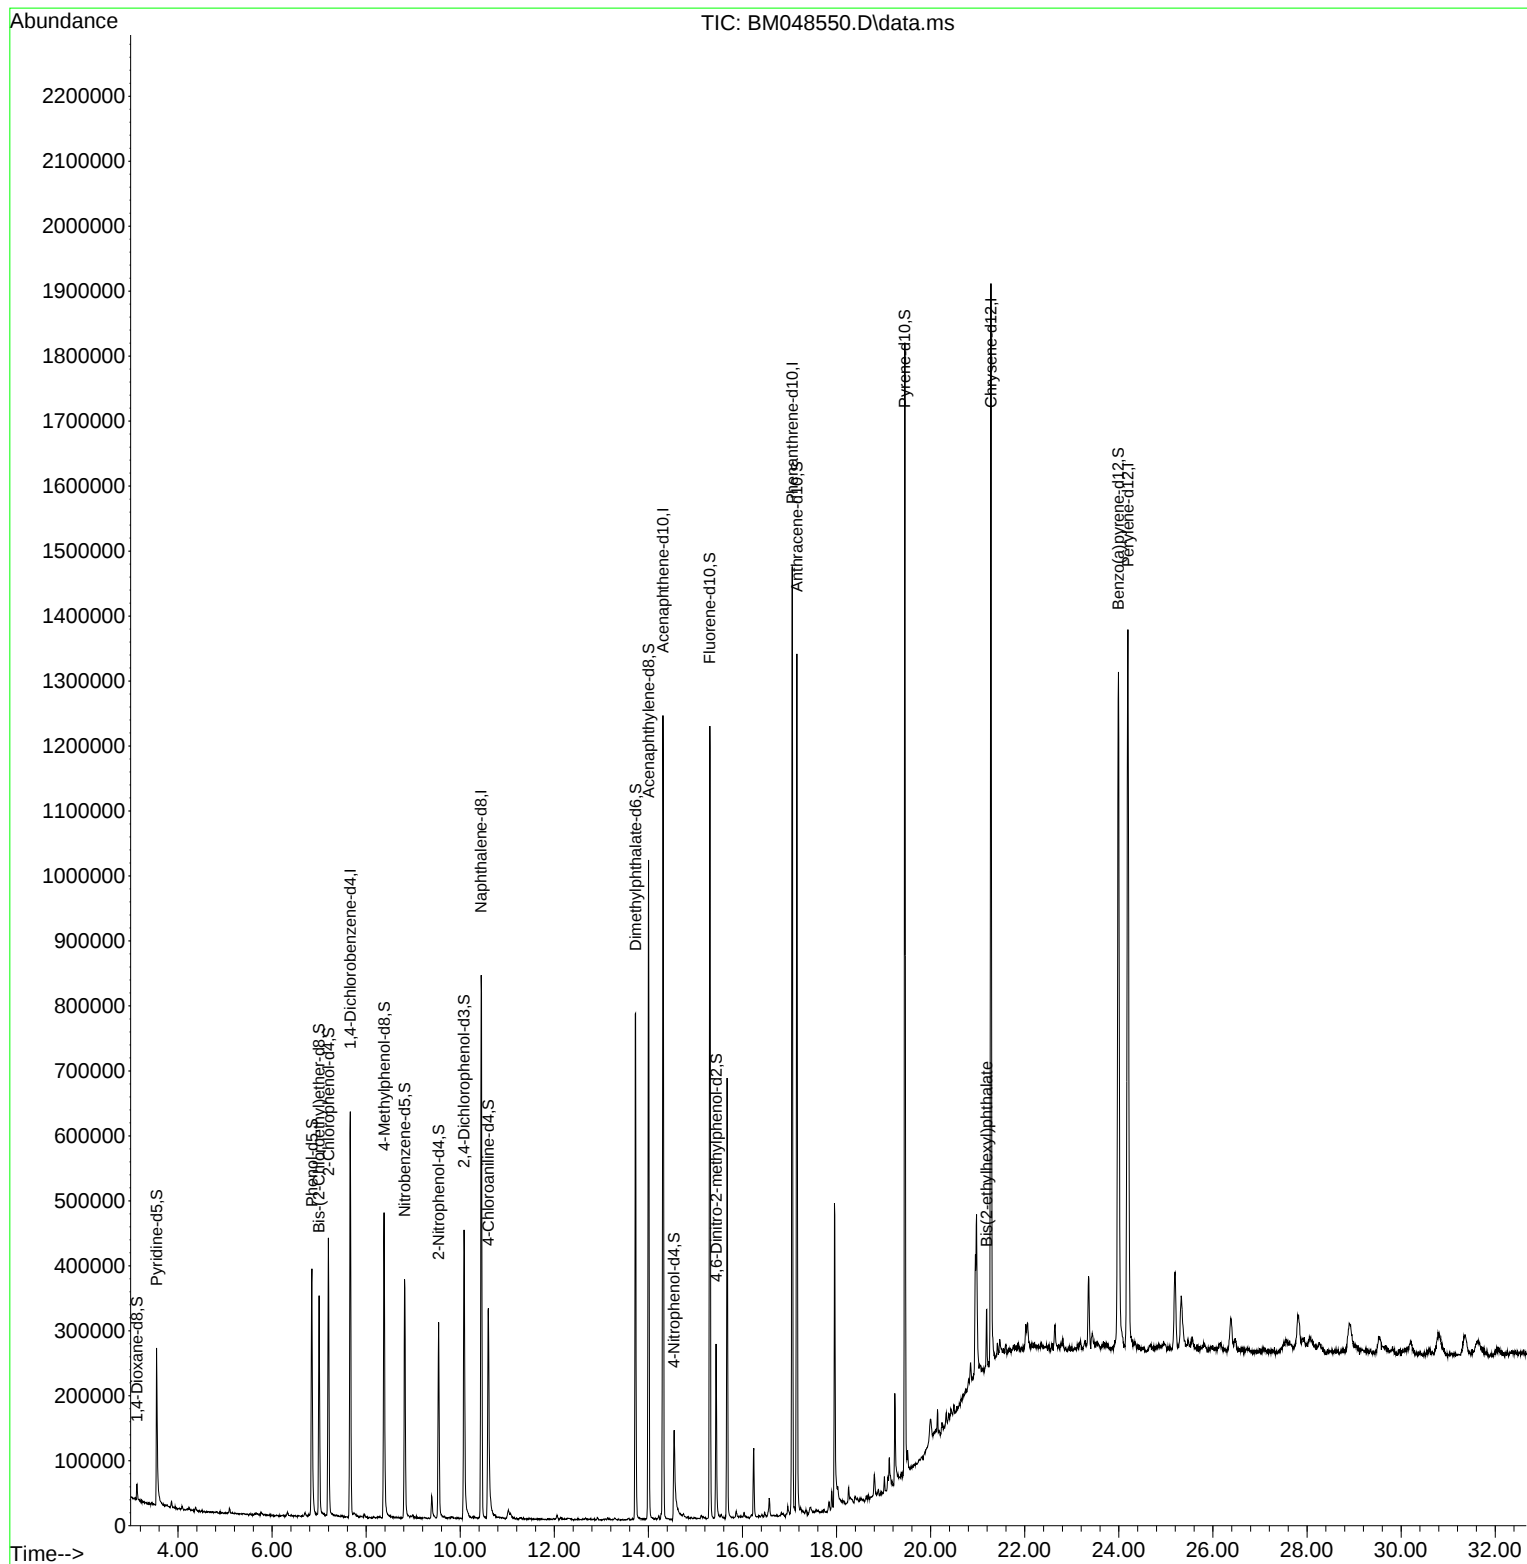

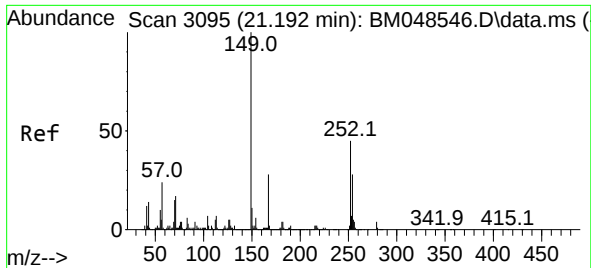

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.169 ng/ul
 RT: 21.192 min Scan# 3095
 Delta R.T. 0.000 min
 Lab File: BM048550.D
 Acq: 09 Nov 2024 04:48

Instrument :
 BNA_M
 ClientSampleId :
 CC0R1

Tgt Ion:149 Resp: 35118
 Ion Ratio Lower Upper
 149 100
 167 27.1 22.0 33.0
 279 4.0 3.1 4.7

