

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048521.D
 Acq On : 08 Nov 2024 08:59
 Operator : RC/JU
 Sample : PB164740BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK740

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	37	rVB	38644	59450	2.14%	0.222%
2	3.546	91	95	111	rBV	394975	681457	24.58%	2.549%
3	3.863	146	149	155	rVB3	8523	12799	0.46%	0.048%
4	6.846	648	656	670	rBV	434909	751376	27.10%	2.810%
5	7.004	677	683	698	rVB	367877	617870	22.28%	2.311%
6	7.198	709	716	729	rBV	474829	803138	28.96%	3.004%
7	7.663	786	795	809	rBV	365553	616971	22.25%	2.308%
8	8.381	910	917	929	rBV	522353	911144	32.86%	3.408%
9	8.822	985	992	1004	rBV	409731	705335	25.44%	2.638%
10	8.992	1019	1021	1024	rVB4	2545	3192	0.12%	0.012%
11	9.545	1107	1115	1125	rBV	316059	569328	20.53%	2.130%
12	9.645	1131	1132	1141	rVB7	2174	4538	0.16%	0.017%
13	10.086	1200	1207	1217	rBV	454710	837973	30.22%	3.134%
14	10.451	1260	1269	1278	rBV	509255	840145	30.30%	3.142%
15	10.598	1286	1294	1317	rBV	386411	892752	32.20%	3.339%
16	10.828	1330	1333	1337	rVB4	2263	3293	0.12%	0.012%
17	11.728	1482	1486	1492	rBV8	2739	5821	0.21%	0.022%
18	12.075	1538	1545	1550	rBV7	5140	12656	0.46%	0.047%
19	13.727	1820	1826	1842	rBV	816079	1234617	44.52%	4.618%
20	14.004	1867	1873	1887	rBV	1030655	1531429	55.23%	5.728%
21	14.310	1919	1925	1936	rBV	692235	1039021	37.47%	3.886%
22	14.545	1958	1965	1987	rBV	177980	493051	17.78%	1.844%
23	14.686	1987	1989	1994	rVB4	6070	8626	0.31%	0.032%
24	14.757	2000	2001	2008	rVB7	2691	3594	0.13%	0.013%
25	15.310	2088	2095	2110	rBV	1296935	1883106	67.91%	7.044%
26	15.445	2112	2118	2132	rVV	278810	481687	17.37%	1.802%
27	15.557	2134	2137	2142	rVV6	8515	14504	0.52%	0.054%
28	15.868	2186	2190	2196	rBV7	4273	7009	0.25%	0.026%
29	16.551	2303	2306	2312	rBV5	3108	5498	0.20%	0.021%
30	17.057	2386	2392	2402	rBV	845192	1198478	43.22%	4.483%
31	17.157	2403	2409	2422	rVV2	1380481	2055048	74.11%	7.687%
32	17.968	2542	2547	2549	rBV6	5216	8031	0.29%	0.030%
33	18.515	2637	2640	2642	rBV3	2508	2777	0.10%	0.010%
34	19.021	2721	2726	2734	rBV3	18140	33376	1.20%	0.125%
35	19.092	2734	2738	2743	rBV3	12631	22615	0.82%	0.085%
36	19.251	2762	2765	2766	rBV2	6289	6625	0.24%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048521.D
Acq On : 08 Nov 2024 08:59
Operator : RC/JU
Sample : PB164740BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK740

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	19.451	2794	2799	2812	rBV	1769808	2517118	90.77%	9.415%
38	20.950	3051	3054	3058	rBV2	40216	54487	1.96%	0.204%
39	21.286	3105	3111	3123	rBV	853451	1412429	50.94%	5.283%
40	23.997	3564	3572	3587	rVB	1204239	2772948	100.00%	10.372%
41	24.197	3598	3606	3621	rVB	614197	1619881	58.42%	6.059%




Sum of corrected areas: 26735193

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048521.D
Acq On : 08 Nov 2024 08:59
Operator : RC/JU
Sample : PB164740BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK740

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

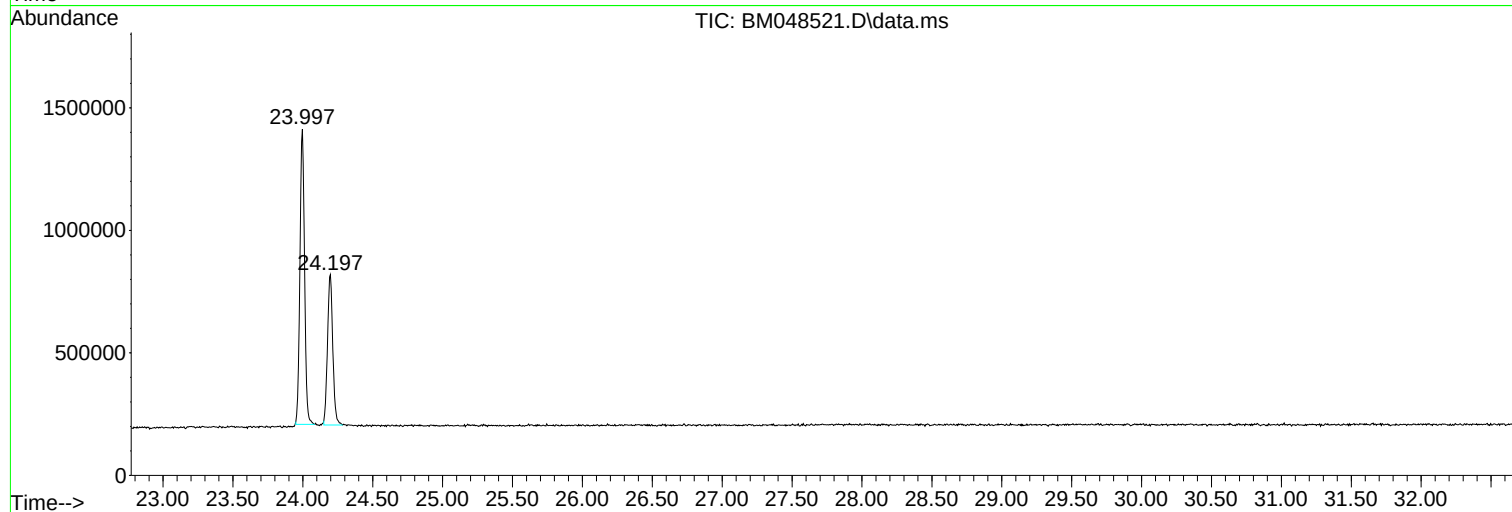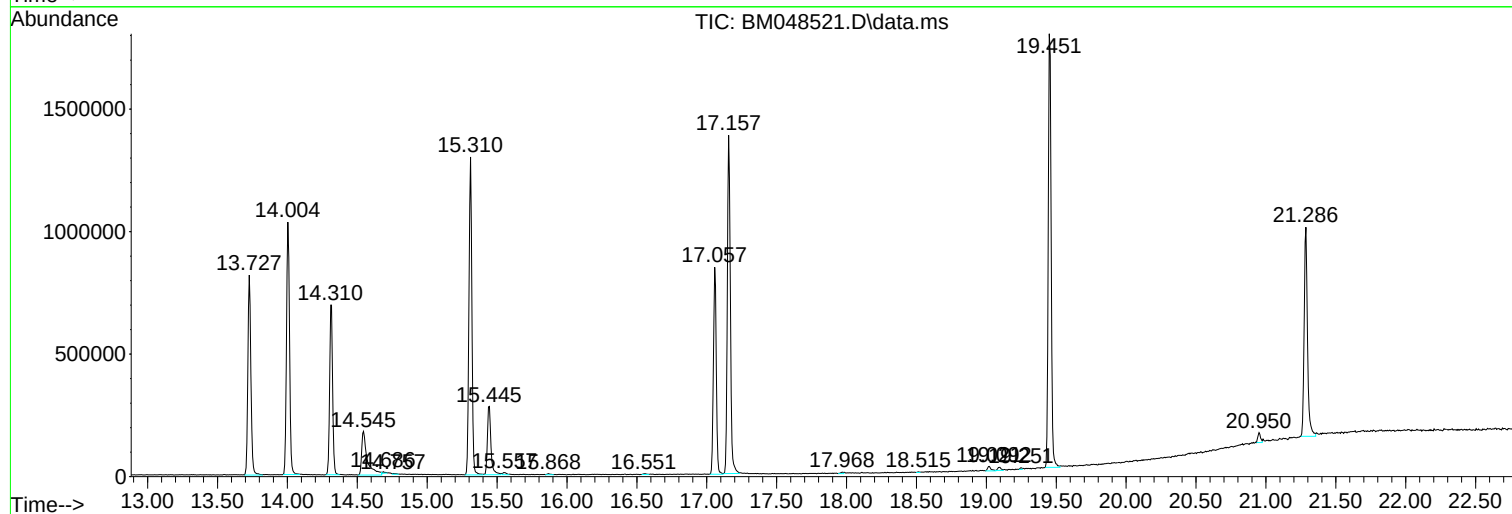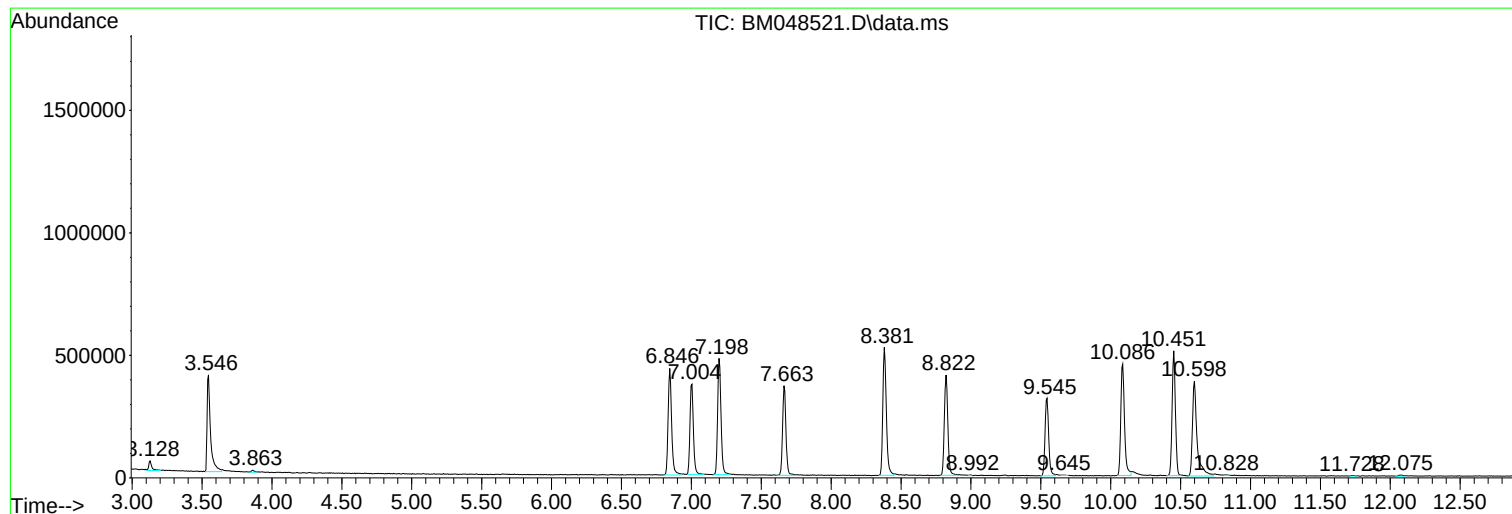

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048521.D
Acq On : 08 Nov 2024 08:59
Operator : RC/JU
Sample : PB164740BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK740

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048521.D
Acq On : 08 Nov 2024 08:59
Operator : RC/JU
Sample : PB164740BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK740

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc