

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048523.D
 Acq On : 08 Nov 2024 10:18
 Operator : RC/JU
 Sample : P4621-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	21	24	32	rVB2	39728	55749	1.60%	0.185%
2	3.558	94	97	109	rBV	81892	156929	4.49%	0.521%
3	3.863	146	149	155	rVB2	7437	9941	0.28%	0.033%
4	4.793	305	307	316	rVB3	12460	21196	0.61%	0.070%
5	6.322	564	567	568	rBV2	3703	3539	0.10%	0.012%
6	6.334	568	569	575	rVB5	6228	6712	0.19%	0.022%
7	6.846	651	656	672	rVB	188231	340046	9.74%	1.130%
8	7.004	676	683	692	rBV	445323	740370	21.21%	2.459%
9	7.198	708	716	727	rBV	531867	916217	26.24%	3.043%
10	7.487	762	765	771	rVB7	2501	5121	0.15%	0.017%
11	7.663	789	795	806	rBV	374813	638027	18.27%	2.119%
12	8.381	910	917	931	rBV	508096	880201	25.21%	2.924%
13	8.492	934	936	942	rVB5	4603	6547	0.19%	0.022%
14	8.822	984	992	1010	rBV	502375	867320	24.84%	2.881%
15	9.245	1060	1064	1067	rBV5	4165	6055	0.17%	0.020%
16	9.545	1107	1115	1125	rBV	397527	702965	20.13%	2.335%
17	10.081	1198	1206	1230	rBV	558153	1118495	32.04%	3.715%
18	10.451	1262	1269	1284	rVB	530623	892561	25.57%	2.965%
19	10.598	1284	1294	1315	rBV	395692	868474	24.88%	2.885%
20	11.016	1363	1365	1370	rVB6	2707	4185	0.12%	0.014%
21	11.081	1373	1376	1379	rBV4	3061	5014	0.14%	0.017%
22	11.739	1482	1488	1493	rVB5	4823	8537	0.24%	0.028%
23	12.016	1530	1535	1536	rBV3	2392	3751	0.11%	0.012%
24	12.069	1539	1544	1550	rVB4	6412	13499	0.39%	0.045%
25	12.363	1591	1594	1600	rVB4	2726	3687	0.11%	0.012%
26	12.663	1640	1645	1650	rVB6	2210	4829	0.14%	0.016%
27	12.922	1685	1689	1693	rBV7	3632	6448	0.18%	0.021%
28	13.216	1735	1739	1743	rBV4	4732	6293	0.18%	0.021%
29	13.292	1747	1752	1757	rBV5	2284	5741	0.16%	0.019%
30	13.639	1806	1811	1816	rVB7	3734	4966	0.14%	0.016%
31	13.727	1820	1826	1831	rVV	1086959	1511321	43.29%	5.020%
32	13.774	1831	1834	1841	rVB	129910	185664	5.32%	0.617%
33	14.004	1864	1873	1884	rBV	1236634	1839942	52.70%	6.112%
34	14.316	1919	1926	1934	rBV	730137	1105700	31.67%	3.673%
35	14.557	1959	1967	1974	rBV2	53443	130356	3.73%	0.433%
36	14.763	1998	2002	2006	rBV5	5051	9535	0.27%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048523.D
Acq On : 08 Nov 2024 10:18
Operator : RC/JU
Sample : P4621-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	14.792	2006	2007	2012	rVB5	4403	4382	0.13%	0.015%
38	15.310	2088	2095	2101	rBV	1590833	2293625	65.70%	7.619%
39	15.363	2101	2104	2110	rVV6	14111	28769	0.82%	0.096%
40	15.439	2111	2117	2133	rVV	419462	645601	18.49%	2.144%
41	15.545	2133	2135	2141	rVB4	8349	12388	0.35%	0.041%
42	15.868	2184	2190	2196	rBV8	4135	8853	0.25%	0.029%
43	16.557	2299	2307	2313	rBV9	3961	10774	0.31%	0.036%
44	17.057	2386	2392	2403	rVV	899771	1276557	36.56%	4.240%
45	17.157	2403	2409	2426	rVV	1775741	2617755	74.98%	8.695%
46	17.962	2540	2546	2551	rBV8	11842	23438	0.67%	0.078%
47	18.027	2555	2557	2562	rVB5	3665	4055	0.12%	0.013%
48	19.015	2722	2725	2732	rVB2	23044	34075	0.98%	0.113%
49	19.092	2733	2738	2742	rBV2	24619	38680	1.11%	0.128%
50	19.245	2761	2764	2768	rBV4	10746	15352	0.44%	0.051%
51	19.451	2793	2799	2811	rBV	2291543	3232062	92.57%	10.736%
52	21.286	3105	3111	3123	rBV	946318	1531032	43.85%	5.086%
53	23.991	3563	3571	3585	rBV	1457138	3491294	100.00%	11.597%
54	24.191	3598	3605	3627	rVB	674630	1751155	50.16%	5.817%




Sum of corrected areas: 30105780

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048523.D
Acq On : 08 Nov 2024 10:18
Operator : RC/JU
Sample : P4621-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6M7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

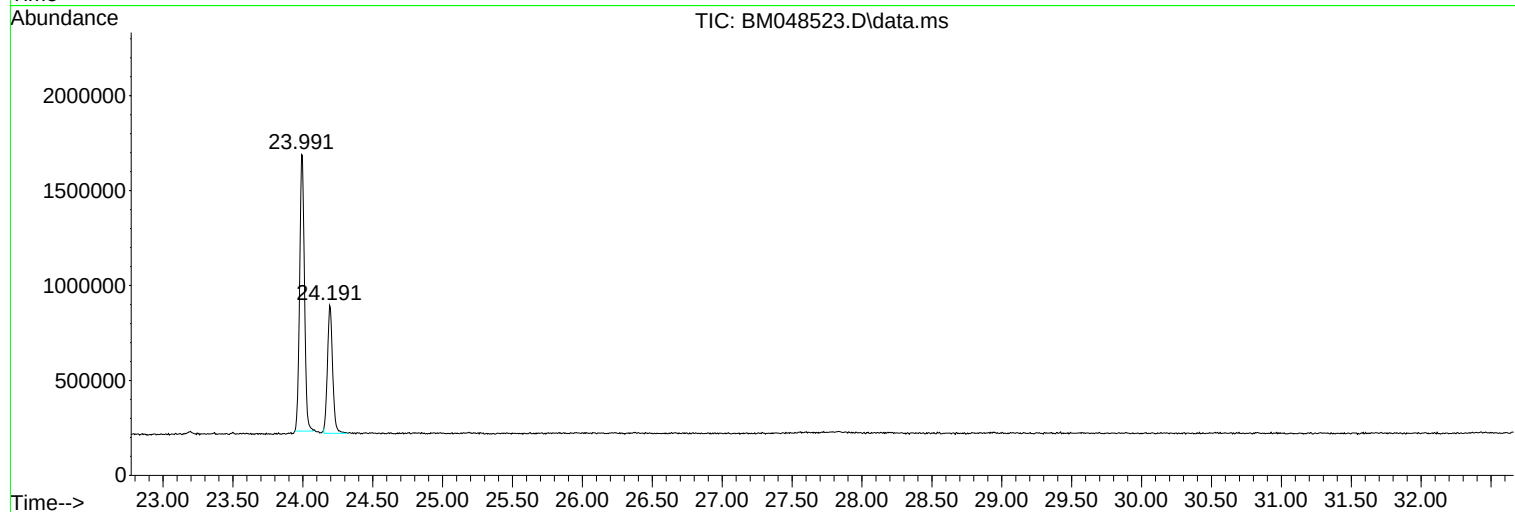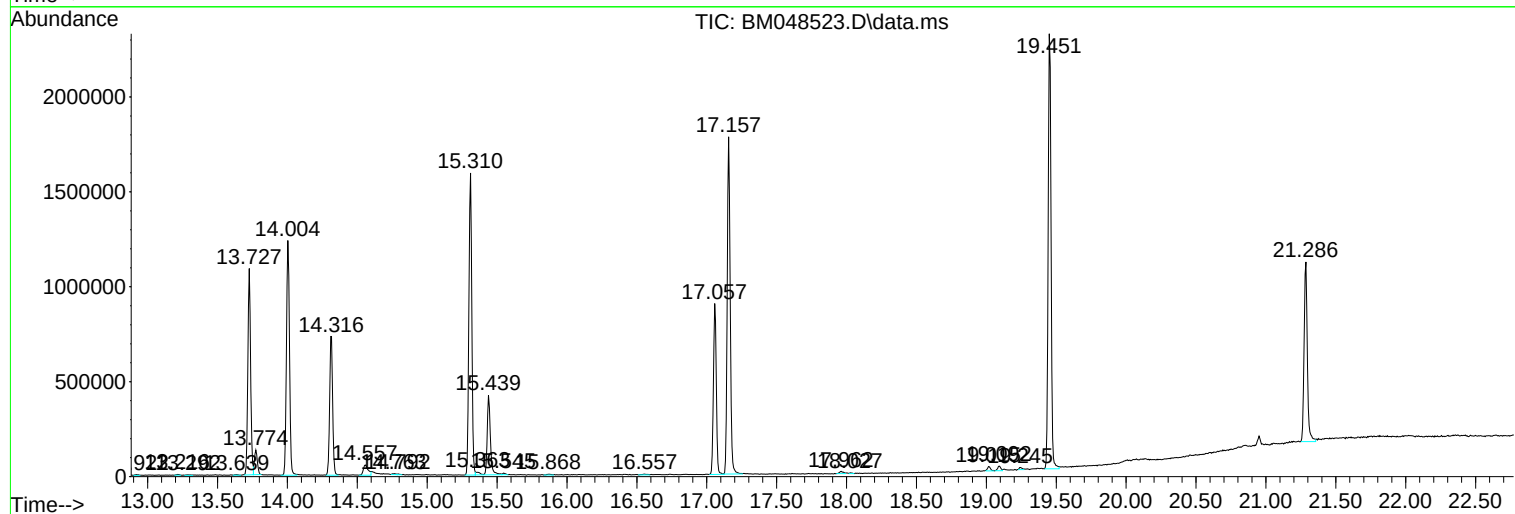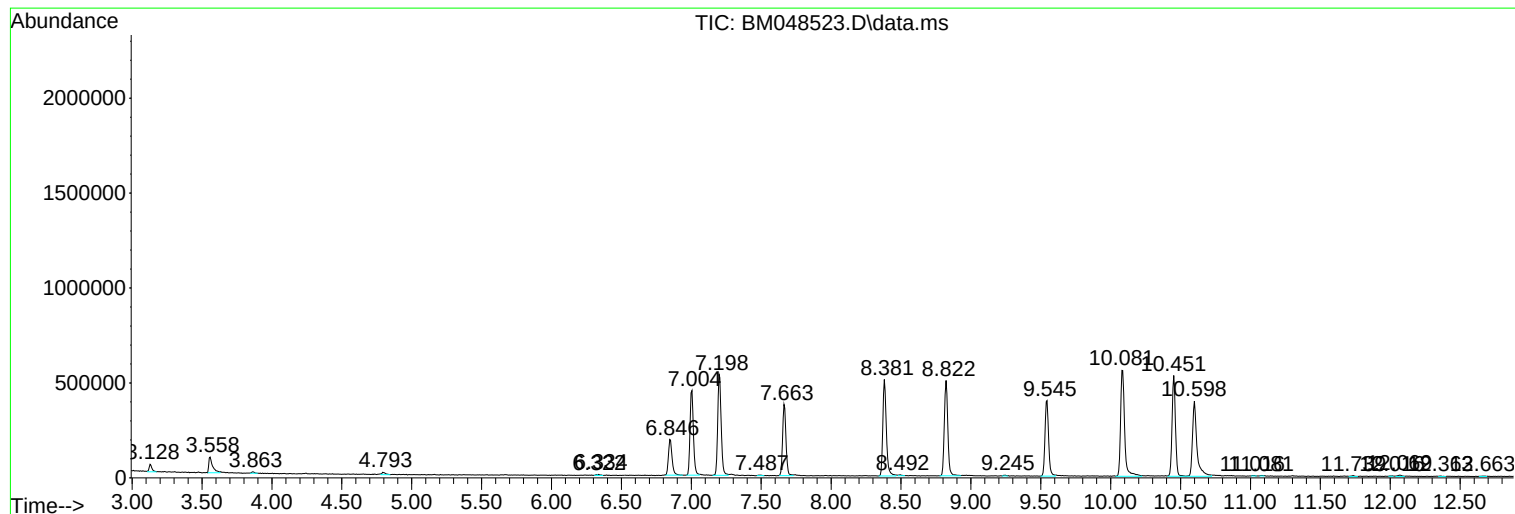

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048523.D
Acq On : 08 Nov 2024 10:18
Operator : RC/JU
Sample : P4621-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6M7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048523.D
Acq On : 08 Nov 2024 10:18
Operator : RC/JU
Sample : P4621-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6M7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc