

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048524.D
 Acq On : 08 Nov 2024 10:58
 Operator : RC/JU
 Sample : P4621-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	21	24	32	rVB	39095	54234	1.51%	0.187%
2	3.552	93	96	111	rBV	90294	175849	4.91%	0.606%
3	3.863	147	149	154	rVB5	7381	10322	0.29%	0.036%
4	4.799	302	308	313	rBV3	8854	17216	0.48%	0.059%
5	4.963	331	336	343	rBV6	5005	11137	0.31%	0.038%
6	6.846	651	656	670	rVB	171273	315080	8.79%	1.087%
7	6.998	676	682	699	rBV	443726	755041	21.07%	2.604%
8	7.198	710	716	728	rBV	546864	896531	25.02%	3.092%
9	7.663	789	795	804	rBV	387156	626518	17.48%	2.161%
10	8.381	909	917	928	rBV	474759	827082	23.08%	2.852%
11	8.822	982	992	1006	rBV	511327	858674	23.96%	2.961%
12	8.981	1017	1019	1028	rVB5	2959	5188	0.14%	0.018%
13	9.240	1060	1063	1067	rBV4	4486	5969	0.17%	0.021%
14	9.540	1107	1114	1128	rBV	397550	701189	19.56%	2.418%
15	10.087	1197	1207	1234	rBV	489708	1093490	30.51%	3.771%
16	10.451	1262	1269	1278	rBV	517316	849888	23.71%	2.931%
17	10.628	1292	1299	1314	rBV6	12765	46545	1.30%	0.161%
18	11.310	1410	1415	1422	rBV7	4626	9962	0.28%	0.034%
19	11.733	1483	1487	1491	rBV5	3174	4818	0.13%	0.017%
20	12.063	1537	1543	1552	rVB4	6036	12356	0.34%	0.043%
21	13.727	1820	1826	1831	rBV	1077607	1507010	42.05%	5.197%
22	13.775	1831	1834	1841	rVB	57916	89128	2.49%	0.307%
23	14.004	1866	1873	1884	rBV	1175213	1737948	48.49%	5.993%
24	14.316	1920	1926	1934	rBV	693145	1048377	29.25%	3.615%
25	14.557	1959	1967	1985	rBV2	56048	174674	4.87%	0.602%
26	15.310	2088	2095	2102	rBV	1564627	2327801	64.95%	8.027%
27	15.363	2102	2104	2111	rVV4	20649	32347	0.90%	0.112%
28	15.439	2111	2117	2131	rVV	433377	685343	19.12%	2.363%
29	15.551	2133	2136	2140	rVB5	9466	13243	0.37%	0.046%
30	15.745	2164	2169	2173	rVB6	2557	4340	0.12%	0.015%
31	15.869	2185	2190	2197	rBV9	4941	10586	0.30%	0.037%
32	16.739	2332	2338	2340	rBV5	2743	5218	0.15%	0.018%
33	16.851	2355	2357	2361	rVB5	3105	3642	0.10%	0.013%
34	17.057	2386	2392	2403	rBV	854491	1231227	34.35%	4.246%
35	17.157	2403	2409	2427	rVV2	1795711	2623924	73.21%	9.049%
36	17.962	2541	2546	2552	rBV8	13787	25925	0.72%	0.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048524.D
Acq On : 08 Nov 2024 10:58
Operator : RC/JU
Sample : P4621-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6M8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	19.021	2721	2726	2733	rBV2	23946	34390	0.96%	0.119%
38	19.092	2733	2738	2742	rBV2	21775	35698	1.00%	0.123%
39	19.245	2760	2764	2769	rBV5	16720	26991	0.75%	0.093%
40	19.451	2793	2799	2812	rBV	2321751	3285112	91.66%	11.329%
41	20.951	3051	3054	3060	rBV2	35707	52680	1.47%	0.182%
42	21.286	3105	3111	3122	rBV	936253	1488422	41.53%	5.133%
43	23.997	3563	3572	3587	rBV	1463616	3583913	100.00%	12.359%
44	24.197	3598	3606	3625	rVB	643744	1693112	47.24%	5.839%




Sum of corrected areas: 28998140

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048524.D
Acq On : 08 Nov 2024 10:58
Operator : RC/JU
Sample : P4621-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6M8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

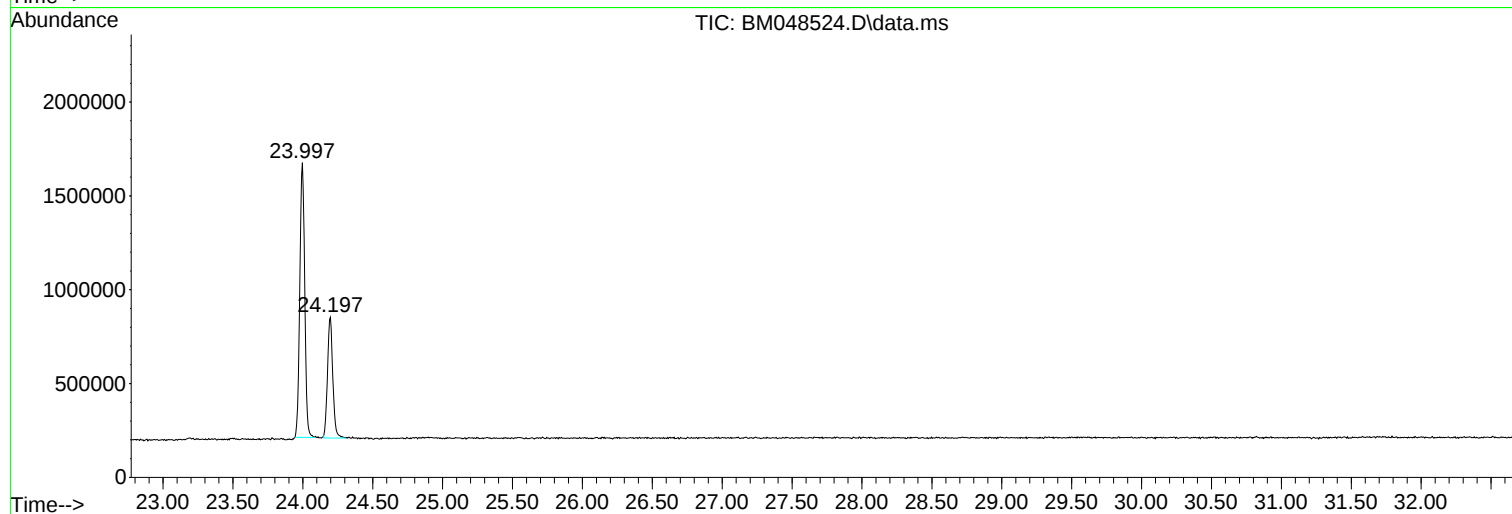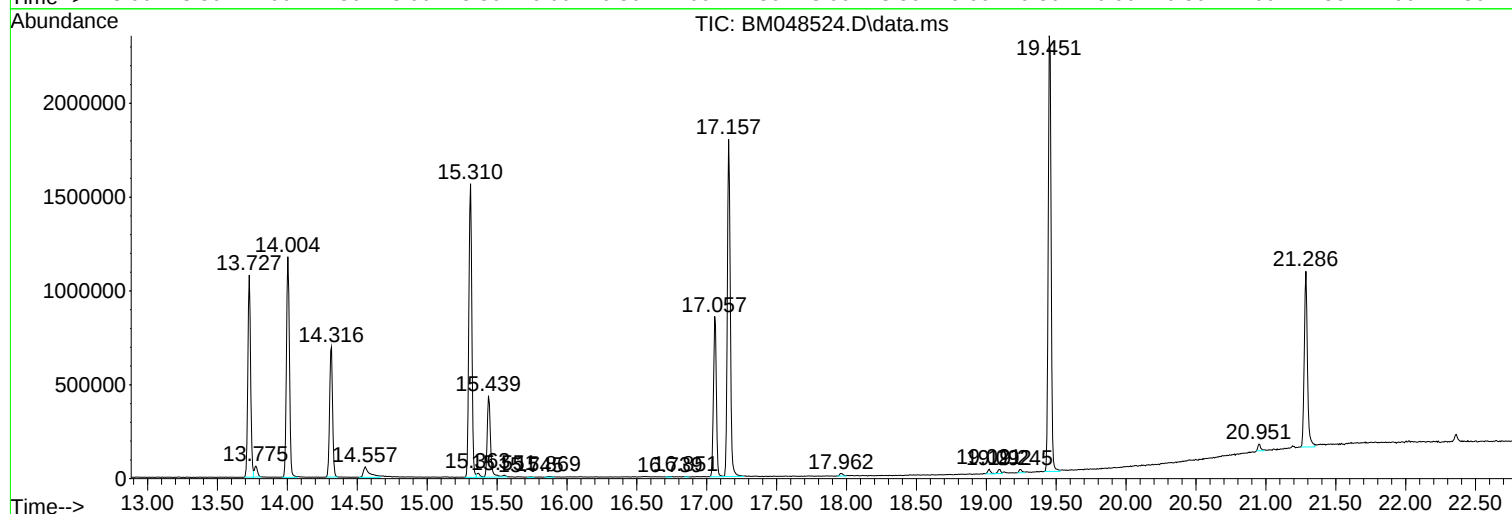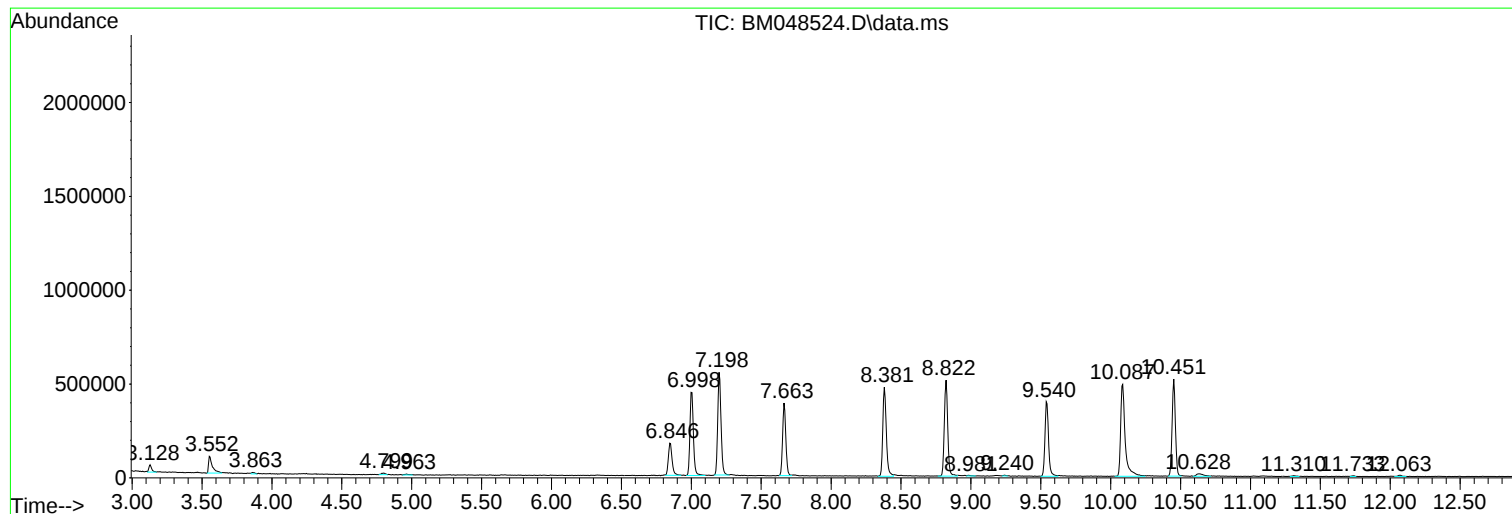

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048524.D
Acq On : 08 Nov 2024 10:58
Operator : RC/JU
Sample : P4621-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6M8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048524.D
Acq On : 08 Nov 2024 10:58
Operator : RC/JU
Sample : P4621-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6M8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc