

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048526.D
 Acq On : 08 Nov 2024 12:16
 Operator : RC/JU
 Sample : P4621-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	34	rVB	38072	57247	1.62%	0.191%
2	3.552	93	96	107	rBV	105074	190921	5.41%	0.637%
3	4.799	303	308	313	rVB3	10191	17014	0.48%	0.057%
4	4.963	333	336	342	rVB6	4850	6677	0.19%	0.022%
5	6.646	616	622	623	rBV6	3032	4077	0.12%	0.014%
6	6.846	647	656	667	rBV	170643	316758	8.98%	1.058%
7	6.999	676	682	695	rBV	445175	734817	20.83%	2.453%
8	7.199	710	716	728	rBV	537373	891433	25.27%	2.976%
9	7.493	763	766	767	rBV3	3253	3551	0.10%	0.012%
10	7.663	786	795	806	rBV	419811	695108	19.71%	2.321%
11	7.740	806	808	814	rVB6	4564	5953	0.17%	0.020%
12	8.381	909	917	933	rBV	479999	851307	24.13%	2.842%
13	8.487	933	935	943	rVB4	5207	11703	0.33%	0.039%
14	8.822	985	992	1006	rBV	506262	861368	24.42%	2.876%
15	9.240	1060	1063	1070	rVB6	4020	6171	0.17%	0.021%
16	9.540	1108	1114	1127	rBV	402577	704300	19.97%	2.352%
17	10.081	1200	1206	1231	rVV	503280	1109311	31.45%	3.704%
18	10.451	1262	1269	1285	rVB	570823	958198	27.16%	3.199%
19	10.628	1293	1299	1312	rBV3	17245	57198	1.62%	0.191%
20	10.940	1348	1352	1356	rVB6	1983	3547	0.10%	0.012%
21	11.028	1361	1367	1371	rBV7	3460	6986	0.20%	0.023%
22	11.081	1373	1376	1381	rVV4	3451	5647	0.16%	0.019%
23	11.304	1410	1414	1417	rBV5	3804	7003	0.20%	0.023%
24	11.734	1483	1487	1492	rBV5	3593	5503	0.16%	0.018%
25	12.069	1537	1544	1549	rBV5	6172	12489	0.35%	0.042%
26	12.775	1661	1664	1669	rBV4	1880	3951	0.11%	0.013%
27	12.922	1685	1689	1693	rBV4	2835	4126	0.12%	0.014%
28	13.222	1734	1740	1744	rBV4	3316	6886	0.20%	0.023%
29	13.728	1820	1826	1831	rBV	1121524	1584066	44.91%	5.289%
30	13.775	1831	1834	1840	rVB	66114	99221	2.81%	0.331%
31	14.004	1867	1873	1889	rBV	1247655	1839685	52.15%	6.142%
32	14.310	1919	1925	1935	rVV	795047	1192851	33.82%	3.983%
33	14.557	1960	1967	1981	rBV2	51059	152144	4.31%	0.508%
34	15.128	2059	2064	2068	rBV5	1869	3646	0.10%	0.012%
35	15.310	2088	2095	2101	rBV	1654574	2417390	68.53%	8.071%
36	15.363	2101	2104	2111	rVV3	24880	43067	1.22%	0.144%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048526.D
 Acq On : 08 Nov 2024 12:16
 Operator : RC/JU
 Sample : P4621-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	15.439	2111	2117	2132	rVV	447765	692522	19.63%	2.312%
38	15.545	2132	2135	2140	rVB5	7348	12977	0.37%	0.043%
39	15.869	2186	2190	2191	rBV3	3376	3549	0.10%	0.012%
40	16.551	2301	2306	2309	rBV6	4254	5213	0.15%	0.017%
41	16.745	2333	2339	2342	rBV6	3121	6788	0.19%	0.023%
42	17.057	2386	2392	2402	rBV	960595	1361365	38.59%	4.545%
43	17.157	2402	2409	2426	rVV	1861103	2705841	76.71%	9.034%
44	17.622	2483	2488	2492	rBV7	2174	3785	0.11%	0.013%
45	17.963	2540	2546	2551	rBV7	8736	18449	0.52%	0.062%
46	18.716	2672	2674	2677	rBV3	3431	4481	0.13%	0.015%
47	19.016	2720	2725	2733	rBV4	23605	40723	1.15%	0.136%
48	19.092	2734	2738	2742	rVV	21809	29695	0.84%	0.099%
49	19.245	2762	2764	2768	rVB4	8875	9655	0.27%	0.032%
50	19.451	2793	2799	2811	rBV	2298268	3299048	93.52%	11.015%
51	20.951	3051	3054	3062	rBV2	29886	44899	1.27%	0.150%
52	21.286	3105	3111	3120	rBV	991537	1561236	44.26%	5.213%
53	23.998	3563	3572	3592	rVB	1421935	3527472	100.00%	11.778%
54	24.192	3598	3605	3619	rVB	686684	1751858	49.66%	5.849%




Sum of corrected areas: 29950876

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048526.D
Acq On : 08 Nov 2024 12:16
Operator : RC/JU
Sample : P4621-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

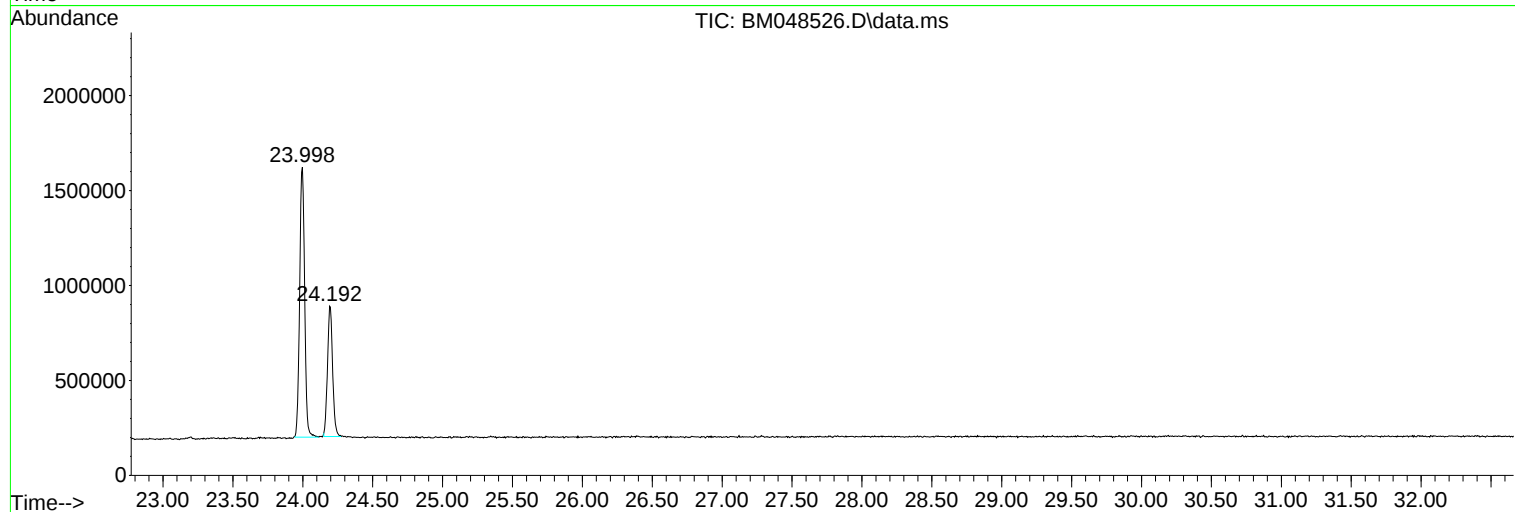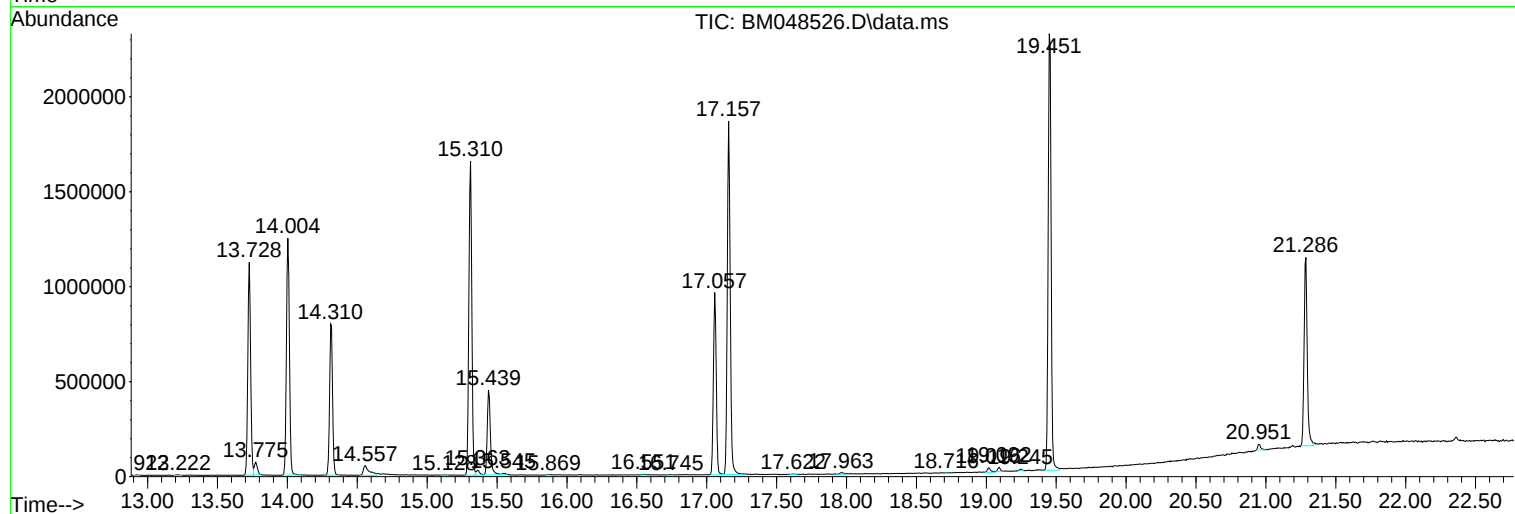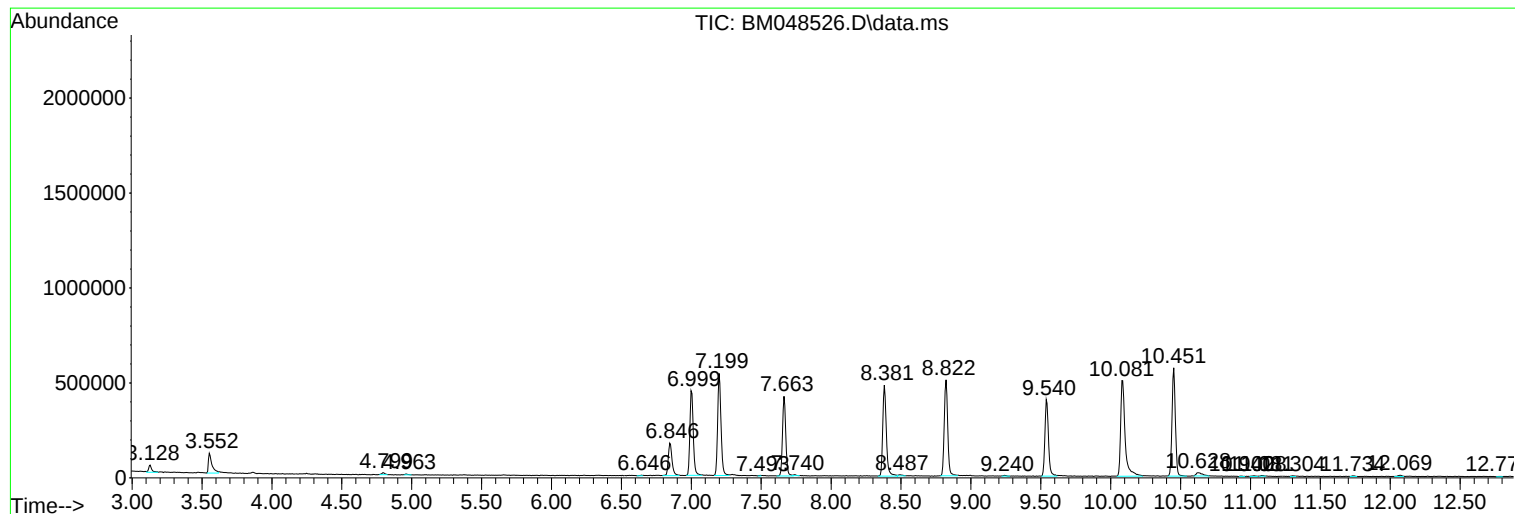

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048526.D
Acq On : 08 Nov 2024 12:16
Operator : RC/JU
Sample : P4621-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048526.D
Acq On : 08 Nov 2024 12:16
Operator : RC/JU
Sample : P4621-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc