

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048534.D
 Acq On : 08 Nov 2024 17:35
 Operator : RC/JU
 Sample : PB164804BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK804

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	33	rVB	39352	59836	1.90%	0.183%
2	3.546	91	95	109	rBV	429404	720666	22.92%	2.201%
3	3.857	146	148	156	rVB4	8816	15228	0.48%	0.047%
4	4.857	316	318	322	rBV4	2201	3204	0.10%	0.010%
5	6.846	648	656	671	rBV	494532	827149	26.30%	2.526%
6	6.998	676	682	693	rBV	414119	666106	21.18%	2.034%
7	7.198	709	716	730	rBV	533906	875624	27.84%	2.674%
8	7.663	788	795	805	rBV	546000	883192	28.09%	2.697%
9	8.381	910	917	934	rBV	590600	1037160	32.98%	3.167%
10	8.822	985	992	1007	rBV	452781	795648	25.30%	2.430%
11	9.539	1108	1114	1129	rBV	362342	640496	20.37%	1.956%
12	10.081	1199	1206	1230	rBV	522441	1008950	32.08%	3.081%
13	10.451	1261	1269	1283	rVB	735159	1208738	38.44%	3.691%
14	10.598	1287	1294	1314	rBV	461772	1033708	32.87%	3.157%
15	12.069	1537	1544	1550	rBV5	8798	17896	0.57%	0.055%
16	13.727	1819	1826	1838	rBV	931902	1369381	43.55%	4.182%
17	14.004	1865	1873	1884	rBV	1189982	1774366	56.42%	5.418%
18	14.310	1918	1925	1934	rBV	1057985	1541105	49.01%	4.706%
19	14.539	1958	1964	1986	rBV	213159	569934	18.12%	1.740%
20	15.310	2088	2095	2107	rBV	1476475	2142497	68.13%	6.543%
21	15.439	2111	2117	2131	rVV	349994	542289	17.24%	1.656%
22	15.551	2131	2136	2142	rVB5	8288	14444	0.46%	0.044%
23	15.868	2184	2190	2198	rBV6	5986	12431	0.40%	0.038%
24	16.545	2302	2305	2309	rBV5	3430	5108	0.16%	0.016%
25	16.851	2353	2357	2359	rBV4	3560	5174	0.16%	0.016%
26	17.057	2386	2392	2402	rVV	1284066	1793536	57.03%	5.477%
27	17.157	2402	2409	2423	rVV	1621041	2359761	75.04%	7.206%
28	17.962	2542	2546	2547	rBV4	3693	4108	0.13%	0.013%
29	18.457	2627	2630	2631	rBV2	2587	3225	0.10%	0.010%
30	18.633	2658	2660	2663	rBV4	2893	4353	0.14%	0.013%
31	18.786	2684	2686	2689	rBV3	2600	3166	0.10%	0.010%
32	19.015	2721	2725	2731	rBV5	20035	33249	1.06%	0.102%
33	19.092	2734	2738	2747	rVV2	19923	31475	1.00%	0.096%
34	19.451	2793	2799	2814	rBV	2060774	2926933	93.08%	8.938%
35	20.950	3051	3054	3061	rBV	92084	119494	3.80%	0.365%
36	21.286	3105	3111	3122	rBV	1349326	2123317	67.52%	6.484%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048534.D
Acq On : 08 Nov 2024 17:35
Operator : RC/JU
Sample : PB164804BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK804

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	23.997	3563	3572	3584	rBV	1302058	3144697	100.00%	9.603%
38	24.197	3598	3606	3618	rVB	969136	2429364	77.25%	7.419%




Sum of corrected areas: 32747008

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048534.D
Acq On : 08 Nov 2024 17:35
Operator : RC/JU
Sample : PB164804BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK804

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

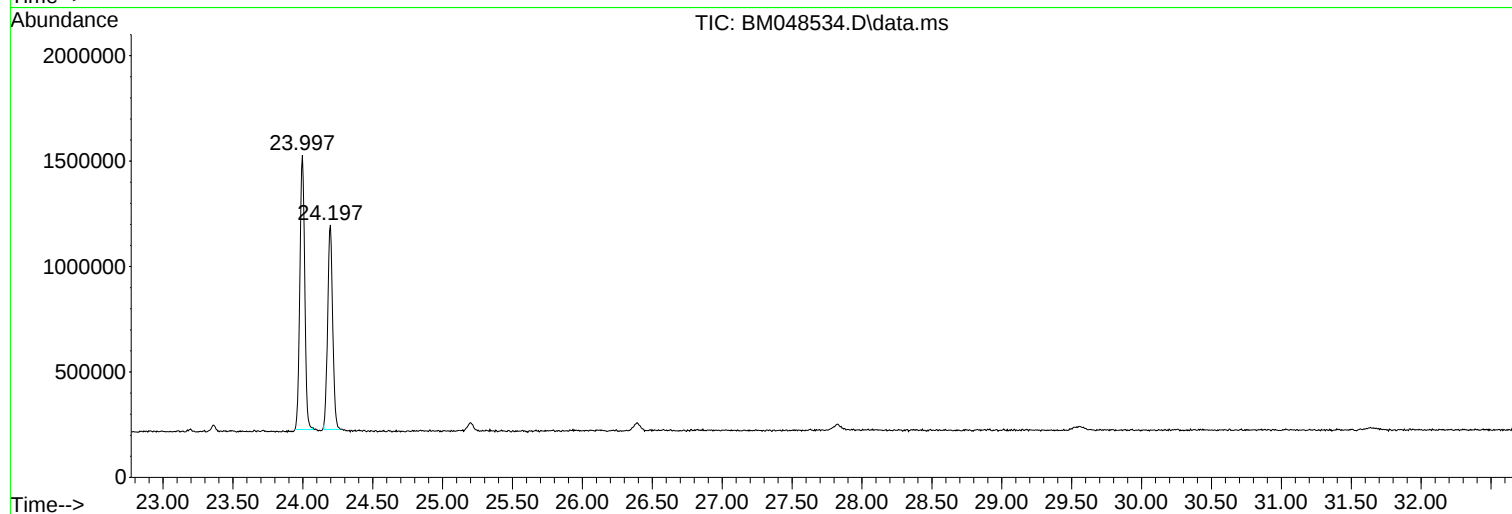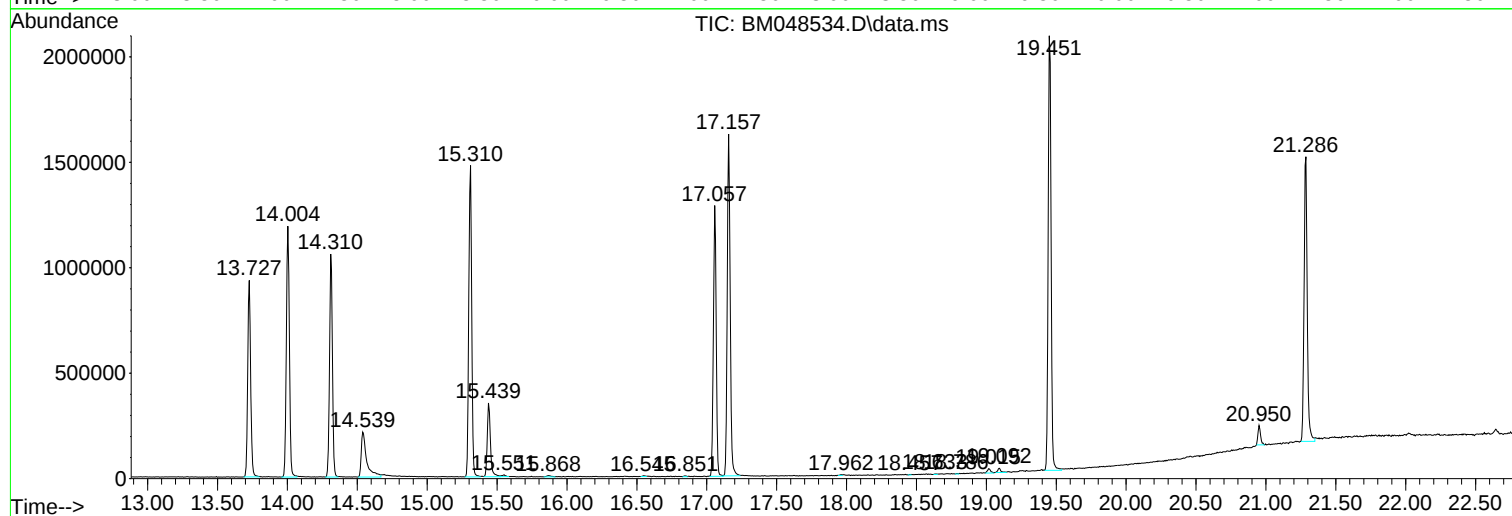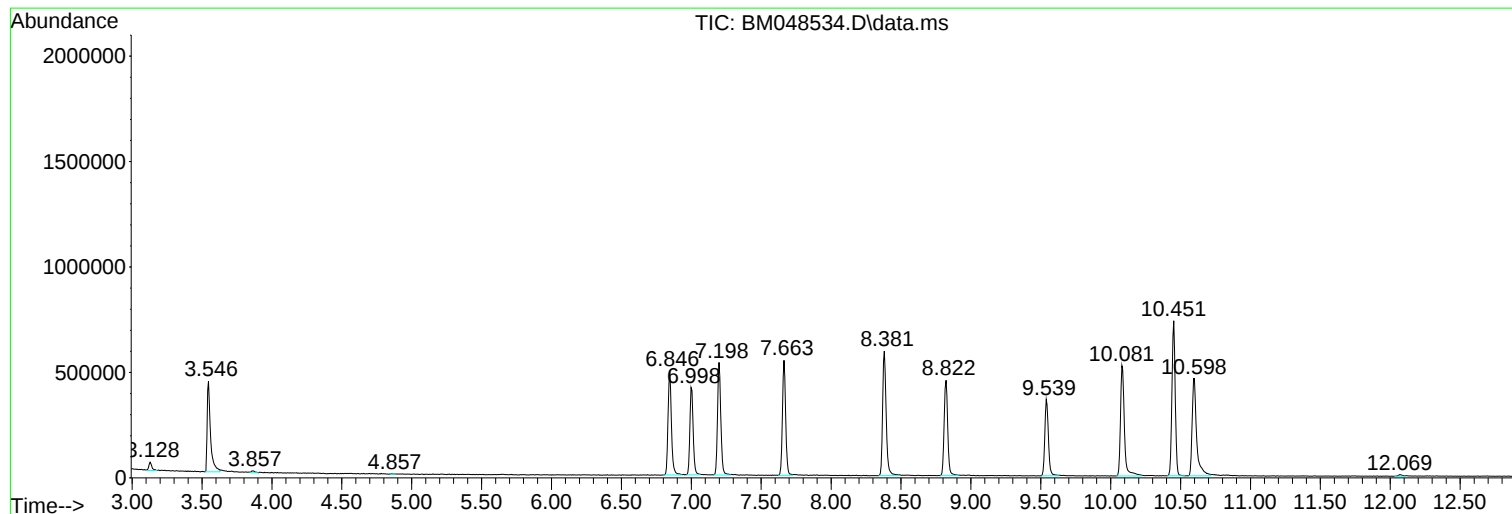

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048534.D
Acq On : 08 Nov 2024 17:35
Operator : RC/JU
Sample : PB164804BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK804

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048534.D
Acq On : 08 Nov 2024 17:35
Operator : RC/JU
Sample : PB164804BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK804

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc