

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048536.D
 Acq On : 08 Nov 2024 18:54
 Operator : RC/JU
 Sample : PB164769BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK769

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	31	rVB	35487	49228	1.72%	0.175%
2	3.546	91	95	114	rBV	404572	677178	23.65%	2.403%
3	3.863	147	149	153	rVB4	7770	8388	0.29%	0.030%
4	6.528	597	602	605	rBV5	3080	4358	0.15%	0.015%
5	6.845	649	656	671	rBV	444117	769329	26.87%	2.731%
6	6.998	675	682	693	rBV	373159	619610	21.64%	2.199%
7	7.198	710	716	727	rBV	495143	816322	28.52%	2.897%
8	7.498	761	767	769	rBV6	1796	3545	0.12%	0.013%
9	7.663	788	795	803	rVV	381175	616867	21.55%	2.189%
10	7.716	803	804	811	rVB6	3773	5184	0.18%	0.018%
11	8.380	910	917	934	rBV	562890	971778	33.95%	3.449%
12	8.822	984	992	1004	rBV	422067	733490	25.62%	2.603%
13	9.233	1059	1062	1066	rBV5	2705	4201	0.15%	0.015%
14	9.539	1107	1114	1126	rBV	358874	633450	22.13%	2.248%
15	10.080	1200	1206	1218	rBV	495548	925262	32.32%	3.284%
16	10.369	1252	1255	1261	rBV6	2477	4004	0.14%	0.014%
17	10.451	1261	1269	1280	rBV	526402	886944	30.98%	3.148%
18	10.598	1287	1294	1315	rBV	428005	947778	33.11%	3.364%
19	10.822	1329	1332	1335	rBV4	1810	3444	0.12%	0.012%
20	11.739	1483	1488	1492	rVB5	2796	4753	0.17%	0.017%
21	12.068	1540	1544	1547	rBV5	6000	9723	0.34%	0.035%
22	13.727	1819	1826	1840	rBV	862251	1295618	45.26%	4.598%
23	14.004	1866	1873	1884	rBV	1134339	1659462	57.97%	5.890%
24	14.080	1884	1886	1890	rVB5	3244	3576	0.12%	0.013%
25	14.310	1918	1925	1937	rBV	766687	1104236	38.57%	3.919%
26	14.545	1959	1965	1986	rBV	191316	514562	17.97%	1.826%
27	14.715	1993	1994	2001	rVB7	4453	6608	0.23%	0.023%
28	15.309	2088	2095	2105	rBV	1345564	1996103	69.73%	7.085%
29	15.439	2111	2117	2130	rBV	311182	493135	17.23%	1.750%
30	15.551	2133	2136	2140	rVV5	8383	12882	0.45%	0.046%
31	15.598	2142	2144	2148	rVB3	2552	3066	0.11%	0.011%
32	15.874	2186	2191	2195	rBV7	5980	11191	0.39%	0.040%
33	16.409	2280	2282	2285	rBV4	2785	3762	0.13%	0.013%
34	16.551	2302	2306	2308	rBV3	4843	5916	0.21%	0.021%
35	17.056	2386	2392	2403	rBV	914890	1280807	44.74%	4.546%
36	17.156	2403	2409	2423	rBV2	1456788	2174028	75.94%	7.716%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048536.D
 Acq On : 08 Nov 2024 18:54
 Operator : RC/JU
 Sample : PB164769BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK769

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	17.974	2543	2548	2551	rBV6	5438	8792	0.31%	0.031%
38	18.297	2600	2603	2605	rBV4	2648	4501	0.16%	0.016%
39	19.015	2722	2725	2730	rBV2	16898	21815	0.76%	0.077%
40	19.086	2734	2737	2743	rVV	16197	23495	0.82%	0.083%
41	19.450	2793	2799	2813	rBV	1966463	2709935	94.66%	9.618%
42	20.950	3050	3054	3060	rBV2	98208	139367	4.87%	0.495%
43	21.286	3105	3111	3122	rBV	895343	1505218	52.58%	5.342%
44	23.997	3563	3572	3583	rBV	1179186	2862760	100.00%	10.161%
45	24.197	3598	3606	3617	rVB	641711	1639592	57.27%	5.819%




Sum of corrected areas: 28175263

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048536.D
Acq On : 08 Nov 2024 18:54
Operator : RC/JU
Sample : PB164769BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

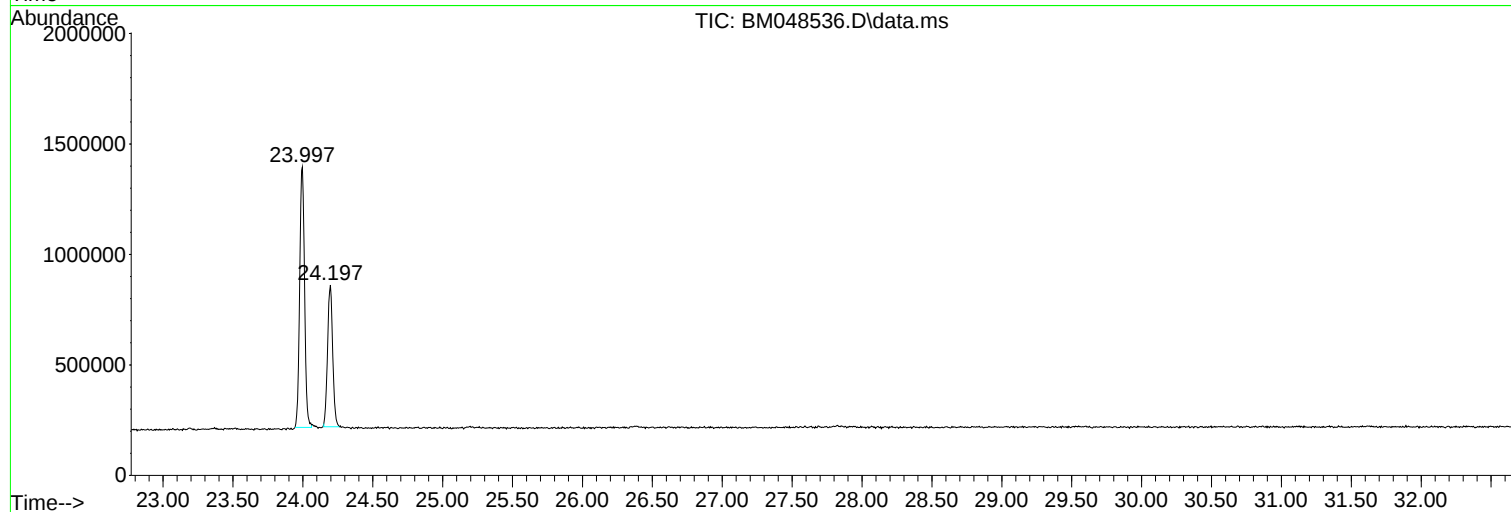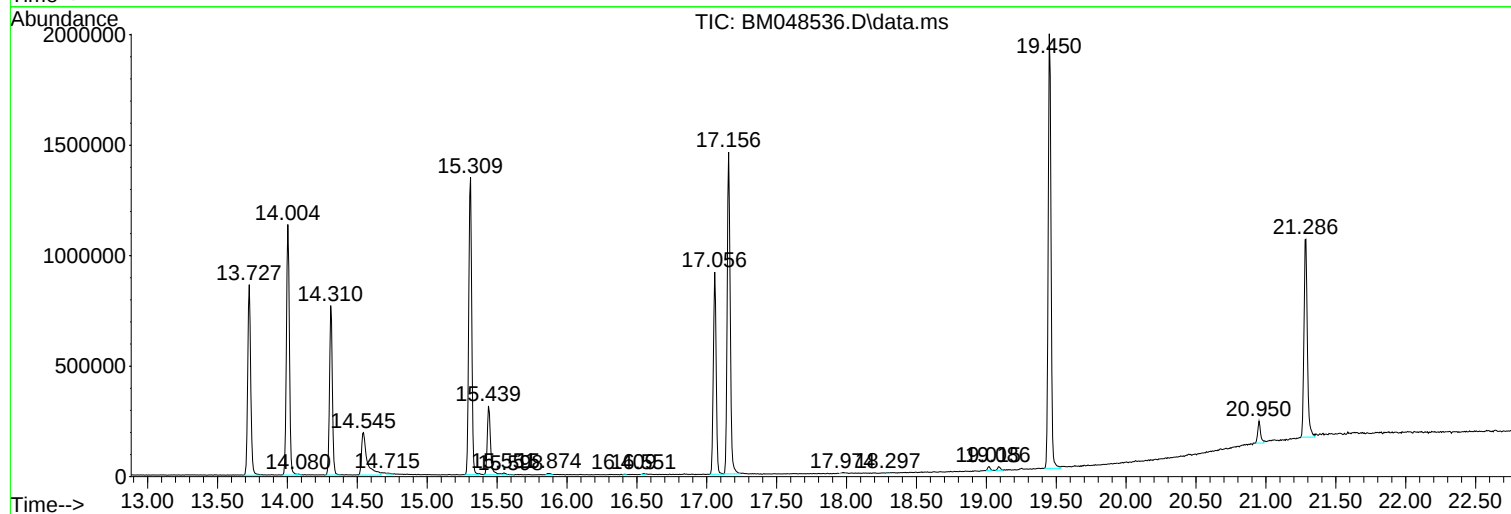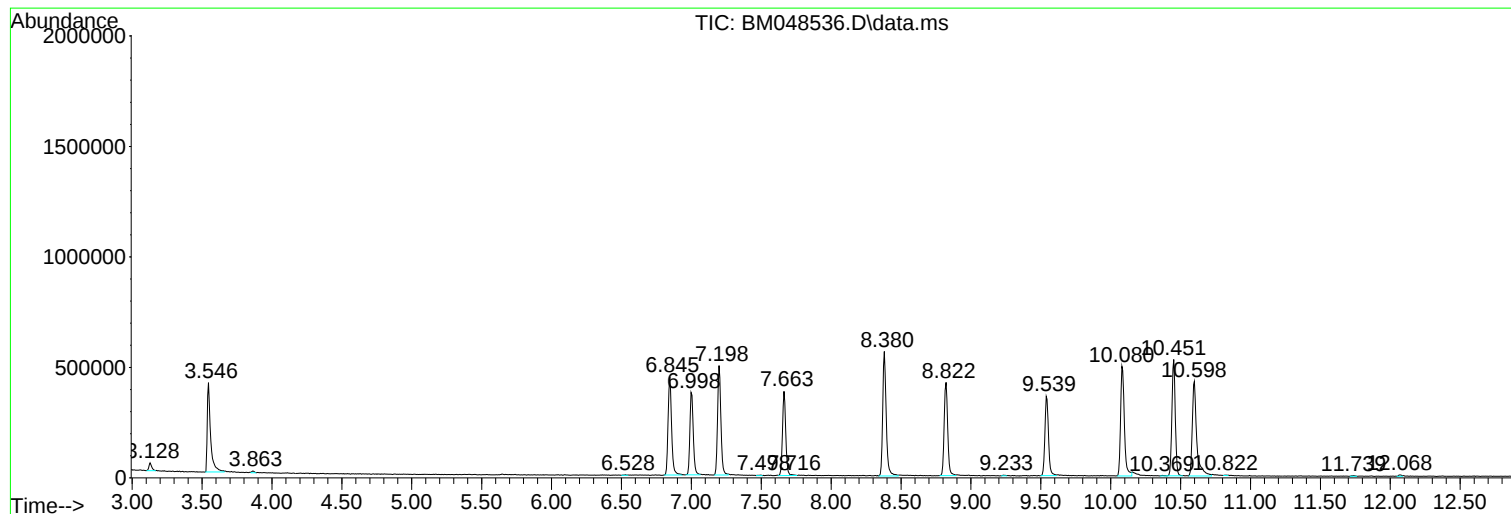

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048536.D
Acq On : 08 Nov 2024 18:54
Operator : RC/JU
Sample : PB164769BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048536.D
Acq On : 08 Nov 2024 18:54
Operator : RC/JU
Sample : PB164769BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc