

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048537.D
 Acq On : 08 Nov 2024 19:34
 Operator : RC/JU
 Sample : P4621-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	30	rBV	34764	44404	1.08%	0.125%
2	3.552	93	96	112	rBV	97619	190250	4.65%	0.534%
3	3.863	146	149	152	rVB3	6872	8302	0.20%	0.023%
4	4.387	233	238	242	rBV4	16238	24331	0.59%	0.068%
5	4.799	306	308	317	rVB7	5910	9284	0.23%	0.026%
6	5.657	449	454	459	rBV7	2719	6983	0.17%	0.020%
7	6.240	551	553	560	rVB7	2742	4657	0.11%	0.013%
8	6.846	650	656	675	rVB	196402	366350	8.95%	1.028%
9	6.998	675	682	696	rBV	454860	751644	18.36%	2.109%
10	7.198	709	716	729	rBV	540462	915130	22.35%	2.568%
11	7.287	729	731	738	rVB8	6124	9651	0.24%	0.027%
12	7.663	788	795	805	rBV	507206	823984	20.12%	2.312%
13	7.728	805	806	814	rVB6	5242	8758	0.21%	0.025%
14	8.381	911	917	930	rBV	516695	893185	21.81%	2.506%
15	8.492	933	936	940	rVB4	5355	7646	0.19%	0.021%
16	8.822	984	992	1002	rBV	513639	874518	21.36%	2.454%
17	9.539	1108	1114	1131	rBV	411603	725017	17.71%	2.034%
18	10.081	1199	1206	1229	rBV	605148	1133885	27.69%	3.182%
19	10.451	1260	1269	1280	rVB	704446	1180122	28.82%	3.311%
20	10.598	1286	1294	1313	rBV	407705	898076	21.93%	2.520%
21	11.028	1364	1367	1372	rVB6	4020	6506	0.16%	0.018%
22	11.081	1372	1376	1380	rBV6	5009	9467	0.23%	0.027%
23	12.069	1538	1544	1547	rBV4	5998	11731	0.29%	0.033%
24	13.216	1734	1739	1744	rVB2	10583	16758	0.41%	0.047%
25	13.727	1819	1826	1831	rBV	1197534	1642200	40.11%	4.608%
26	13.774	1831	1834	1843	rVB	60937	88382	2.16%	0.248%
27	14.004	1866	1873	1892	rBV	1353203	2010733	49.11%	5.642%
28	14.186	1898	1904	1909	rBV7	4292	11116	0.27%	0.031%
29	14.310	1919	1925	1935	rVB	1017992	1495695	36.53%	4.197%
30	14.457	1945	1950	1956	rVB7	3394	5540	0.14%	0.016%
31	14.551	1958	1966	1981	rBV2	83164	231692	5.66%	0.650%
32	15.310	2088	2095	2101	rBV	1755199	2558877	62.49%	7.180%
33	15.357	2101	2103	2109	rVV5	23331	37700	0.92%	0.106%
34	15.439	2111	2117	2133	rVV	521971	791406	19.33%	2.221%
35	15.551	2133	2136	2143	rVB5	9854	13264	0.32%	0.037%
36	15.868	2187	2190	2193	rBV5	6376	7688	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048537.D
 Acq On : 08 Nov 2024 19:34
 Operator : RC/JU
 Sample : P4621-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	16.551	2301	2306	2313	rBV7	6697	15218	0.37%	0.043%
38	16.721	2330	2335	2342	rBV	58658	101554	2.48%	0.285%
39	17.057	2386	2392	2403	rBV	1236794	1762020	43.03%	4.944%
40	17.157	2403	2409	2422	rVV	2119717	3078902	75.19%	8.639%
41	17.468	2458	2462	2468	rBV7	3217	6810	0.17%	0.019%
42	17.957	2541	2545	2551	rBV6	18077	31001	0.76%	0.087%
43	18.033	2556	2558	2561	rVB4	4662	4445	0.11%	0.012%
44	19.015	2722	2725	2730	rVB3	26948	32303	0.79%	0.091%
45	19.092	2734	2738	2742	rBV2	29720	42914	1.05%	0.120%
46	19.245	2760	2764	2768	rBV5	17023	25731	0.63%	0.072%
47	19.451	2793	2799	2812	rBV	2755099	3944585	96.34%	11.068%
48	20.950	3050	3054	3062	rBV	96321	150384	3.67%	0.422%
49	21.286	3105	3111	3122	rBV	1360150	2083128	50.87%	5.845%
50	23.997	3563	3572	3586	rVB	1749429	4094610	100.00%	11.489%
51	24.191	3597	3605	3624	rVB	940136	2451271	59.87%	6.878%




Sum of corrected areas: 35639808

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048537.D
Acq On : 08 Nov 2024 19:34
Operator : RC/JU
Sample : P4621-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

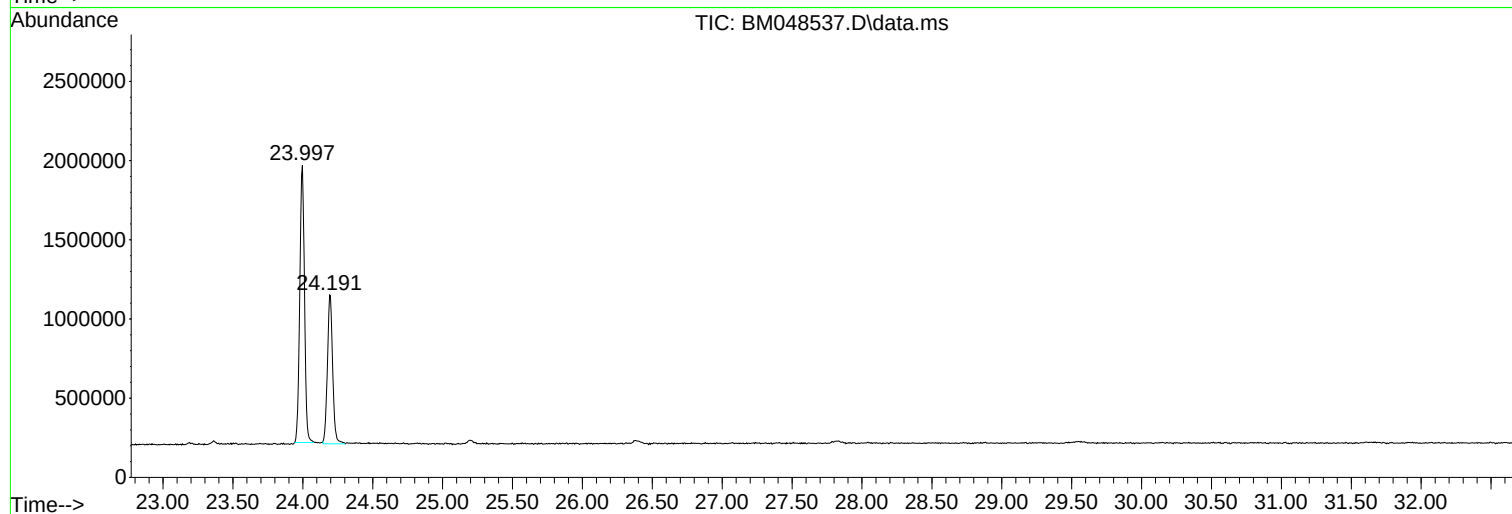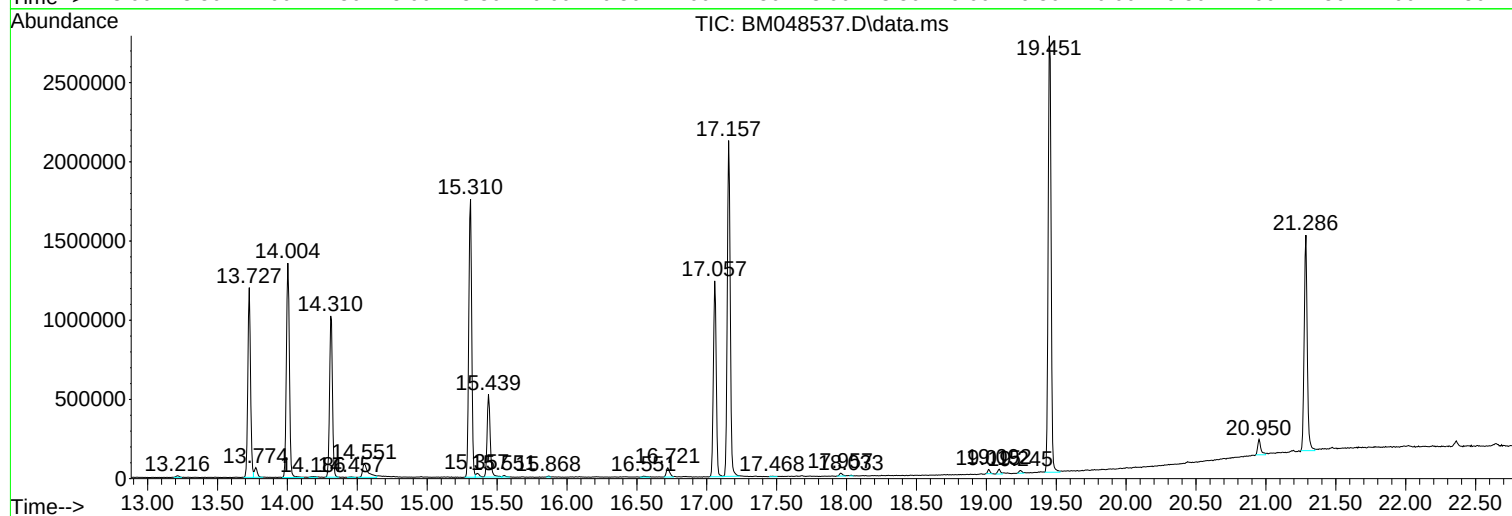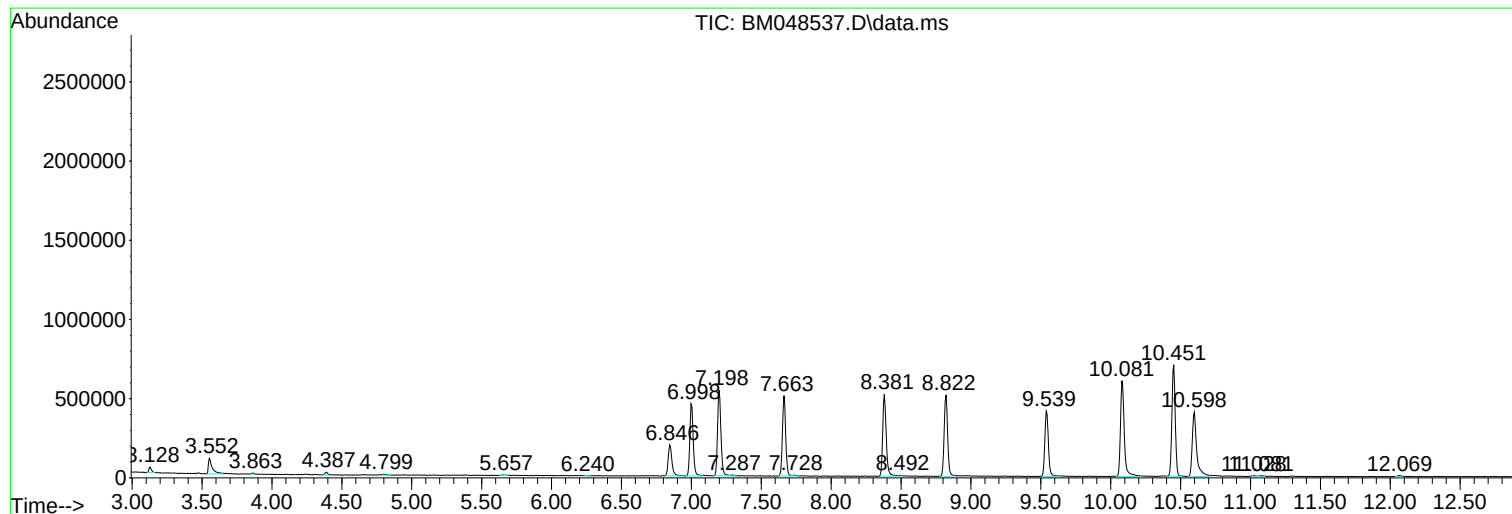

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048537.D
Acq On : 08 Nov 2024 19:34
Operator : RC/JU
Sample : P4621-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048537.D
Acq On : 08 Nov 2024 19:34
Operator : RC/JU
Sample : P4621-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc