

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048538.D
 Acq On : 08 Nov 2024 20:13
 Operator : RC/JU
 Sample : P4621-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	32	rVB	36568	53045	1.33%	0.157%
2	3.551	93	96	109	rBV	81355	154987	3.88%	0.460%
3	3.863	147	149	154	rVB2	9095	11850	0.30%	0.035%
4	4.798	304	308	312	rVB7	5669	9597	0.24%	0.028%
5	6.845	650	656	671	rVB	192061	343531	8.59%	1.019%
6	6.998	676	682	696	rBV	445241	729643	18.25%	2.165%
7	7.198	709	716	726	rBV	547428	891062	22.29%	2.643%
8	7.292	728	732	734	rBV5	3666	4644	0.12%	0.014%
9	7.663	788	795	804	rBV	502558	804296	20.12%	2.386%
10	7.745	804	809	812	rVB4	5430	9862	0.25%	0.029%
11	8.381	910	917	929	rBV	517897	891850	22.31%	2.646%
12	8.492	933	936	942	rVB6	4870	9571	0.24%	0.028%
13	8.822	984	992	1005	rBV	502435	869038	21.74%	2.578%
14	9.539	1107	1114	1129	rBV	408031	715894	17.91%	2.124%
15	9.669	1133	1136	1142	rVB6	2826	5587	0.14%	0.017%
16	10.080	1200	1206	1228	rBV	520444	1132627	28.33%	3.360%
17	10.451	1262	1269	1278	rBV	686146	1139415	28.50%	3.380%
18	10.516	1278	1280	1284	rVB5	3577	4226	0.11%	0.013%
19	10.616	1288	1297	1310	rBV	38299	118186	2.96%	0.351%
20	11.080	1371	1376	1379	rBV5	2879	4880	0.12%	0.014%
21	11.133	1379	1385	1388	rBV7	3287	6347	0.16%	0.019%
22	11.298	1411	1413	1419	rVB7	3377	5396	0.13%	0.016%
23	12.063	1538	1543	1549	rBV4	6198	13361	0.33%	0.040%
24	13.286	1746	1751	1753	rBV5	3138	5557	0.14%	0.016%
25	13.727	1819	1826	1831	rBV	1201248	1677527	41.96%	4.977%
26	13.774	1831	1834	1845	rVB	64400	95870	2.40%	0.284%
27	14.004	1865	1873	1884	rBV	1304112	1908513	47.74%	5.662%
28	14.310	1918	1925	1934	rBV	988613	1452299	36.33%	4.308%
29	14.551	1960	1966	1985	rBV2	71772	212289	5.31%	0.630%
30	14.757	1997	2001	2007	rVB6	7935	11914	0.30%	0.035%
31	15.309	2088	2095	2101	rBV	1683852	2559453	64.02%	7.593%
32	15.357	2101	2103	2111	rVV3	30579	51857	1.30%	0.154%
33	15.439	2111	2117	2132	rVV	512680	783681	19.60%	2.325%
34	15.551	2132	2136	2142	rVB5	10329	17709	0.44%	0.053%
35	15.862	2186	2189	2196	rBV4	6350	11510	0.29%	0.034%
36	16.204	2244	2247	2252	rVB7	3647	4769	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048538.D
Acq On : 08 Nov 2024 20:13
Operator : RC/JU
Sample : P4621-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	16.551	2302	2306	2310	rBV5	5760	8428	0.21%	0.025%
38	16.727	2332	2336	2343	rVB6	11591	20775	0.52%	0.062%
39	17.056	2386	2392	2402	rBV	1179255	1686196	42.18%	5.002%
40	17.156	2403	2409	2421	rVV	2038396	2963830	74.13%	8.793%
41	17.956	2540	2545	2554	rBV8	12194	28515	0.71%	0.085%
42	18.027	2554	2557	2562	rVB3	3464	5907	0.15%	0.018%
43	19.015	2721	2725	2729	rBV2	26953	37619	0.94%	0.112%
44	19.092	2733	2738	2741	rBV	27545	38088	0.95%	0.113%
45	19.245	2760	2764	2769	rBV7	12952	21593	0.54%	0.064%
46	19.450	2793	2799	2812	rBV	2628957	3664782	91.67%	10.872%
47	20.950	3050	3054	3063	rBV	93033	146125	3.65%	0.433%
48	21.280	3105	3110	3120	rBV	1258720	1973760	49.37%	5.855%
49	23.991	3563	3571	3591	rVB	1629275	3997993	100.00%	11.861%
50	24.191	3597	3605	3620	rVB	932631	2392877	59.85%	7.099%




Sum of corrected areas: 33708331

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048538.D
Acq On : 08 Nov 2024 20:13
Operator : RC/JU
Sample : P4621-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

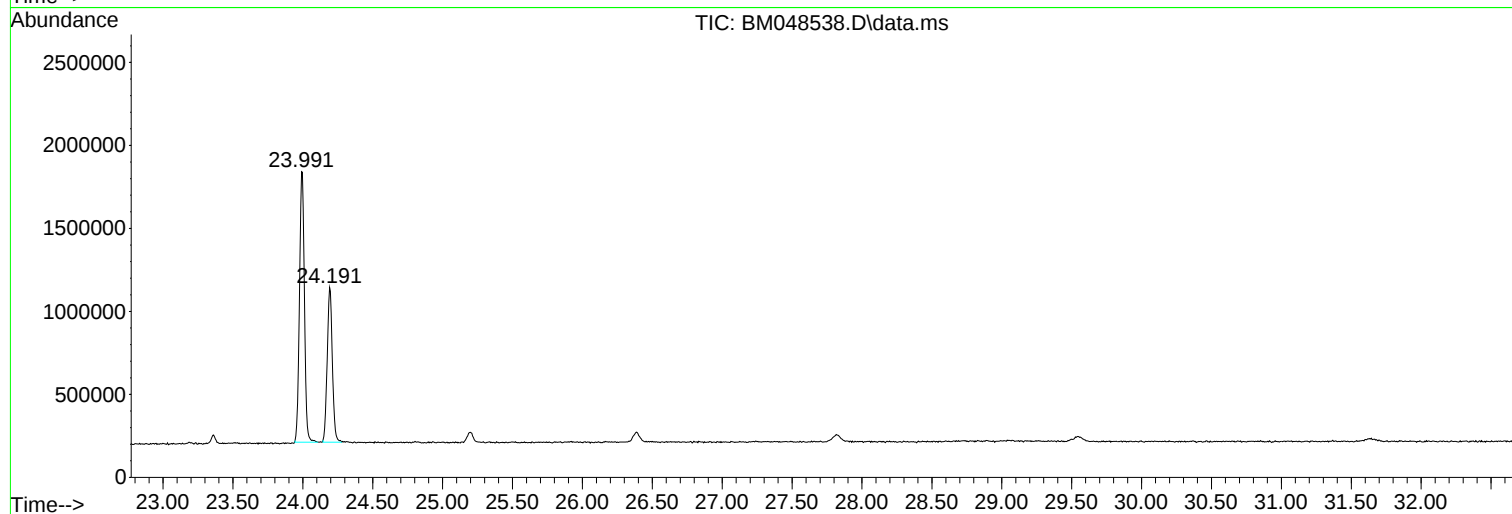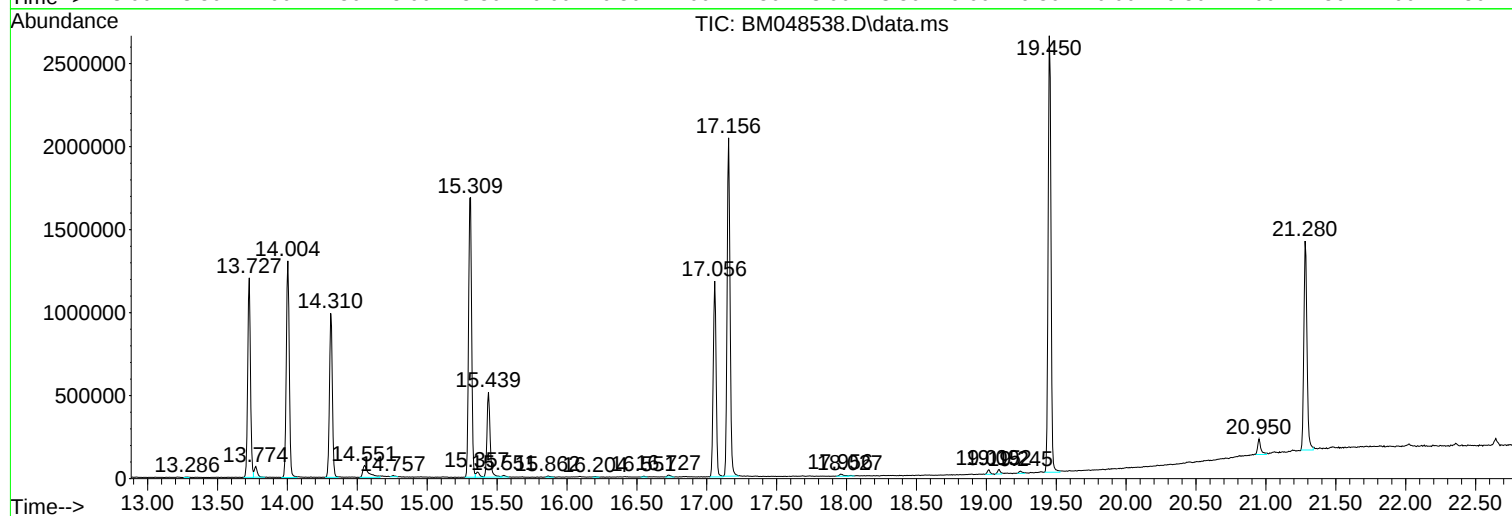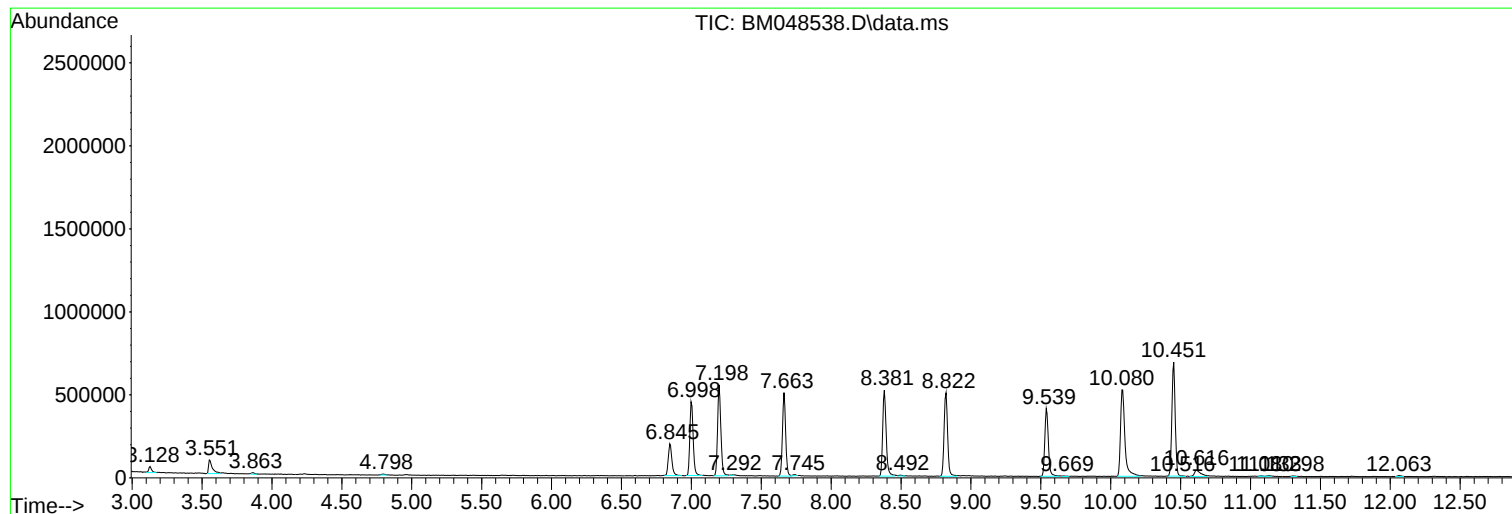

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048538.D
Acq On : 08 Nov 2024 20:13
Operator : RC/JU
Sample : P4621-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048538.D
Acq On : 08 Nov 2024 20:13
Operator : RC/JU
Sample : P4621-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc