

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048539.D
 Acq On : 08 Nov 2024 20:53
 Operator : RC/JU
 Sample : P4621-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048539.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	21	24	31	rVB	35642	47059	1.21%	0.133%
2	3.552	92	96	114	rBV	151274	292690	7.54%	0.828%
3	3.863	145	149	152	rVB4	8810	10998	0.28%	0.031%
4	4.375	234	236	240	rVB5	3722	4884	0.13%	0.014%
5	5.646	449	452	458	rBV6	2669	4904	0.13%	0.014%
6	6.846	650	656	670	rBV	192417	342859	8.83%	0.970%
7	6.999	676	682	696	rBV	493789	795380	20.48%	2.251%
8	7.199	709	716	727	rBV	576780	950742	24.48%	2.691%
9	7.422	751	754	757	rVB4	3179	4509	0.12%	0.013%
10	7.487	762	765	769	rVV6	2996	4167	0.11%	0.012%
11	7.663	788	795	805	rBV	513676	840449	21.64%	2.379%
12	7.734	805	807	811	rVB4	3368	4257	0.11%	0.012%
13	8.381	910	917	926	rBV	510652	875184	22.54%	2.477%
14	8.498	933	937	941	rVB6	5013	8978	0.23%	0.025%
15	8.822	984	992	1002	rBV	527988	910583	23.45%	2.577%
16	9.540	1107	1114	1127	rBV	438334	751238	19.34%	2.126%
17	10.081	1199	1206	1217	rBV	628101	1145874	29.51%	3.243%
18	10.451	1261	1269	1278	rBV	695367	1181541	30.43%	3.344%
19	10.598	1286	1294	1314	rBV	455124	1014025	26.11%	2.870%
20	11.028	1362	1367	1371	rVB6	3194	5923	0.15%	0.017%
21	11.081	1373	1376	1380	rBV5	2589	4471	0.12%	0.013%
22	11.304	1409	1414	1419	rVB7	2354	4885	0.13%	0.014%
23	12.069	1539	1544	1551	rBV3	7658	15278	0.39%	0.043%
24	12.922	1687	1689	1694	rVB6	4162	6281	0.16%	0.018%
25	13.728	1819	1826	1831	rBV	1263416	1784011	45.94%	5.049%
26	13.775	1831	1834	1840	rVB	124357	179423	4.62%	0.508%
27	14.004	1866	1873	1883	rBV	1395187	2051427	52.83%	5.806%
28	14.310	1918	1925	1934	rBV	1026454	1507101	38.81%	4.266%
29	14.557	1961	1967	1974	rBV	61526	146206	3.76%	0.414%
30	14.757	1999	2001	2008	rVB6	5261	8263	0.21%	0.023%
31	15.310	2088	2095	2102	rBV	1736189	2617187	67.39%	7.408%
32	15.357	2102	2103	2111	rVV7	18196	26985	0.69%	0.076%
33	15.439	2111	2117	2132	rVV	489874	736661	18.97%	2.085%
34	15.551	2132	2136	2141	rVB6	8721	14539	0.37%	0.041%
35	15.874	2185	2191	2194	rBV5	4995	9448	0.24%	0.027%
36	16.551	2301	2306	2309	rBV4	3658	6359	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048539.D
Acq On : 08 Nov 2024 20:53
Operator : RC/JU
Sample : P4621-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	16.839	2350	2355	2357	rBV5	3204	5727	0.15%	0.016%
38	17.057	2385	2392	2402	rBV	1285750	1765853	45.47%	4.998%
39	17.157	2402	2409	2423	rVV	2063930	2996737	77.17%	8.482%
40	17.686	2493	2499	2501	rBV5	2395	3892	0.10%	0.011%
41	17.721	2504	2505	2511	rVB6	3888	4526	0.12%	0.013%
42	17.963	2542	2546	2552	rBV9	9681	19178	0.49%	0.054%
43	19.015	2721	2725	2730	rBV3	23989	35275	0.91%	0.100%
44	19.086	2733	2737	2741	rBV	25483	38377	0.99%	0.109%
45	19.245	2761	2764	2769	rBV7	10701	15621	0.40%	0.044%
46	19.451	2793	2799	2813	rBV	2675631	3687259	94.95%	10.436%
47	20.951	3050	3054	3063	rBV	82295	125554	3.23%	0.355%
48	21.280	3105	3110	3121	rBV	1315275	2056583	52.96%	5.821%
49	23.992	3563	3571	3584	rBV	1591436	3883435	100.00%	10.992%
50	24.192	3597	3605	3618	rVB	947625	2378022	61.24%	6.731%




Sum of corrected areas: 35330808

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048539.D
Acq On : 08 Nov 2024 20:53
Operator : RC/JU
Sample : P4621-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

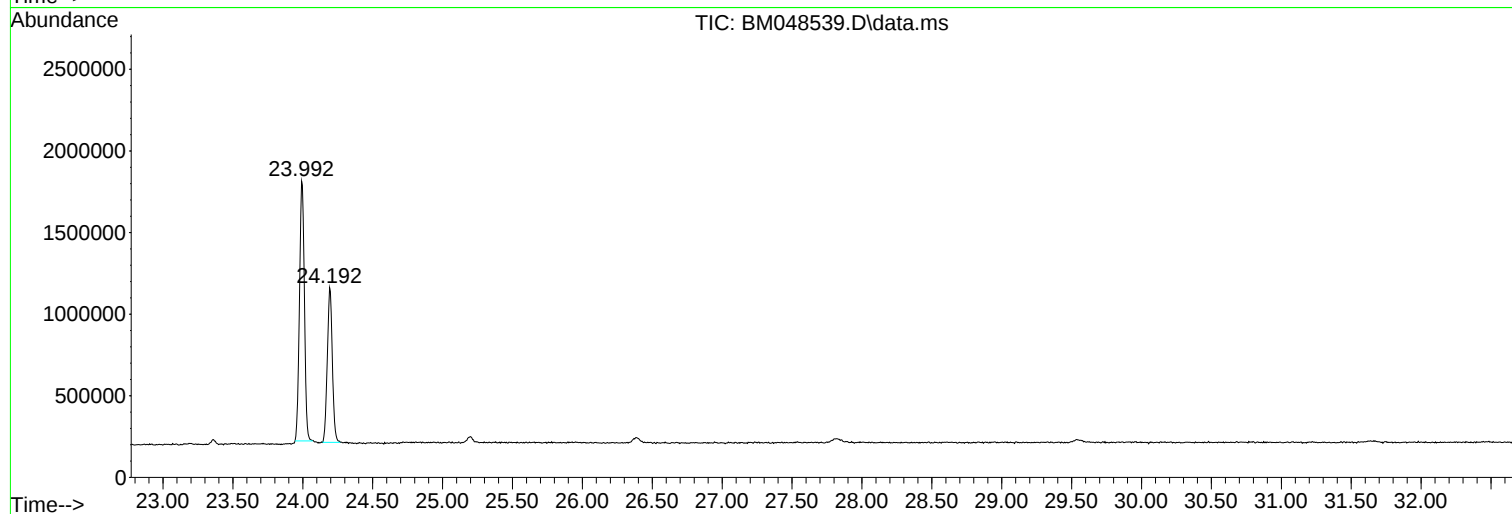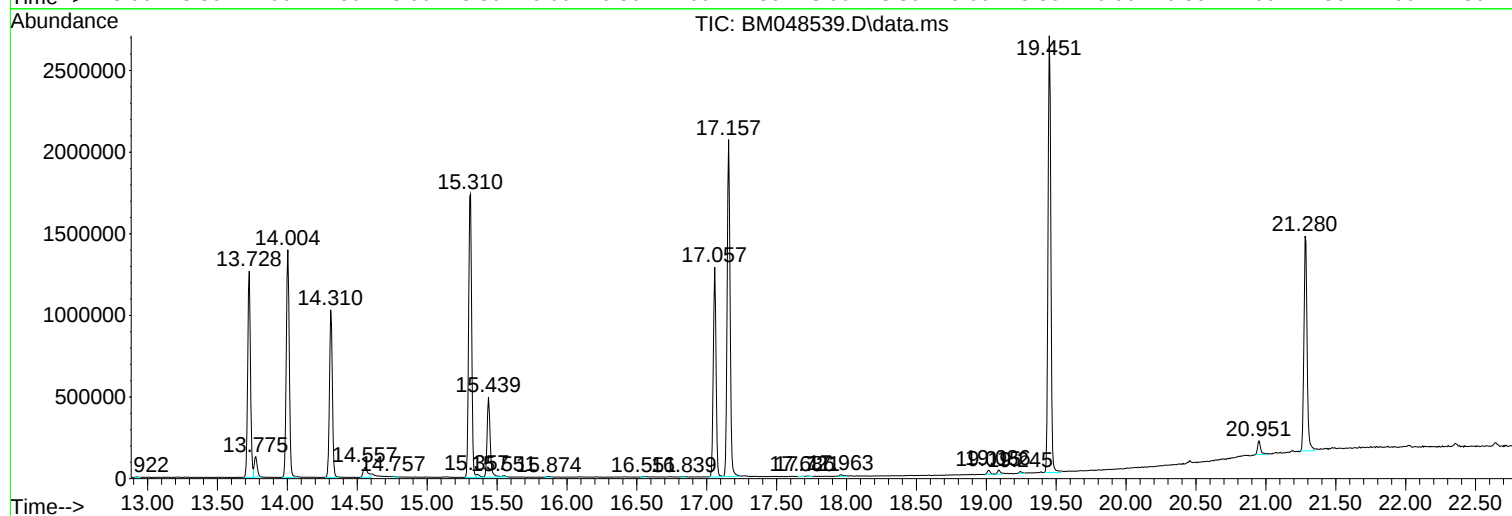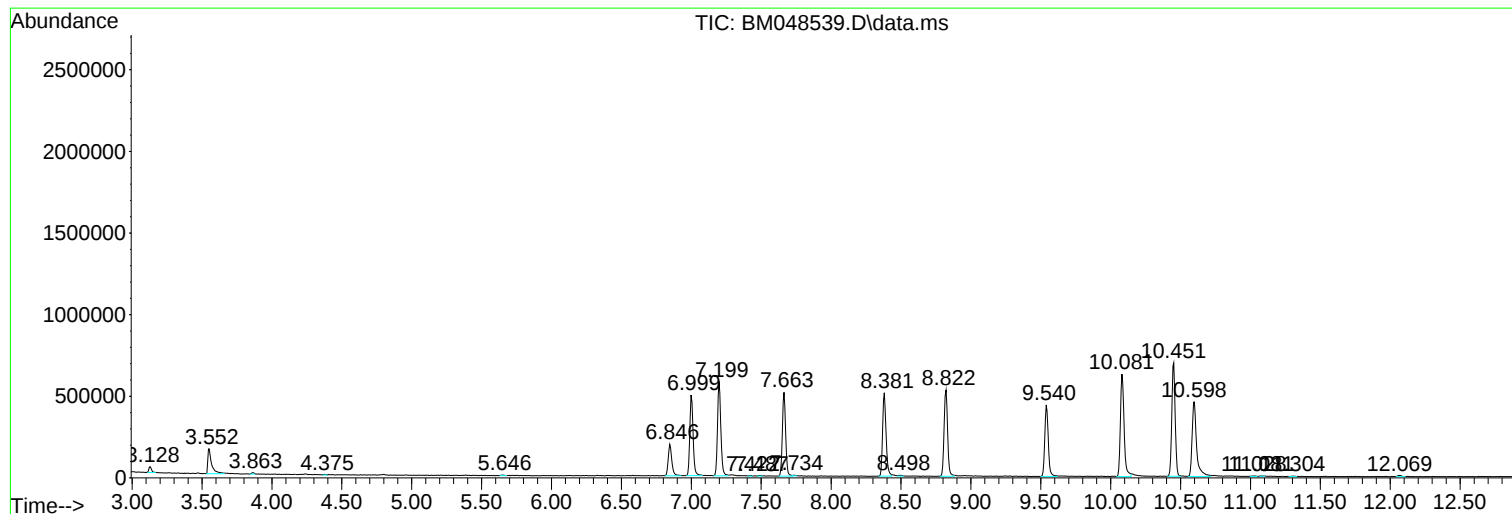

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048539.D
Acq On : 08 Nov 2024 20:53
Operator : RC/JU
Sample : P4621-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048539.D
Acq On : 08 Nov 2024 20:53
Operator : RC/JU
Sample : P4621-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc