

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048540.D
 Acq On : 08 Nov 2024 21:32
 Operator : RC/JU
 Sample : P4621-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	29	rBV	36249	49147	1.34%	0.147%
2	3.475	79	83	86	rBV5	5529	7019	0.19%	0.021%
3	3.551	93	96	110	rBV	84748	164087	4.49%	0.491%
4	3.863	145	149	152	rBV2	9235	12094	0.33%	0.036%
5	4.798	305	308	314	rVB3	6569	10221	0.28%	0.031%
6	4.963	333	336	340	rVB6	6452	9810	0.27%	0.029%
7	5.651	447	453	455	rBV6	3613	7068	0.19%	0.021%
8	6.334	565	569	574	rVB8	4774	9077	0.25%	0.027%
9	6.845	649	656	670	rVV	182902	332409	9.10%	0.995%
10	6.998	676	682	696	rBV	462392	774415	21.19%	2.319%
11	7.198	709	716	726	rBV	554997	924229	25.29%	2.768%
12	7.663	788	795	807	rBV	478399	788151	21.57%	2.360%
13	8.381	910	917	932	rBV	506604	876925	24.00%	2.626%
14	8.498	932	937	943	rVB4	9511	18421	0.50%	0.055%
15	8.822	985	992	1006	rBV	524545	898552	24.59%	2.691%
16	9.539	1108	1114	1127	rBV	428473	732645	20.05%	2.194%
17	10.022	1191	1196	1200	rVB6	3274	5676	0.16%	0.017%
18	10.080	1200	1206	1228	rBV	560168	1171926	32.07%	3.509%
19	10.451	1262	1269	1287	rVB	671184	1122854	30.73%	3.362%
20	10.610	1290	1296	1315	rVV	49990	141328	3.87%	0.423%
21	11.010	1357	1364	1370	rBV4	8159	20160	0.55%	0.060%
22	11.075	1370	1375	1383	rVB3	9208	22329	0.61%	0.067%
23	11.304	1409	1414	1418	rVB6	3061	5483	0.15%	0.016%
24	12.063	1537	1543	1551	rVB3	7920	15085	0.41%	0.045%
25	12.316	1582	1586	1590	rVB5	2477	3947	0.11%	0.012%
26	12.657	1642	1644	1650	rBV4	2604	4587	0.13%	0.014%
27	12.921	1683	1689	1694	rBV6	3746	7811	0.21%	0.023%
28	13.210	1735	1738	1739	rBV3	5751	4340	0.12%	0.013%
29	13.727	1820	1826	1830	rBV	1224264	1652026	45.21%	4.947%
30	13.774	1830	1834	1845	rVB	202559	302300	8.27%	0.905%
31	14.004	1865	1873	1884	rBV	1339906	1966422	53.81%	5.888%
32	14.310	1918	1925	1935	rBV	960736	1409724	38.58%	4.221%
33	14.551	1959	1966	1977	rBV2	67474	179990	4.93%	0.539%
34	14.951	2031	2034	2037	rVB3	3585	5080	0.14%	0.015%
35	14.992	2037	2041	2044	rBV4	6097	7587	0.21%	0.023%
36	15.110	2054	2061	2065	rBV6	9424	14735	0.40%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048540.D
 Acq On : 08 Nov 2024 21:32
 Operator : RC/JU
 Sample : P4621-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	15.310	2088	2095	2101	rBV	1699235	2556493	69.96%	7.655%
38	15.362	2101	2104	2109	rVV3	31148	48041	1.31%	0.144%
39	15.439	2109	2117	2131	rVV	498670	765735	20.95%	2.293%
40	15.545	2131	2135	2139	rVV6	12460	24334	0.67%	0.073%
41	15.574	2139	2140	2145	rVB5	7057	7297	0.20%	0.022%
42	15.674	2151	2157	2162	rBV6	7974	14432	0.39%	0.043%
43	15.809	2177	2180	2186	rVV5	3742	6407	0.18%	0.019%
44	15.868	2186	2190	2197	rVB5	10012	17674	0.48%	0.053%
45	15.939	2197	2202	2206	rBV7	2780	4999	0.14%	0.015%
46	16.039	2215	2219	2226	rVB7	9509	16259	0.44%	0.049%
47	16.174	2239	2242	2246	rBV4	4593	5213	0.14%	0.016%
48	16.215	2246	2249	2252	rVB3	3317	3921	0.11%	0.012%
49	16.362	2271	2274	2279	rVB5	4041	5970	0.16%	0.018%
50	16.421	2279	2284	2290	rBV5	14882	26972	0.74%	0.081%
51	16.551	2303	2306	2308	rBV4	3831	3761	0.10%	0.011%
52	16.609	2312	2316	2319	rBV6	5529	10389	0.28%	0.031%
53	16.727	2329	2336	2340	rBV9	8641	17203	0.47%	0.052%
54	16.933	2369	2371	2377	rVB7	4414	5856	0.16%	0.018%
55	17.056	2386	2392	2402	rBV	1191096	1654546	45.28%	4.955%
56	17.156	2402	2409	2423	rBV	2044833	2858575	78.23%	8.560%
57	17.268	2425	2428	2431	rVB5	7393	10542	0.29%	0.032%
58	17.351	2440	2442	2444	rVB3	5514	4728	0.13%	0.014%
59	17.468	2458	2462	2467	rBV6	6431	12535	0.34%	0.038%
60	17.727	2502	2506	2510	rVB5	6367	8390	0.23%	0.025%
61	17.956	2542	2545	2551	rBV7	8690	14630	0.40%	0.044%
62	18.121	2571	2573	2579	rVB5	6618	7706	0.21%	0.023%
63	18.333	2606	2609	2611	rVB4	7055	8168	0.22%	0.024%
64	18.856	2695	2698	2702	rBV3	10680	14103	0.39%	0.042%
65	19.015	2721	2725	2729	rVB3	28511	37736	1.03%	0.113%
66	19.092	2733	2738	2741	rBV2	25712	37370	1.02%	0.112%
67	19.245	2761	2764	2769	rBV5	10270	15791	0.43%	0.047%
68	19.450	2793	2799	2814	rBV	2508283	3555974	97.31%	10.648%
69	19.697	2838	2841	2843	rBV4	12071	12921	0.35%	0.039%
70	20.950	3051	3054	3061	rVB	87843	106508	2.91%	0.319%
71	21.286	3105	3111	3121	rBV2	1212014	1944184	53.20%	5.822%
72	23.997	3563	3572	3584	rBV	1538007	3654239	100.00%	10.943%
73	24.197	3597	3606	3619	rVB	854997	2217521	60.68%	6.640%




Sum of corrected areas: 33394783

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048540.D
Acq On : 08 Nov 2024 21:32
Operator : RC/JU
Sample : P4621-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

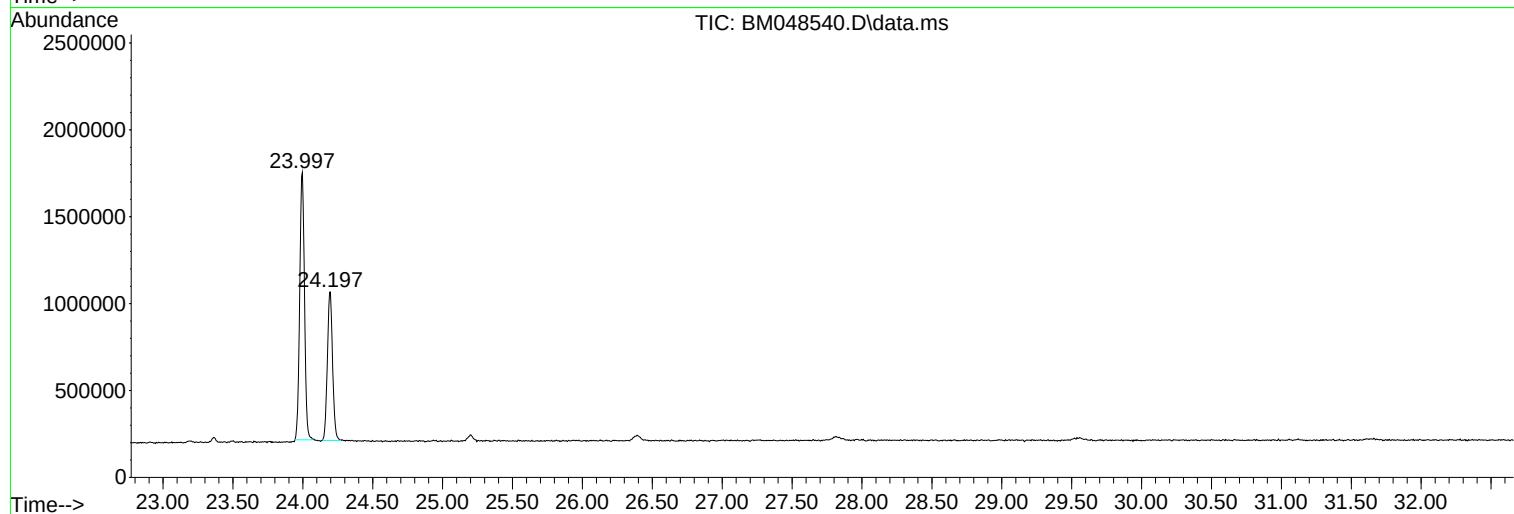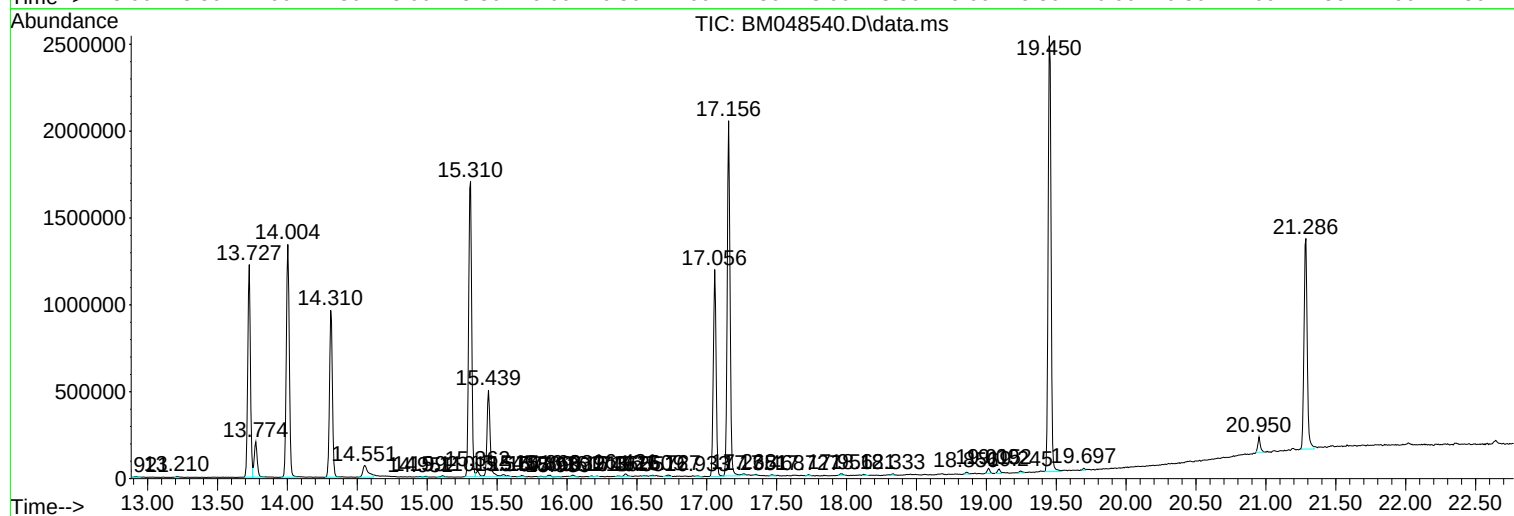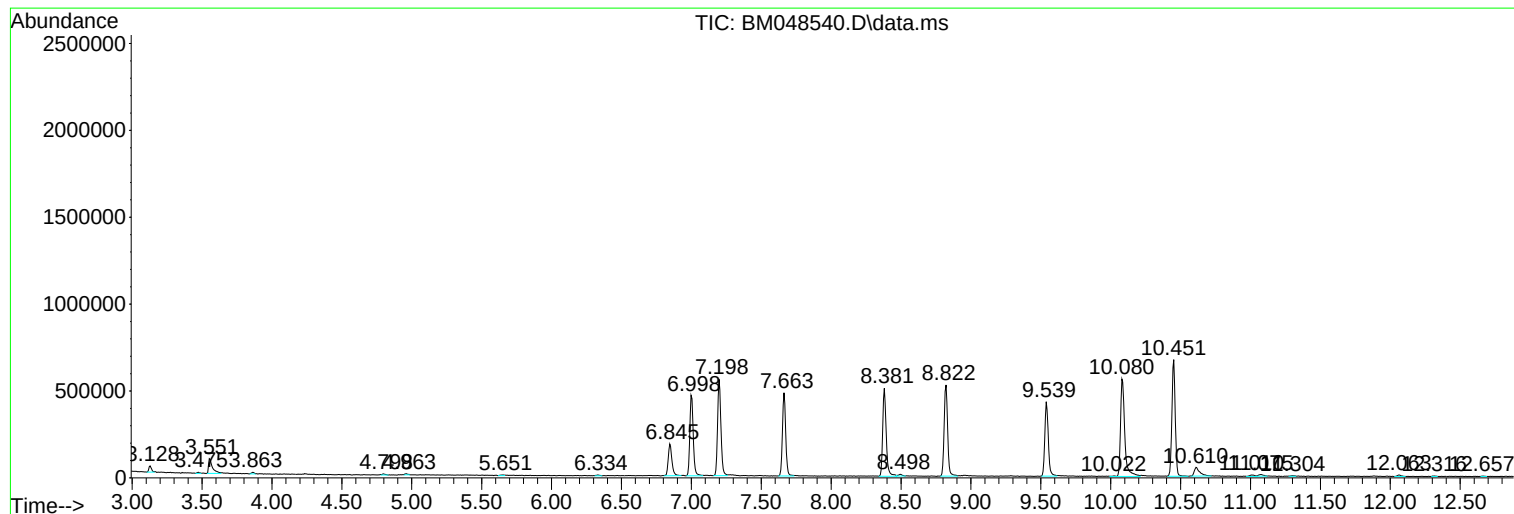

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048540.D
Acq On : 08 Nov 2024 21:32
Operator : RC/JU
Sample : P4621-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048540.D
Acq On : 08 Nov 2024 21:32
Operator : RC/JU
Sample : P4621-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc