

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048541.D
 Acq On : 08 Nov 2024 22:12
 Operator : RC/JU
 Sample : P4621-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	30	rVB	39888	51901	1.32%	0.147%
2	3.546	92	95	111	rBV	182759	338935	8.60%	0.962%
3	3.863	146	149	154	rVB3	8224	10402	0.26%	0.030%
4	4.240	209	213	217	rVB7	4646	7256	0.18%	0.021%
5	4.793	305	307	314	rVB3	7055	11551	0.29%	0.033%
6	5.257	384	386	391	rVB6	3158	4113	0.10%	0.012%
7	5.381	404	407	410	rBV5	3914	5581	0.14%	0.016%
8	5.646	448	452	455	rBV5	3912	5491	0.14%	0.016%
9	6.493	592	596	599	rBV5	2513	4311	0.11%	0.012%
10	6.846	650	656	669	rBV	217335	386597	9.81%	1.097%
11	6.998	676	682	693	rBV	470786	775310	19.67%	2.200%
12	7.198	710	716	729	rBV	571721	957811	24.30%	2.717%
13	7.287	729	731	737	rVB7	5065	8193	0.21%	0.023%
14	7.663	788	795	805	rBV	491101	810991	20.57%	2.301%
15	8.381	910	917	933	rBV	551954	955797	24.25%	2.712%
16	8.493	933	936	942	rVB6	5038	8990	0.23%	0.026%
17	8.822	985	992	1004	rBV	532522	926463	23.50%	2.629%
18	9.540	1107	1114	1126	rBV	437624	751519	19.06%	2.132%
19	10.081	1199	1206	1228	rBV	627532	1198775	30.41%	3.401%
20	10.451	1262	1269	1282	rVB	671451	1141882	28.97%	3.240%
21	10.592	1286	1293	1315	rBV	470595	1047628	26.58%	2.972%
22	11.028	1359	1367	1371	rBV8	4627	11855	0.30%	0.034%
23	11.086	1371	1377	1384	rVB7	4714	11058	0.28%	0.031%
24	11.304	1411	1414	1418	rBV5	3247	4965	0.13%	0.014%
25	12.063	1538	1543	1549	rBV5	7131	15305	0.39%	0.043%
26	13.727	1819	1826	1841	rBV	1185970	1714593	43.49%	4.865%
27	14.004	1864	1873	1883	rBV	1380031	2077874	52.71%	5.895%
28	14.310	1919	1925	1945	rBV	993608	1455507	36.92%	4.130%
29	14.551	1959	1966	1982	rBV	81455	224255	5.69%	0.636%
30	14.757	1999	2001	2007	rVB7	5044	7726	0.20%	0.022%
31	15.310	2088	2095	2101	rBV	1779503	2616704	66.38%	7.424%
32	15.363	2101	2104	2111	rVV4	22439	40417	1.03%	0.115%
33	15.439	2111	2117	2133	rVV	474498	743498	18.86%	2.109%
34	15.557	2133	2137	2142	rVB5	9945	17194	0.44%	0.049%
35	15.869	2183	2190	2196	rBV9	5597	10512	0.27%	0.030%
36	16.545	2303	2305	2312	rBV6	4705	9113	0.23%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048541.D
Acq On : 08 Nov 2024 22:12
Operator : RC/JU
Sample : P4621-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	17.057	2386	2392	2403	rBV	1187766	1700162	43.13%	4.824%
38	17.157	2403	2409	2421	rBV	2074412	2968781	75.31%	8.423%
39	17.268	2426	2428	2433	rVV5	4946	8549	0.22%	0.024%
40	17.351	2437	2442	2444	rBV5	3728	4334	0.11%	0.012%
41	17.680	2494	2498	2502	rBV6	6121	8522	0.22%	0.024%
42	17.962	2540	2546	2551	rBV7	16468	31076	0.79%	0.088%
43	18.033	2556	2558	2562	rVB3	4331	5043	0.13%	0.014%
44	19.015	2721	2725	2732	rVB3	27741	38138	0.97%	0.108%
45	19.092	2734	2738	2741	rBV	23691	33165	0.84%	0.094%
46	19.245	2759	2764	2771	rBV10	18534	34798	0.88%	0.099%
47	19.451	2793	2799	2810	rBV	2736708	3763709	95.47%	10.678%
48	20.951	3051	3054	3060	rVB	73945	89366	2.27%	0.254%
49	21.286	3105	3111	3120	rBV	1267301	1977855	50.17%	5.612%
50	23.997	3563	3572	3589	rVB	1614770	3942108	100.00%	11.184%
51	24.192	3597	3605	3617	rVB	876364	2270527	57.60%	6.442%




Sum of corrected areas: 35246206

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048541.D
Acq On : 08 Nov 2024 22:12
Operator : RC/JU
Sample : P4621-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

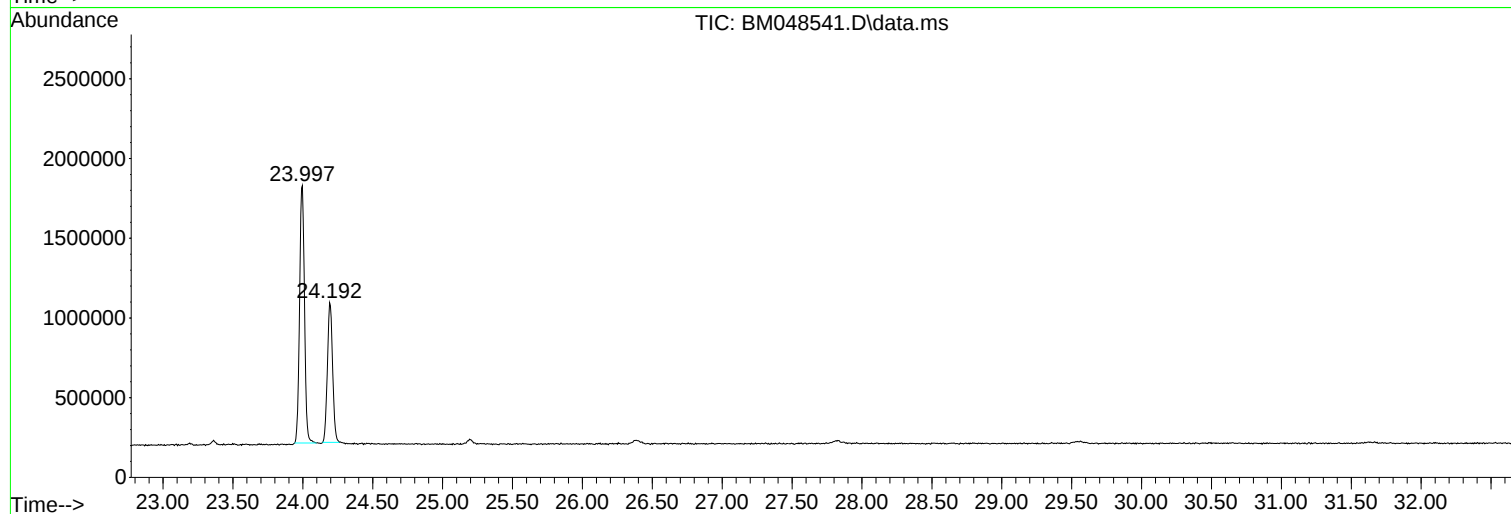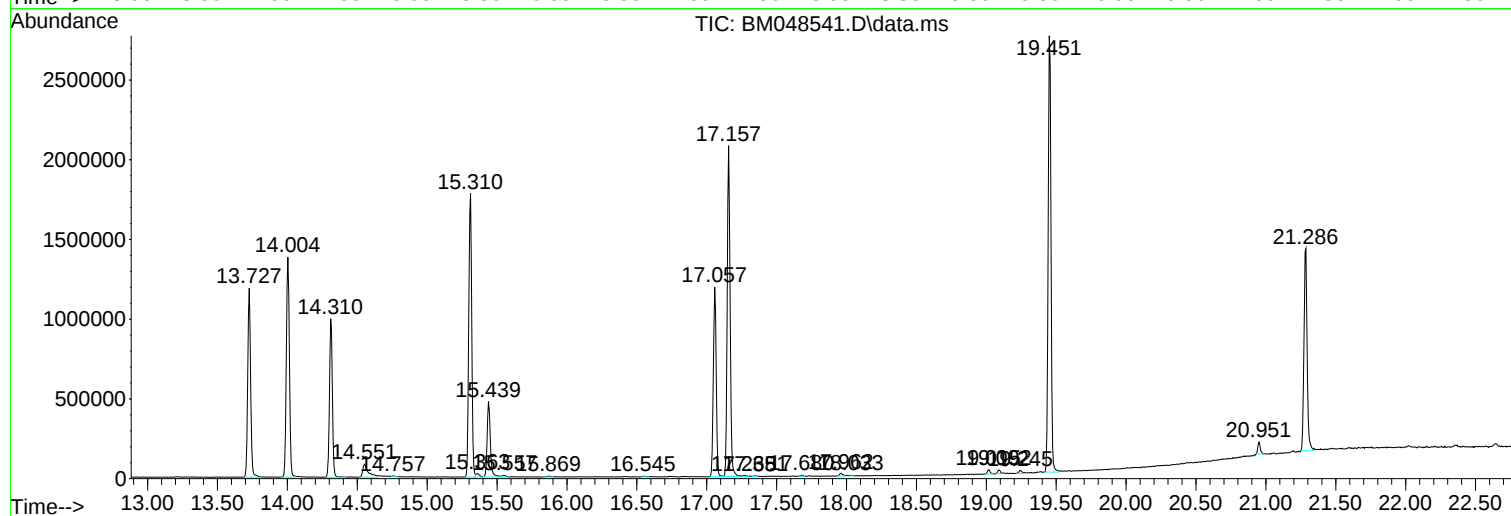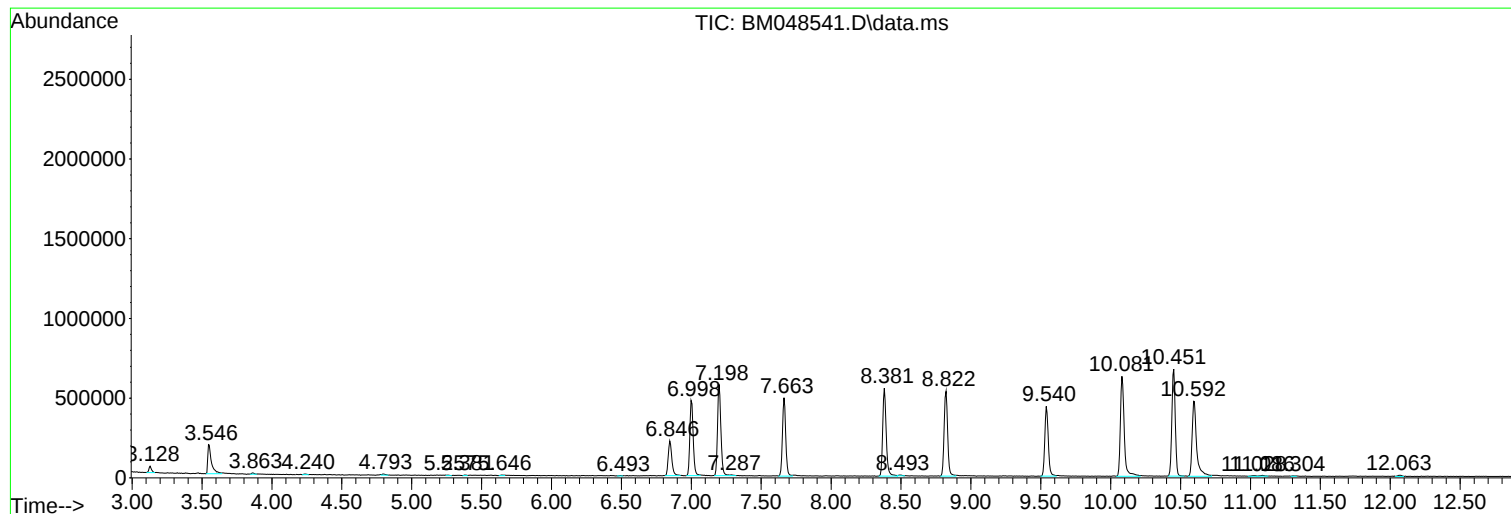

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048541.D
Acq On : 08 Nov 2024 22:12
Operator : RC/JU
Sample : P4621-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048541.D
Acq On : 08 Nov 2024 22:12
Operator : RC/JU
Sample : P4621-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc