

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048542.D
 Acq On : 08 Nov 2024 22:51
 Operator : RC/JU
 Sample : P4621-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH6N7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	29	rBV	32265	41749	1.20%	0.133%
2	3.551	93	96	107	rBV	85025	149971	4.30%	0.477%
3	3.863	146	149	153	rVB	9848	10190	0.29%	0.032%
4	4.957	332	335	340	rVB3	7163	10029	0.29%	0.032%
5	6.845	650	656	669	rBV	145053	263439	7.54%	0.838%
6	6.998	676	682	698	rBV	422293	695391	19.92%	2.211%
7	7.198	709	716	728	rBV	493199	816018	23.37%	2.594%
8	7.663	788	795	804	rBV	519821	847874	24.28%	2.696%
9	7.745	807	809	815	rVB6	4973	7486	0.21%	0.024%
10	8.380	910	917	932	rBV	404911	721855	20.67%	2.295%
11	8.498	932	937	945	rVB5	6838	16433	0.47%	0.052%
12	8.822	985	992	1007	rBV	462593	814746	23.33%	2.590%
13	9.539	1107	1114	1125	rBV	373469	652564	18.69%	2.075%
14	10.080	1199	1206	1229	rVV	503841	1039753	29.78%	3.306%
15	10.451	1262	1269	1281	rVB	683104	1159410	33.21%	3.686%
16	10.604	1288	1295	1316	rBV	166630	431573	12.36%	1.372%
17	11.022	1361	1366	1370	rBV4	4653	7448	0.21%	0.024%
18	11.086	1370	1377	1383	rVB7	5737	11359	0.33%	0.036%
19	12.063	1538	1543	1550	rBV2	7565	13463	0.39%	0.043%
20	12.139	1554	1556	1561	rVB5	3271	4508	0.13%	0.014%
21	13.215	1734	1739	1742	rVB5	2744	3700	0.11%	0.012%
22	13.727	1819	1826	1840	rBV	1057867	1517923	43.47%	4.826%
23	14.004	1865	1873	1884	rBV	1221208	1793839	51.38%	5.703%
24	14.310	1919	1925	1933	rBV	990679	1444093	41.36%	4.591%
25	14.557	1962	1967	1982	rBV3	45953	144255	4.13%	0.459%
26	14.757	1998	2001	2003	rBV3	4435	4559	0.13%	0.014%
27	15.309	2088	2095	2111	rBV	1590332	2339258	67.00%	7.438%
28	15.439	2111	2117	2130	rVV	447631	678544	19.43%	2.157%
29	15.551	2133	2136	2140	rVB4	8992	12380	0.35%	0.039%
30	15.874	2185	2191	2194	rBV6	5970	9930	0.28%	0.032%
31	16.421	2279	2284	2289	rBV7	3414	6423	0.18%	0.020%
32	16.551	2301	2306	2308	rBV6	4534	5917	0.17%	0.019%
33	16.739	2332	2338	2342	rBV7	3449	7094	0.20%	0.023%
34	17.056	2386	2392	2402	rBV	1203492	1717101	49.18%	5.459%
35	17.156	2402	2409	2423	rVV	1788990	2668730	76.43%	8.485%
36	17.733	2501	2507	2512	rBV8	3615	6522	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048542.D
Acq On : 08 Nov 2024 22:51
Operator : RC/JU
Sample : P4621-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	17.956	2541	2545	2553	rBV3	31314	51413	1.47%	0.163%
38	18.033	2556	2558	2561	rVB3	4194	3970	0.11%	0.013%
39	19.015	2721	2725	2732	rBV4	25162	38171	1.09%	0.121%
40	19.092	2734	2738	2741	rBV2	23797	32409	0.93%	0.103%
41	19.121	2741	2743	2746	rVB4	9617	10477	0.30%	0.033%
42	19.239	2760	2763	2770	rBV5	32893	51023	1.46%	0.162%
43	19.450	2793	2799	2811	rBV	2429281	3312024	94.86%	10.530%
44	20.950	3050	3054	3062	rBV	80171	117760	3.37%	0.374%
45	21.280	3105	3110	3123	rBV	1296191	2016287	57.75%	6.411%
46	23.997	3563	3572	3589	rVB	1437981	3491581	100.00%	11.101%
47	24.191	3597	3605	3616	rVB	909733	2251460	64.48%	7.158%




Sum of corrected areas: 31452102

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048542.D
Acq On : 08 Nov 2024 22:51
Operator : RC/JU
Sample : P4621-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

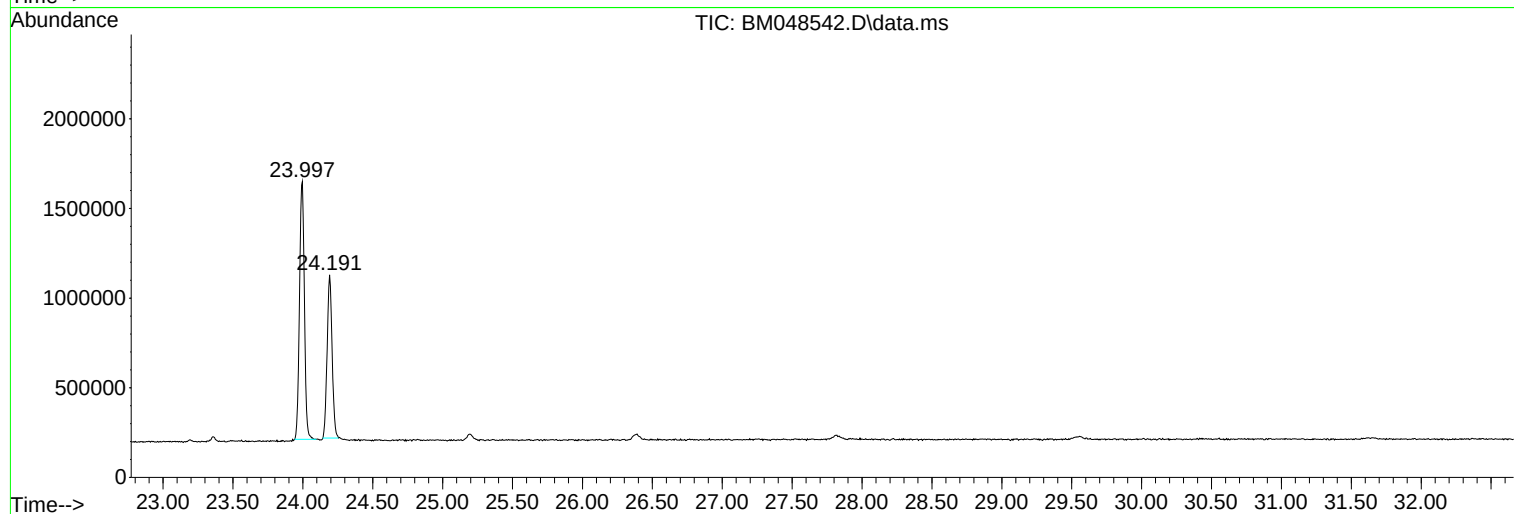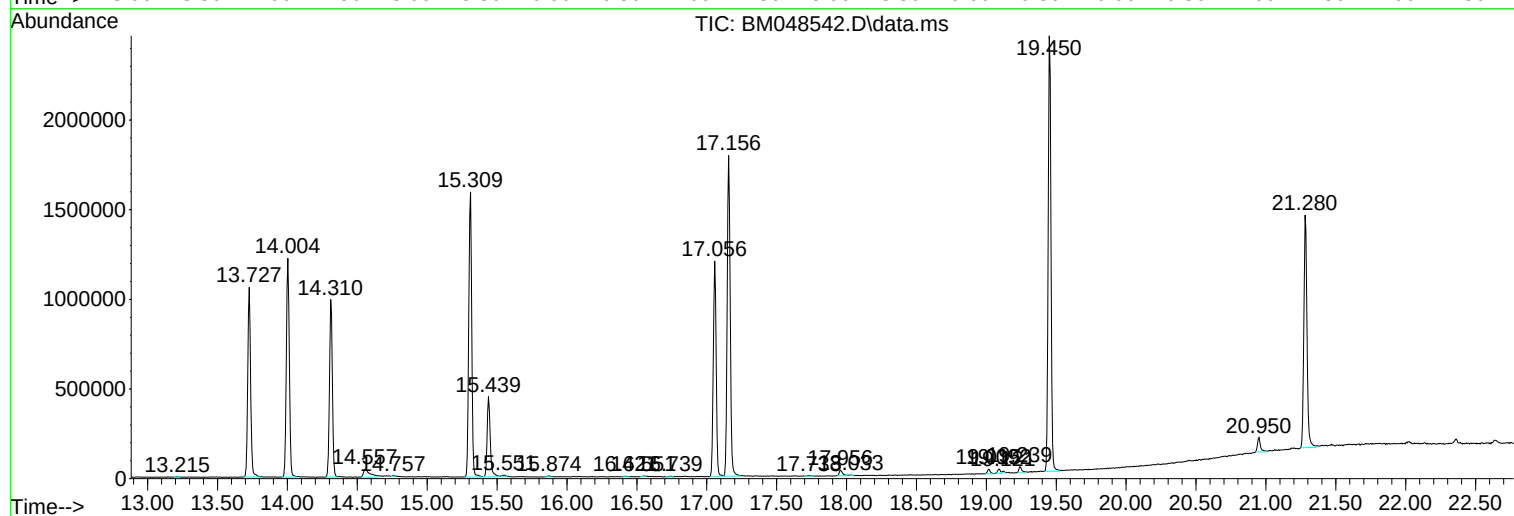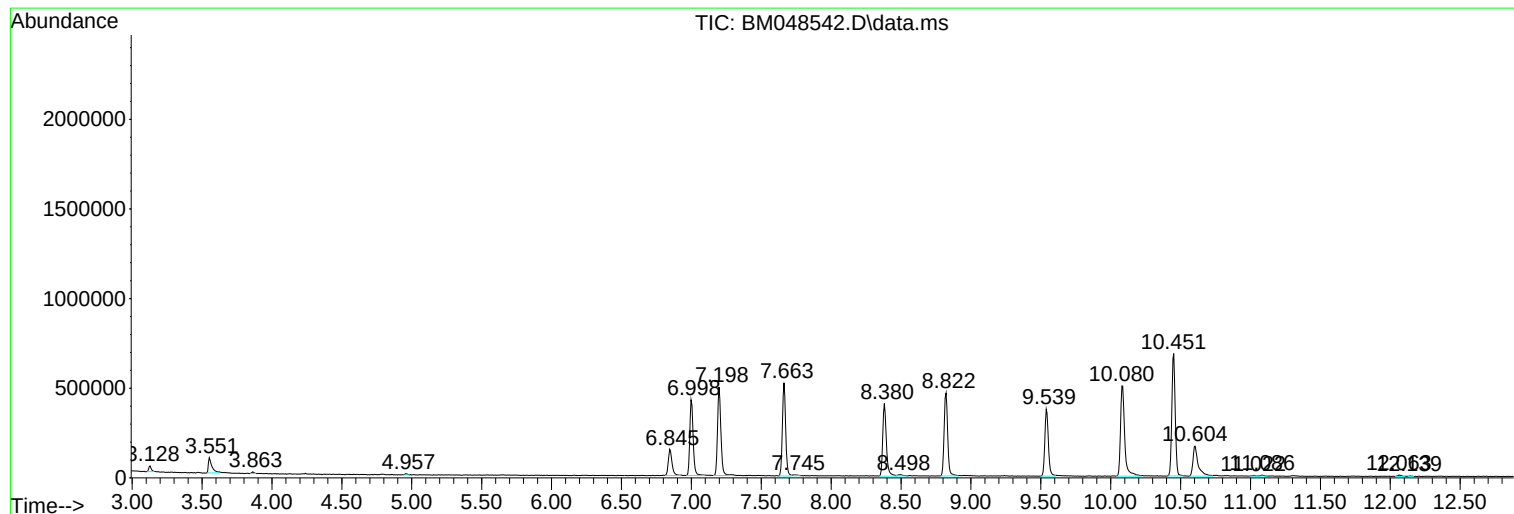

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048542.D
Acq On : 08 Nov 2024 22:51
Operator : RC/JU
Sample : P4621-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048542.D
Acq On : 08 Nov 2024 22:51
Operator : RC/JU
Sample : P4621-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH6N7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc