

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048554.D
 Acq On : 09 Nov 2024 07:25
 Operator : RC/JU
 Sample : P4717-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	33	rVB	36892	58061	1.29%	0.143%
2	3.546	92	95	109	rBV	163333	299214	6.67%	0.738%
3	3.864	145	149	153	rVB2	11444	19104	0.43%	0.047%
4	4.370	231	235	244	rVB	43259	60508	1.35%	0.149%
5	4.958	330	335	347	rVB	85696	132136	2.94%	0.326%
6	5.093	354	358	366	rBV4	11227	17627	0.39%	0.043%
7	5.311	391	395	400	rVB6	3263	6531	0.15%	0.016%
8	5.640	448	451	454	rBV5	3373	4656	0.10%	0.011%
9	5.775	469	474	475	rBV5	4018	6086	0.14%	0.015%
10	6.322	565	567	577	rVB6	5164	8131	0.18%	0.020%
11	6.528	599	602	607	rVB6	3751	5767	0.13%	0.014%
12	6.846	646	656	674	rBV	171039	319068	7.11%	0.787%
13	6.999	676	682	695	rBV	540955	865420	19.28%	2.134%
14	7.199	709	716	725	rBV	625600	1008330	22.46%	2.487%
15	7.663	788	795	804	rVV	657000	1055783	23.52%	2.604%
16	8.281	895	900	906	rVB8	5412	10035	0.22%	0.025%
17	8.381	910	917	931	rBV	472811	835949	18.62%	2.062%
18	8.816	984	991	1002	rBV	590758	1015876	22.63%	2.506%
19	9.540	1106	1114	1124	rBV	506615	875434	19.50%	2.159%
20	10.081	1198	1206	1223	rBV	733419	1341201	29.88%	3.308%
21	10.446	1254	1268	1276	rBV	895707	1502226	33.47%	3.705%
22	10.593	1286	1293	1313	rBV	454690	951397	21.20%	2.347%
23	11.287	1403	1411	1422	rBV4	16619	48415	1.08%	0.119%
24	11.728	1482	1486	1492	rVB7	2534	4923	0.11%	0.012%
25	12.057	1536	1542	1548	rBV5	8724	20306	0.45%	0.050%
26	13.728	1819	1826	1842	rBV	1308287	1951840	43.48%	4.814%
27	14.004	1864	1873	1881	rBV	1505775	2268673	50.54%	5.595%
28	14.310	1919	1925	1934	rBV	1296816	1883732	41.97%	4.646%
29	14.557	1961	1967	1981	rBV2	52936	154310	3.44%	0.381%
30	14.757	1999	2001	2006	rVB5	5944	6828	0.15%	0.017%
31	15.304	2088	2094	2105	rBV	1960458	2963680	66.03%	7.310%
32	15.439	2110	2117	2128	rBV	371113	553493	12.33%	1.365%
33	15.545	2132	2135	2143	rVB5	9642	17060	0.38%	0.042%
34	15.869	2183	2190	2197	rBV6	10273	22630	0.50%	0.056%
35	16.004	2208	2213	2217	rBV7	3870	6328	0.14%	0.016%
36	16.098	2225	2229	2233	rVB7	2330	4707	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048554.D
 Acq On : 09 Nov 2024 07:25
 Operator : RC/JU
 Sample : P4717-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAFO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	16.551	2300	2306	2311	rBV6	11123	21603	0.48%	0.053%
38	16.610	2314	2316	2322	rVB7	5223	6530	0.15%	0.016%
39	16.851	2350	2357	2362	rBV7	5446	11306	0.25%	0.028%
40	16.933	2367	2371	2374	rBV2	10197	13298	0.30%	0.033%
41	17.057	2385	2392	2401	rBV	1545234	2196250	48.93%	5.417%
42	17.157	2402	2409	2421	rVV	2235827	3314186	73.84%	8.174%
43	17.263	2424	2427	2434	rVB8	10837	18330	0.41%	0.045%
44	17.351	2436	2442	2444	rBV5	3794	6332	0.14%	0.016%
45	17.727	2504	2506	2511	rVB6	4248	6593	0.15%	0.016%
46	17.957	2541	2545	2552	rBV6	16631	23956	0.53%	0.059%
47	18.298	2600	2603	2607	rBV5	9104	11099	0.25%	0.027%
48	18.457	2625	2630	2633	rBV5	13872	23459	0.52%	0.058%
49	18.651	2661	2663	2667	rBV4	4719	5199	0.12%	0.013%
50	19.016	2721	2725	2730	rBV2	33368	49521	1.10%	0.122%
51	19.086	2733	2737	2742	rBV	37624	55819	1.24%	0.138%
52	19.451	2793	2799	2812	rBV	3127000	4227858	94.19%	10.428%
53	20.951	3050	3054	3062	rVB	180971	247597	5.52%	0.611%
54	21.280	3105	3110	3123	rBV2	1705106	2533690	56.45%	6.249%
55	23.992	3563	3571	3588	rVB	1796460	4488563	100.00%	11.071%
56	24.192	3597	3605	3617	rVB	1209619	2978601	66.36%	7.346%




Sum of corrected areas: 40545255

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048554.D
Acq On : 09 Nov 2024 07:25
Operator : RC/JU
Sample : P4717-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

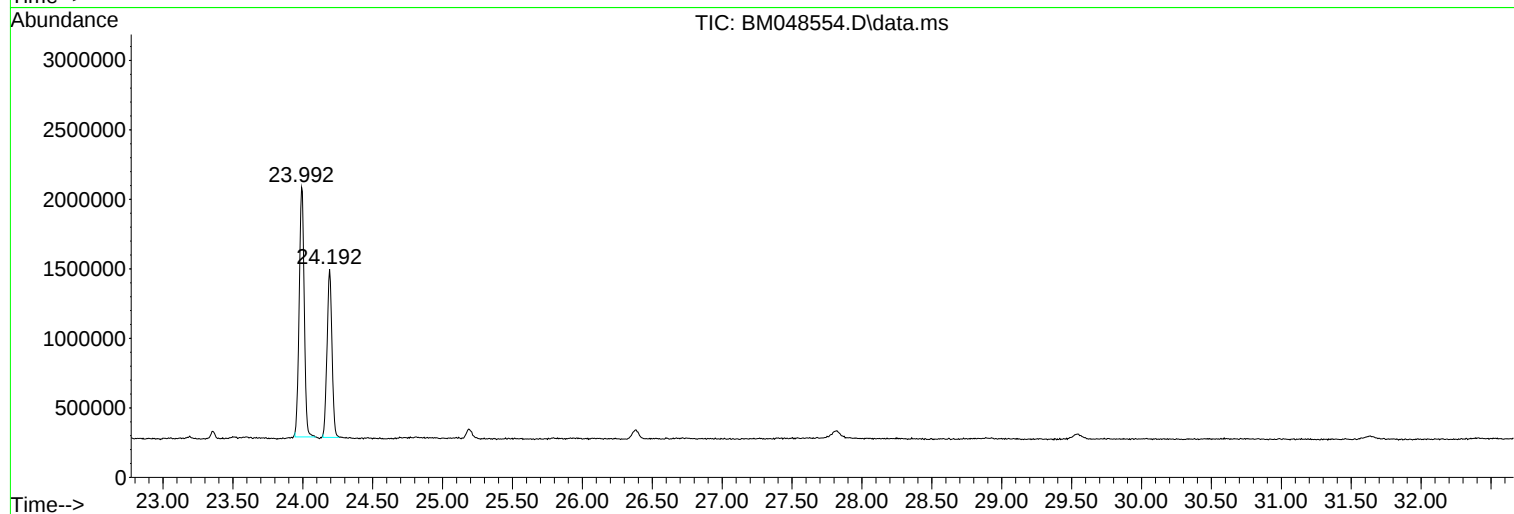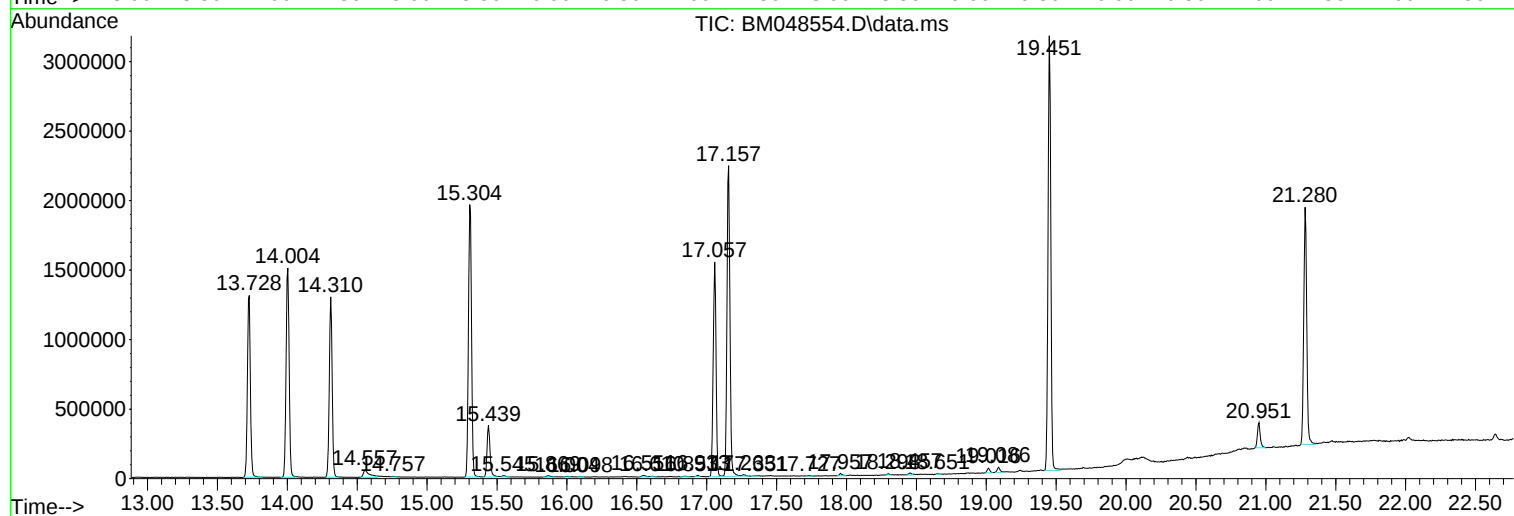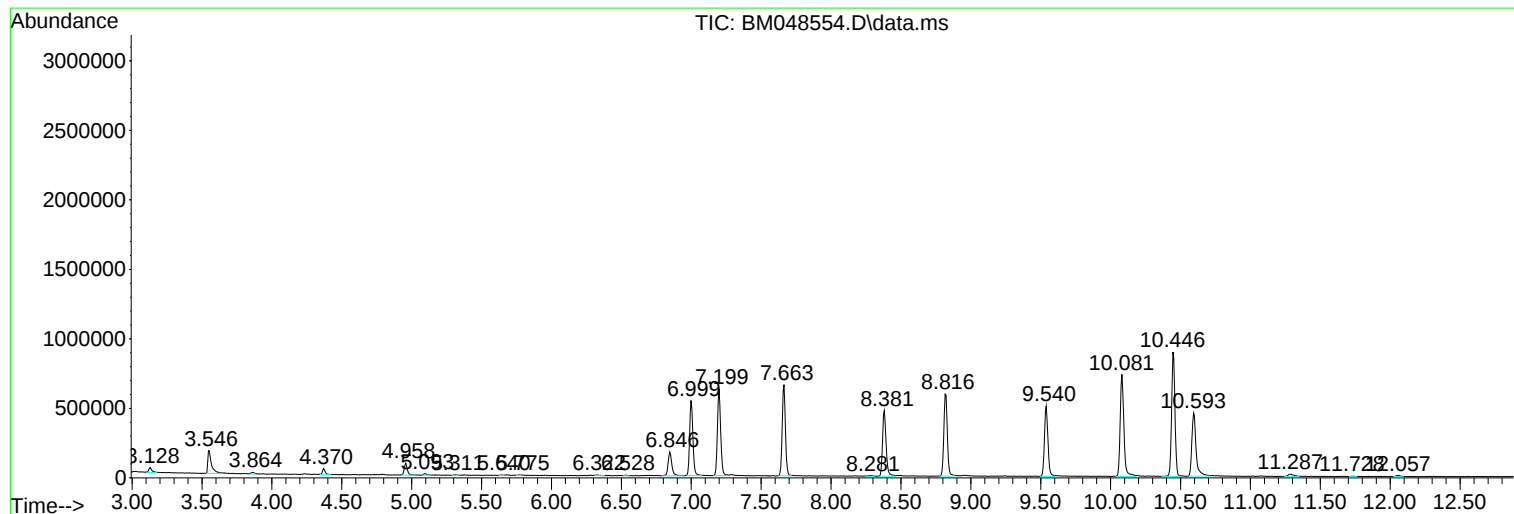

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048554.D
Acq On : 09 Nov 2024 07:25
Operator : RC/JU
Sample : P4717-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048554.D
Acq On : 09 Nov 2024 07:25
Operator : RC/JU
Sample : P4717-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc